
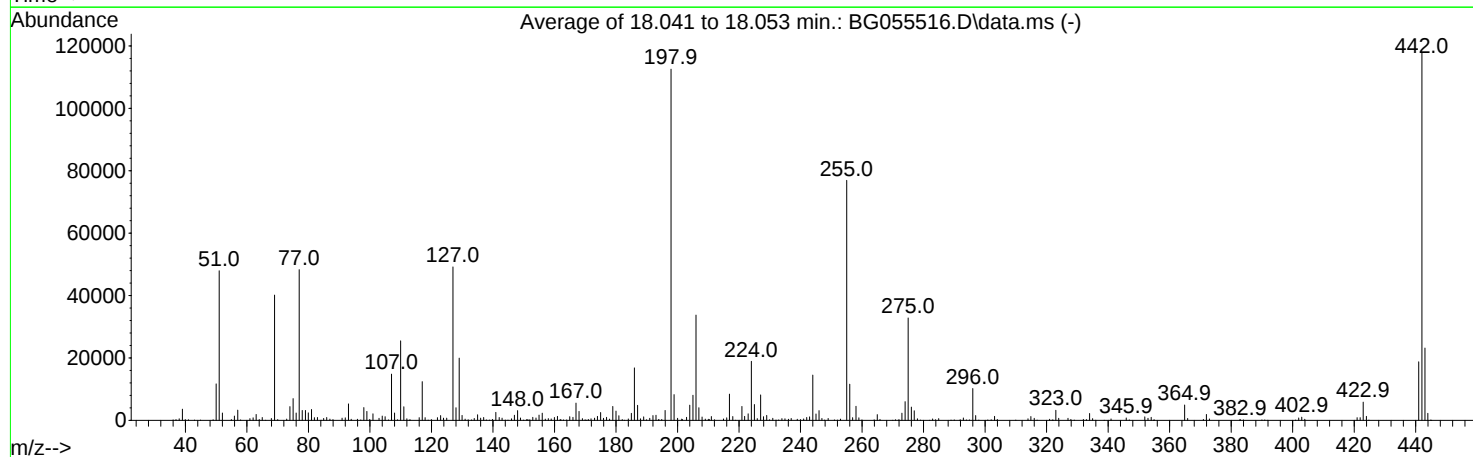


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110922\
Data File : BG055516.D
Acq On : 9 Nov 2022 9:32
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG110922.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Nov 10 03:39:46 2022

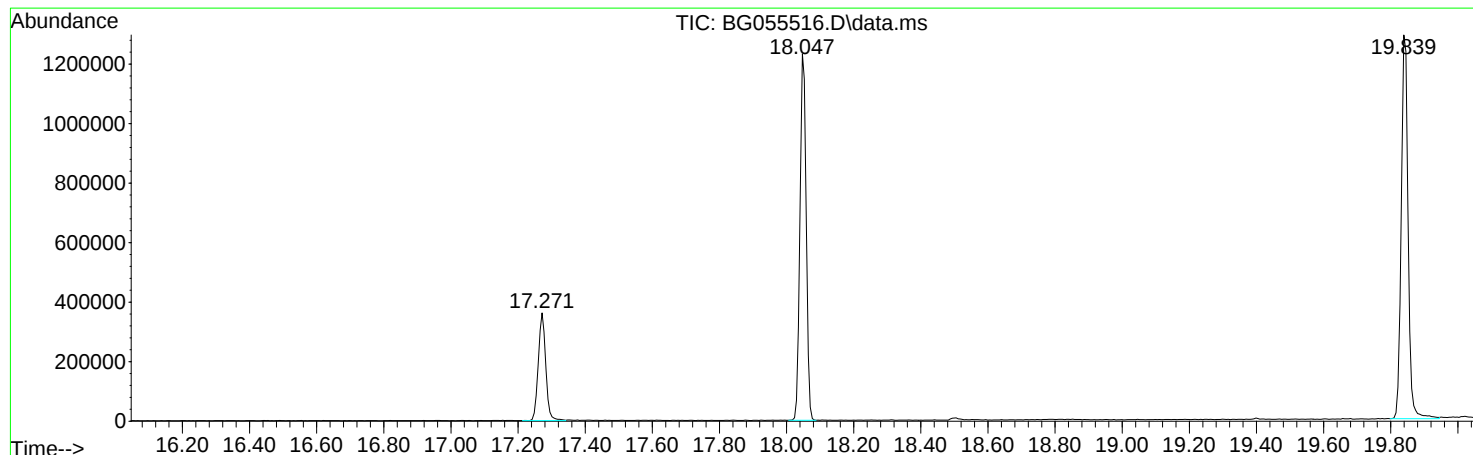




AutoFind: Scans 2511, 2512, 2513; Background Corrected with Scan 2505

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.6	47955	PASS
68	69	0.00	2	1.5	595	PASS
69	198	0.00	100	35.7	40141	PASS
70	69	0.00	2	0.5	218	PASS
127	198	10	80	43.7	49168	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	112565	PASS
199	198	5	9	7.3	8233	PASS
275	198	10	60	29.1	32805	PASS
365	198	1	100	4.4	4924	PASS
441	198	0.01	100	16.7	18764	PASS
442	442	50	100	100.0	117941	PASS
443	442	15	24	19.6	23164	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110922\
Data File : BG055516.D
Acq On : 9 Nov 2022 9:32
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Nov 09 16:21:45 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG110922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 09 16:20:23 2022
Response via : Initial Calibration

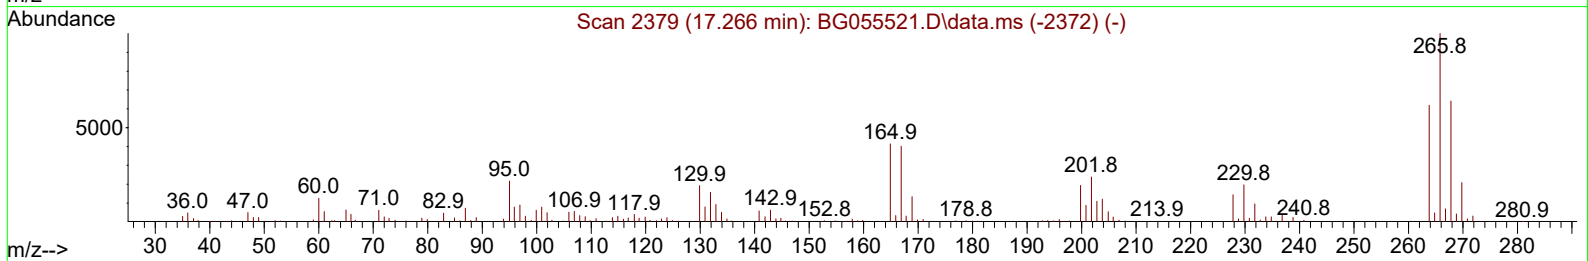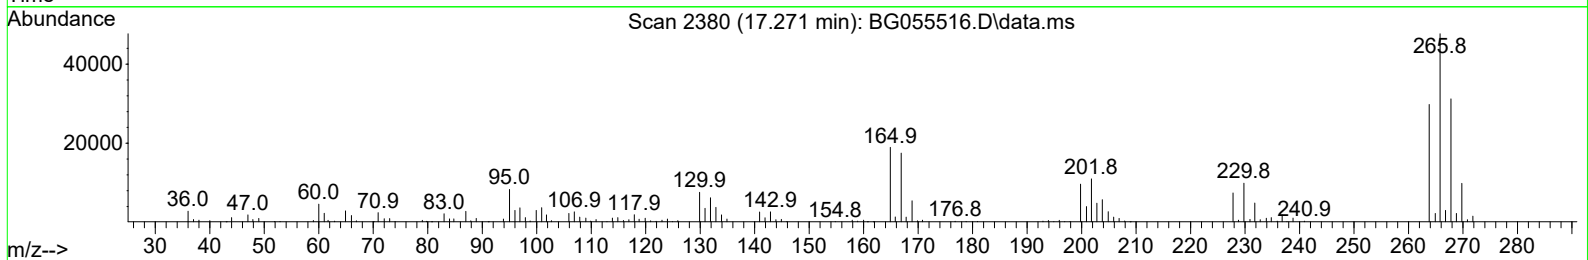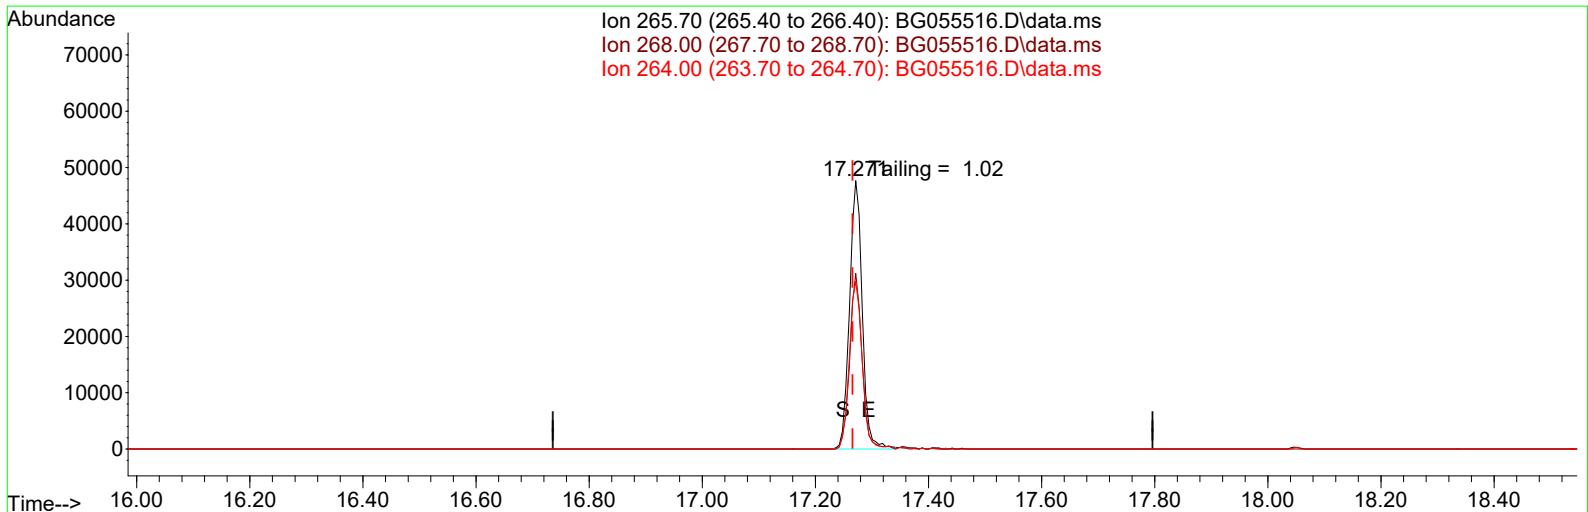

TIC: BG055516.D\data.ms

(70) Pentachlorophenol (C)

17.271min (+ 0.005) 17349.30 ng




response 74816

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.20	65.44
264.00	61.90	62.48
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110922\
Data File : BG055516.D
Acq On : 9 Nov 2022 9:32
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Nov 09 16:21:45 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG110922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 09 16:20:23 2022
Response via : Initial Calibration

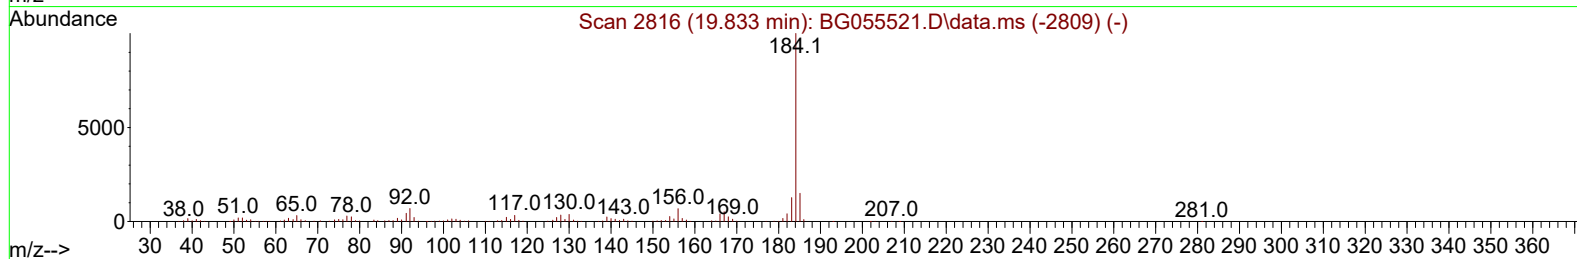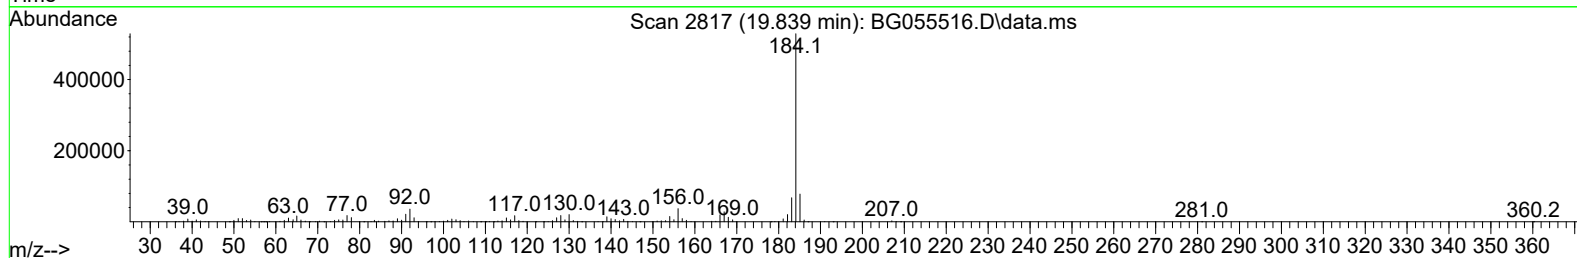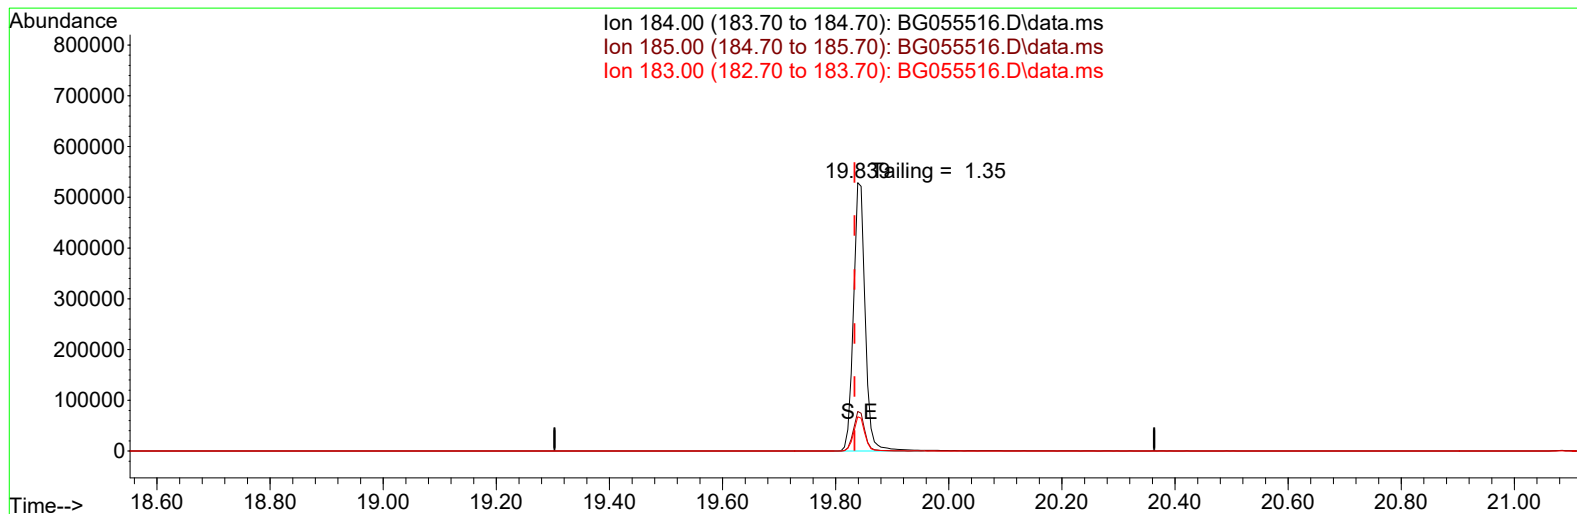

TIC: BG055516.D\data.ms

(77) Benzidine

19.839min (+ 0.006) 85400.85 ng

response 762445

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.00	14.75
183.00	12.70	12.78
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/9/2022	BNA_G	<u>BG055516.D</u>
Compound Name	Response	Retention Time
DDT	233393	21.085
DDD	13616	20.626
DDE	357	20.127
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
13973	247366	5.65

Instrument :
BNA_G
ClientSampleId :
DFTPP