

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG111015\
 Data File : BG019558.D
 Acq On : 10 Nov 2015 23:25
 Operator : UM/NP
 Sample : G4308-14
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 D9KR2

Quant Time: Nov 13 08:38:48 2015
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG102815.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Nov 13 08:28:14 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.17	152	44036	20.00	ng/ul	0.00
18) Naphthalene-d8	11.00	136	188471	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.81	164	154446	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.55	188	430594	20.00	ng/ul	0.00
78) Chrysene-d12	21.83	240	547039	20.00	ng/ul	0.00
86) Perylene-d12	25.18	264	527180	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.47	96	1029	1.12	ng/uL	-0.01
5) Phenol-d5	7.32	99	26130	6.46	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.49	67	80305	31.34	ng/ul	0.00
9) 2-Chlorophenol-d4	7.70	132	55826	22.12	ng/ul	0.00
13) 4-Methylphenol-d8	8.87	113	49620	15.41	ng/ul	0.00
19) Nitrobenzene-d5	9.35	128	40184	29.01	ng/ul	0.00
22) 2-Nitrophenol-d4	10.07	143	46665	28.38	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.62	165	89786	25.17	ng/ul	0.00
29) 4-Chloroaniline-d4	11.13	131	5261	1.46	ng/ul	0.00
44) Dimethylphthalate-d6	14.20	166	381622	29.97	ng/ul	0.00
47) Acenaphthylene-d8	14.50	160	401613	28.48	ng/ul	0.00
52) 4-Nitrophenol-d4	14.99	143	11912	5.89	ng/ul	0.00
58) Fluorene-d10	15.79	176	326465	27.71	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.90	200	68244	24.49	ng/ul	0.00
71) Anthracene-d10	17.64	188	555151	28.28	ng/ul	0.00
79) Pyrene-d10	19.92	212	659663	27.56	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.94	264	732075	27.67	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
45) Dimethylphthalate	14.25	163	62638	4.81	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG111015\
Data File : BG019558.D
Acq On : 10 Nov 2015 23:25
Operator : UM/NP
Sample : G4308-14
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
D9KR2

Quant Time: Nov 13 08:38:48 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG102815.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Nov 13 08:28:14 2015
Response via : Initial Calibration

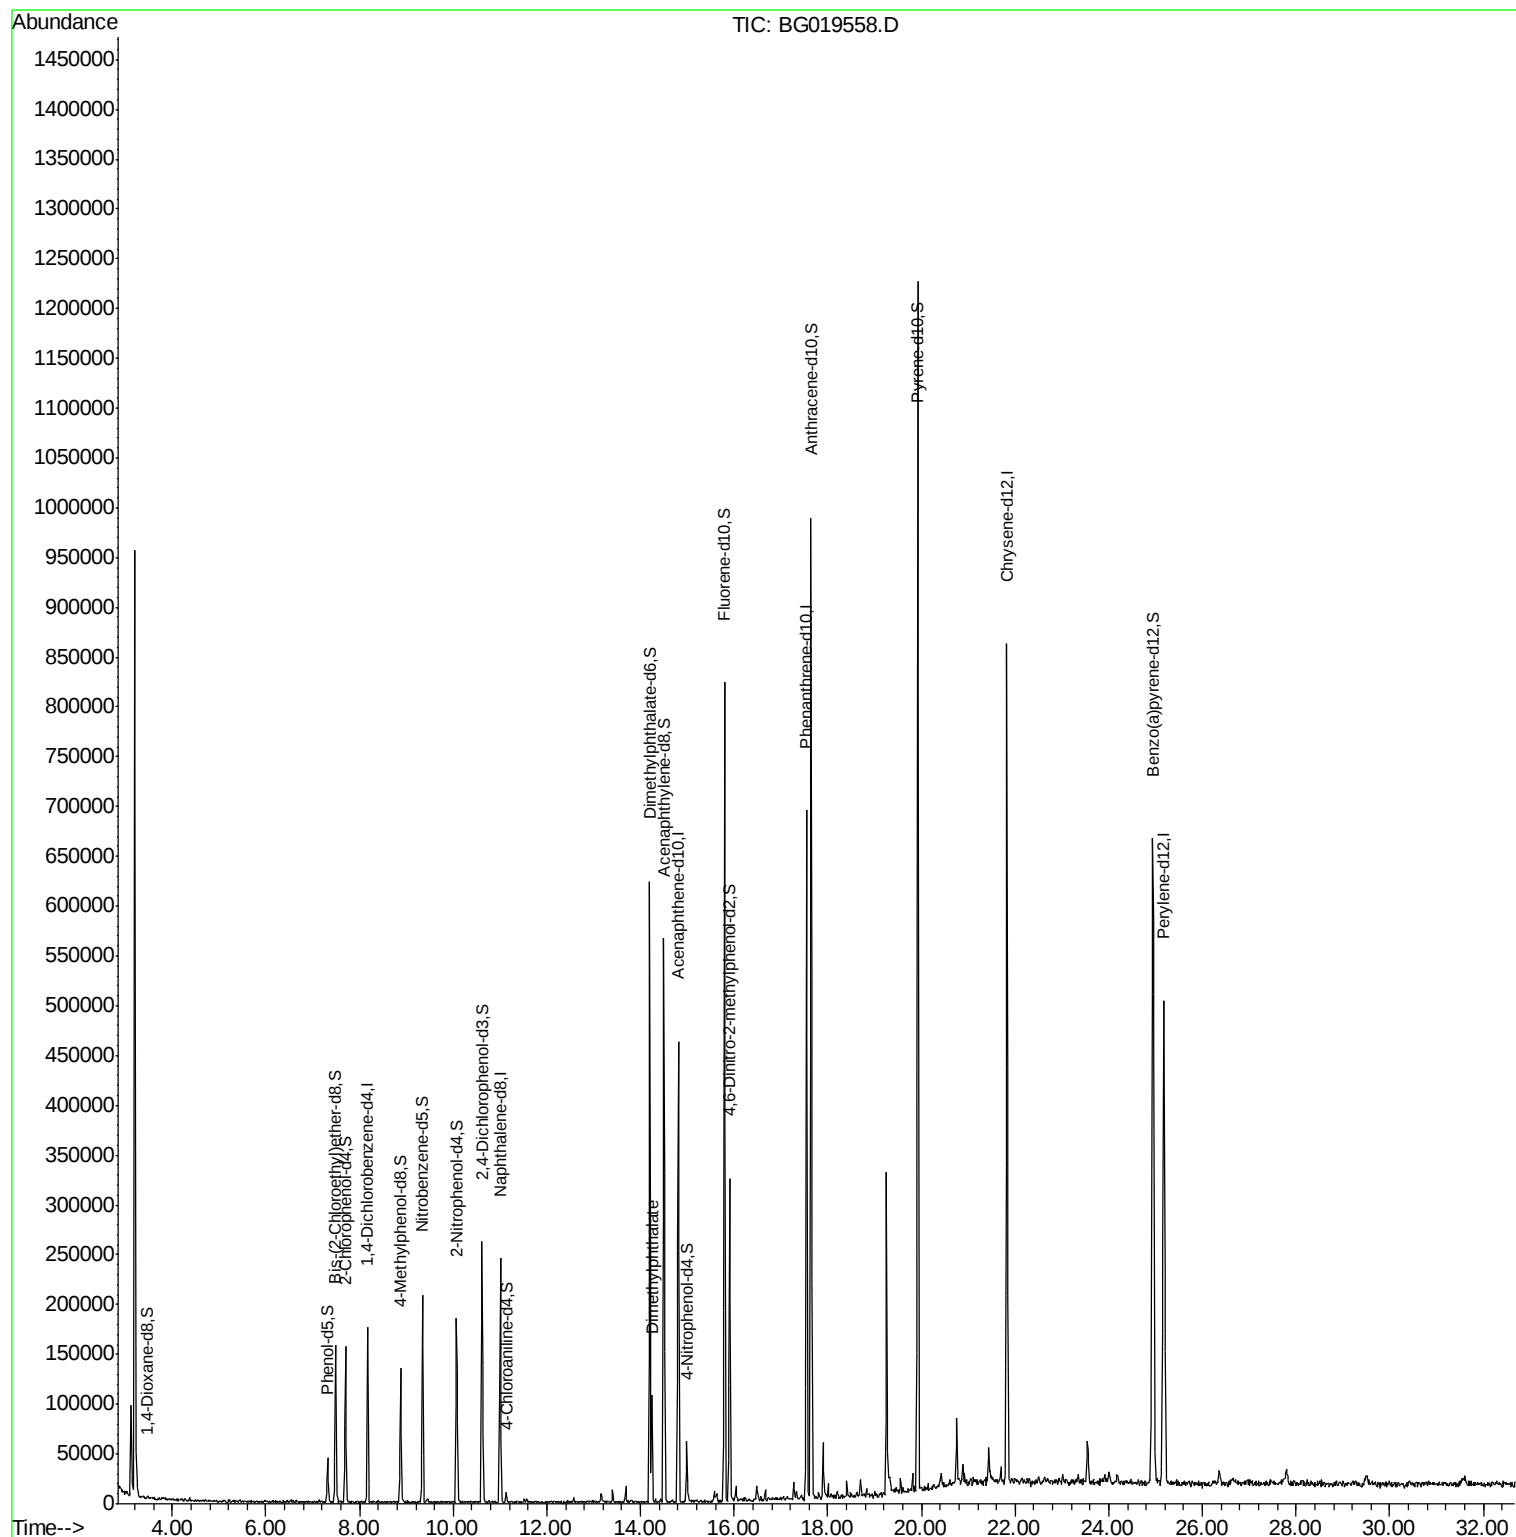

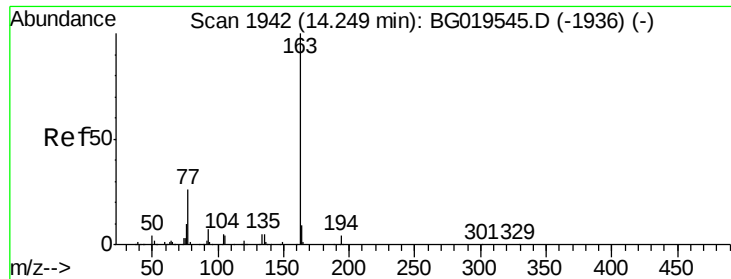

#45

Dimethylphthalate

Concen: 4.81 ng/ul

RT: 14.25 min Scan# 1942

Delta R.T. 0.00 min

Lab File: BG019558.D

Acq: 10 Nov 2015 23:25

Instrument :

BNA_G

ClientSampleId :

D9KR2


Tgt Ion:163 Resp: 62638

Ion Ratio Lower Upper

163 100

194 4.4 4.3 6.5

164 10.0 7.5 11.3

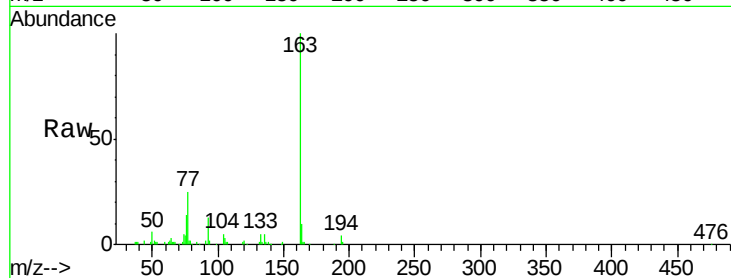

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

