

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG111015\
 Data File : BG019567.D
 Acq On : 11 Nov 2015 13:02
 Operator : UM/NP
 Sample : G4308-20
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 D9KS4

Quant Time: Nov 13 08:39:49 2015
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG102815.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Nov 13 08:28:14 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.17	152	30712	20.00	ng/ul	0.00
18) Naphthalene-d8	11.00	136	132947	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.81	164	108331	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.55	188	309304	20.00	ng/ul	0.00
78) Chrysene-d12	21.83	240	379990	20.00	ng/ul	0.00
86) Perylene-d12	25.18	264	365734	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.48	96	1242	1.94	ng/uL	0.00
5) Phenol-d5	7.32	99	30835	10.94	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.48	67	77179	43.18	ng/ul	0.00
9) 2-Chlorophenol-d4	7.70	132	56390	32.04	ng/ul	0.00
13) 4-Methylphenol-d8	8.88	113	55409	24.67	ng/ul	0.00
19) Nitrobenzene-d5	9.34	128	39288	40.21	ng/ul	0.00
22) 2-Nitrophenol-d4	10.07	143	44782	38.61	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.62	165	91312	36.29	ng/ul	0.00
29) 4-Chloroaniline-d4	11.14	131	5433	2.13	ng/ul	0.00
44) Dimethylphthalate-d6	14.20	166	382292	42.80	ng/ul	0.00
47) Acenaphthylene-d8	14.50	160	399725	40.41	ng/ul	0.00
52) 4-Nitrophenol-d4	14.99	143	12974	9.14	ng/ul	0.00
58) Fluorene-d10	15.79	176	331111	40.07	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.90	200	70177	35.05	ng/ul	0.00
71) Anthracene-d10	17.64	188	564131	40.01	ng/ul	0.00
79) Pyrene-d10	19.92	212	656718	39.49	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.95	264	735943	40.10	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
84) Bis(2-ethylhexyl)phthalate	21.69	149	20574	2.09	ng/ul#	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG111015\
Data File : BG019567.D
Acq On : 11 Nov 2015 13:02
Operator : UM/NP
Sample : G4308-20
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
D9KS4

Quant Time: Nov 13 08:39:49 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG102815.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Nov 13 08:28:14 2015
Response via : Initial Calibration

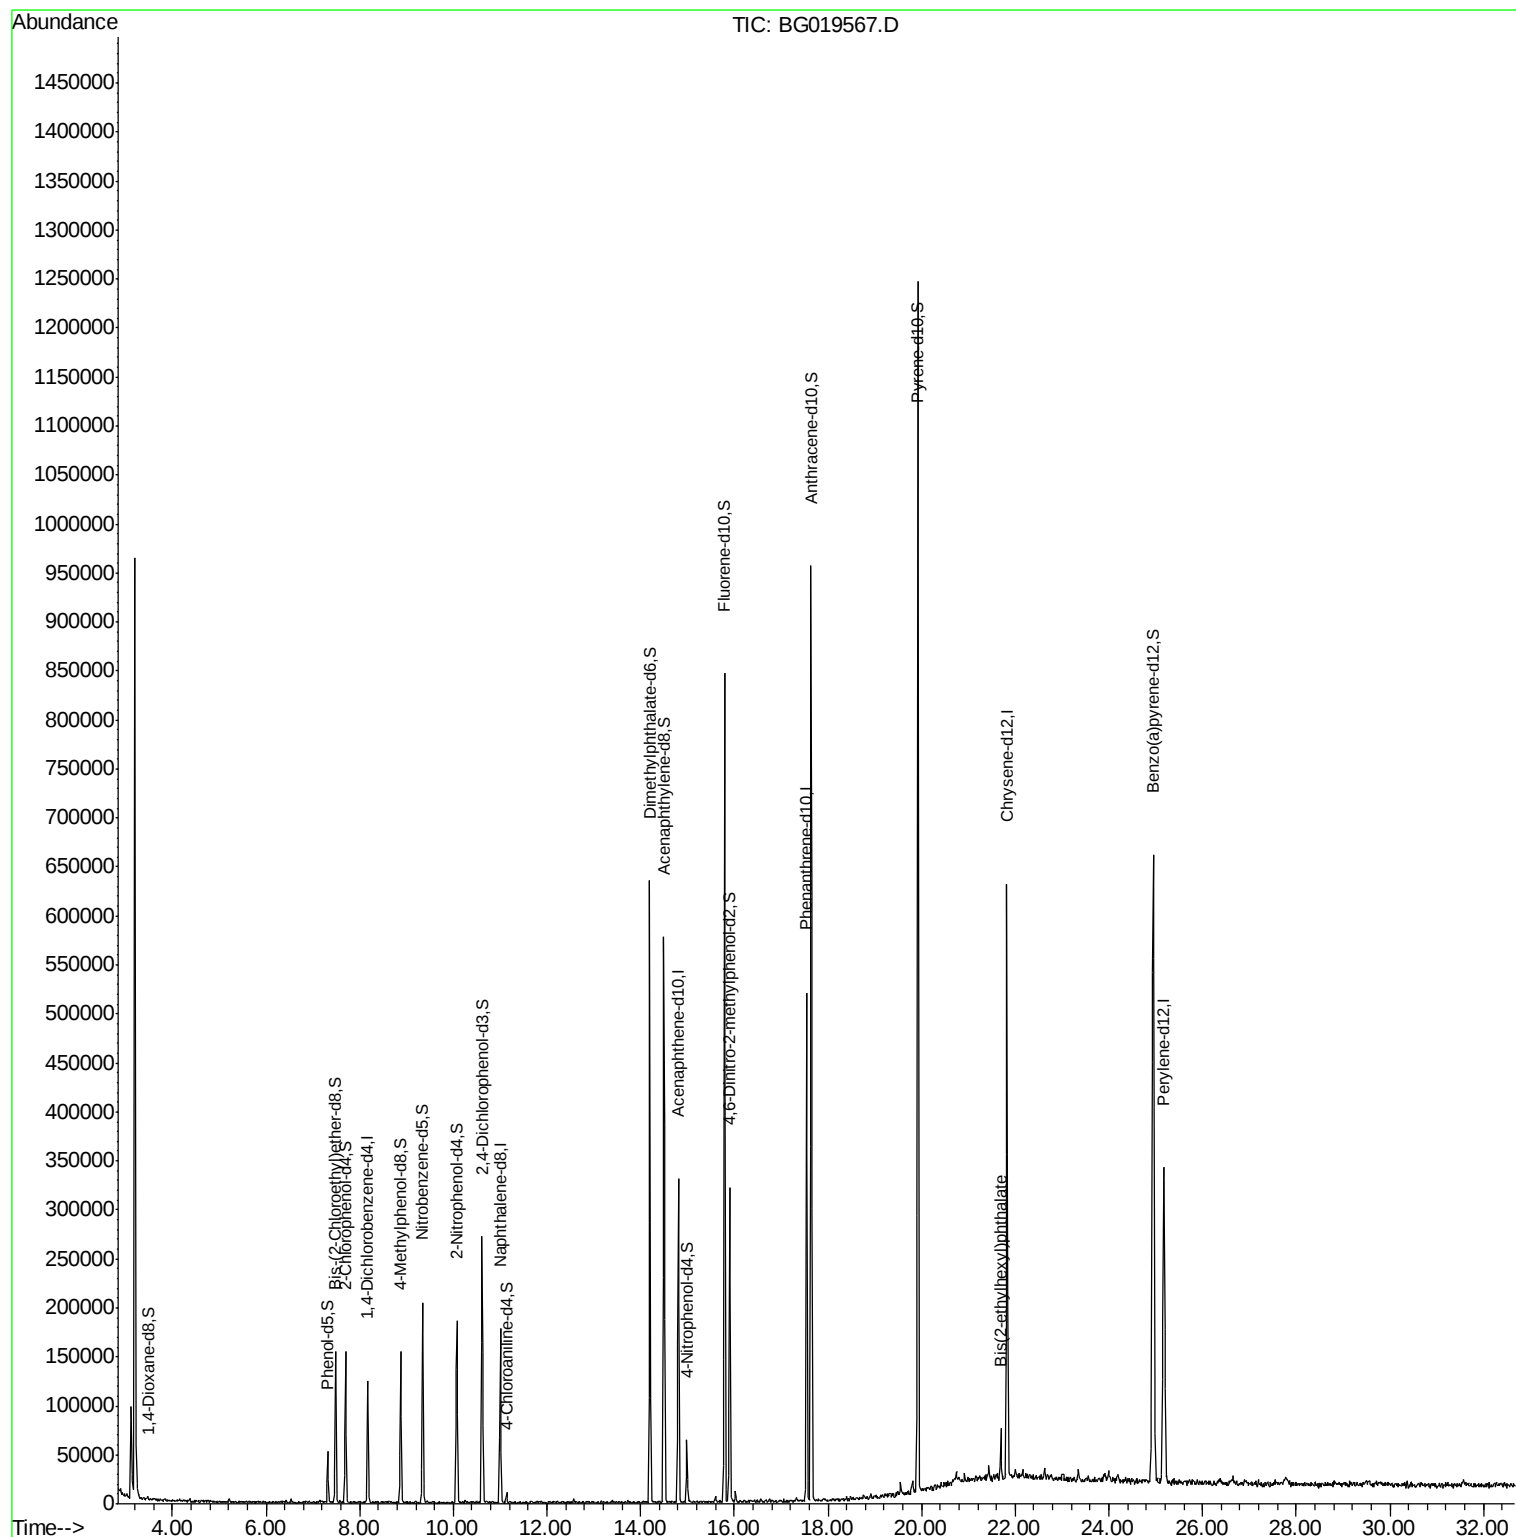

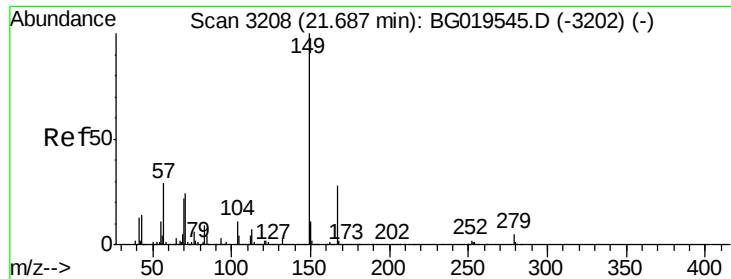

#84

Bis(2-ethylhexyl)phthalate

Concen: 2.09 ng/ul

RT: 21.69 min Scan# 3209

Delta R.T. 0.00 min

Lab File: BG019567.D

Acq: 11 Nov 2015 13:02

Instrument :

BNA_G

ClientSampleId :

D9KS4


Tgt Ion:149 Resp: 20574

Ion Ratio Lower Upper

149 100

167 26.3 23.2 34.8

279 3.4 5.0 7.4#

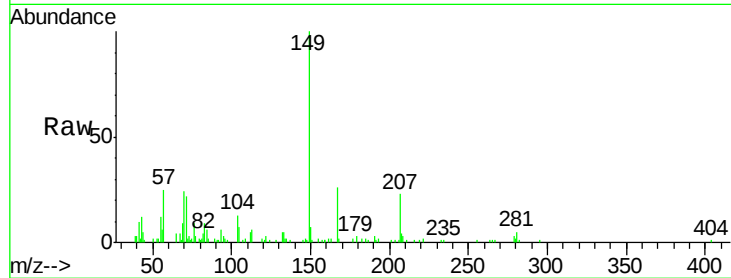

Abundance Ion 149.00 (148.70 to 149.70): E

Ion 167.00 (166.70 to 167.70): E

Ion 279.00 (278.70 to 279.70): E

