

Quantitation Report (QT/LSC Reviewed)

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG111015\
Data File : BG019549.D
Acq On : 10 Nov 2015 17:40
Operator : UM/NP
Sample : G4308-05
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
D9KR4

Quant Time: Nov 13 08:49:56 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG102815.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Nov 13 08:28:14 2015
Response via : Initial Calibration

Manual Integrations
APPROVED

Mmdadoda
11/13/2015 5:21:54 PM

Internal Standards	R.T.	Qlon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.17	152	41437	20.00	ng/ul	0.00
18) Naphthalene-d8	11.00	136	173425	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.81	164	149192	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.55	188	413827	20.00	ng/ul	0.00
78) Chrysene-d12	21.83	240	542161	20.00	ng/ul	0.00
86) Perylene-d12	25.18	264	513767	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.48	96	1195	1.38	ng/uL	0.00
5) Phenol-d5	7.31	99	26950	7.08	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.48	67	75622	31.36	ng/ul	0.00
9) 2-Chlorophenol-d4	7.70	132	56244	23.69	ng/ul	0.00
13) 4-Methylphenol-d8	8.88	113	49583	16.37	ng/ul	0.00
19) Nitrobenzene-d5	9.35	128	37779	29.64	ng/ul	0.00
22) 2-Nitrophenol-d4	10.08	143	45053	29.78	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.62	165	84834	25.85	ng/ul	0.00
29) 4-Chloroaniline-d4	11.13	131	1663m	0.50	ng/ul	0.00
44) Dimethylphthalate-d6	14.20	166	363173	29.52	ng/ul	0.00
47) Acenaphthylene-d8	14.51	160	373521	27.42	ng/ul	0.00
52) 4-Nitrophenol-d4	14.99	143	11155	5.71	ng/ul	0.00
58) Fluorene-d10	15.79	176	307536	27.03	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.90	200	65112	24.31	ng/ul	0.00
71) Anthracene-d10	17.65	188	540457	28.65	ng/ul	0.00
79) Pyrene-d10	19.92	212	657303	27.70	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.95	264	747154	28.98	ng/ul	0.00

U.M.
11/23/15

Target Compounds	Qvalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_G\DATA\BG111015\
 Data File : BG019549.D
 Acq On : 10 Nov 2015 17:40
 Operator : UM/NP
 Sample : G4308-05
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 D9KR4

Quant Time: Nov 13 08:37:52 2015
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG102815.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Nov 13 08:28:14 2015
 Response via : Initial Calibration

Manual Integrations
 APPROVED

Mmdadoda
 11/13/2015 5:21:54 PM

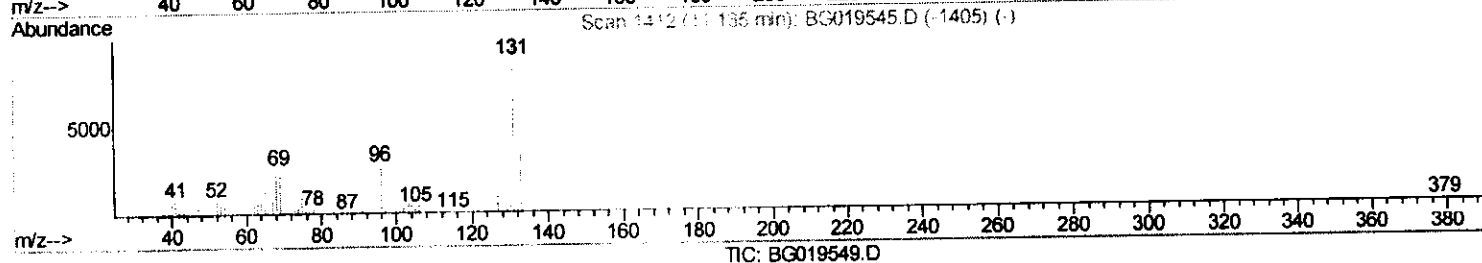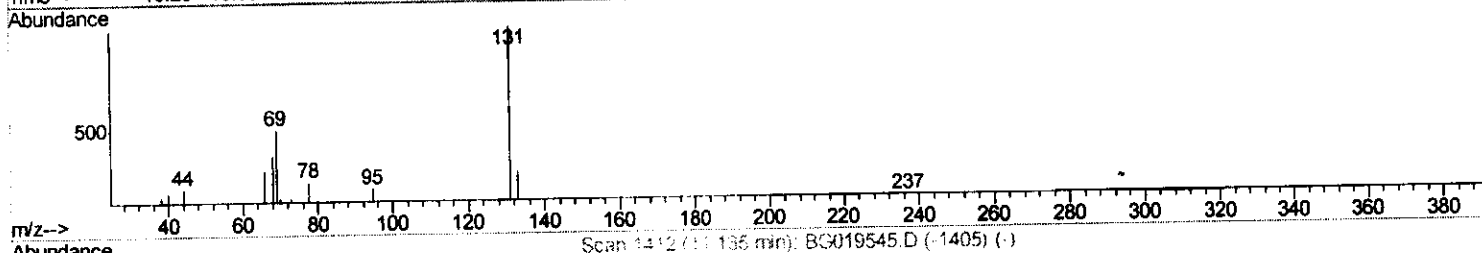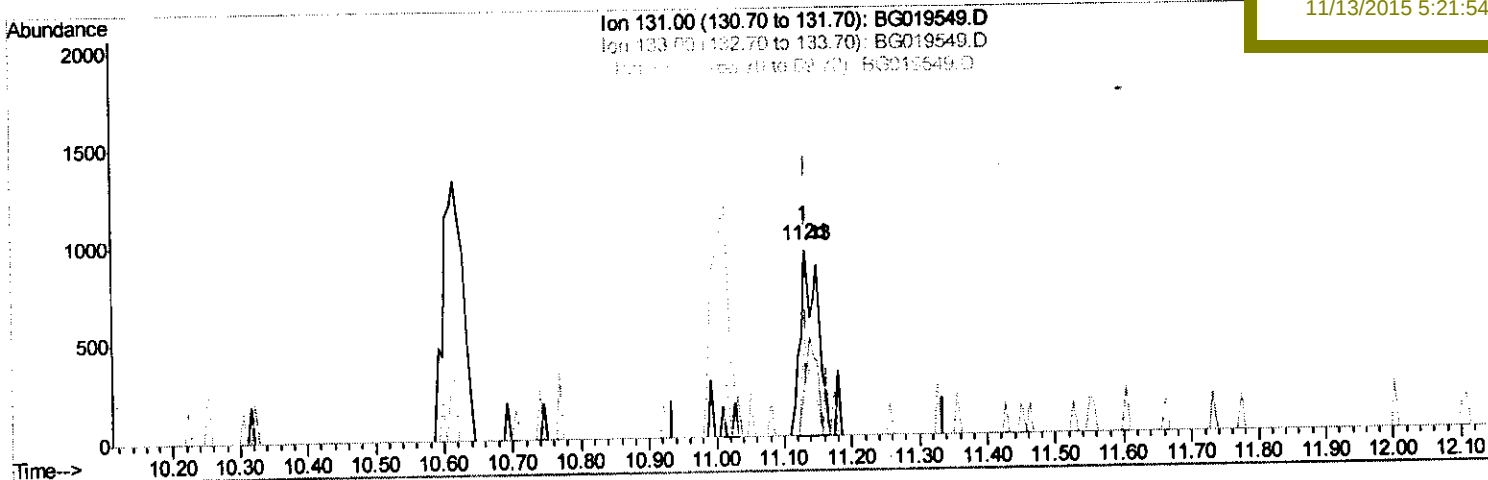

(29) 4-Chloroaniline-d4 (S)

11.133min (-0.002) 0.50ng/ul m > U.M.
 11/23/15

response 1663

Ion	Exp%	Act%
131.00	100	100
133.00	29.30	30.34
69.00	23.70	50.88#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_G\DATA\BG111015\
Data File : BG019549.D
Acq On : 10 Nov 2015 17:40
Operator : UM/NP
Sample : G4308-05
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
D9KR4

Quant Time: Nov 13 08:37:52 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG102815.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Nov 13 08:28:14 2015
Response via : Initial Calibration

Manual Integrations
APPROVED

Mmdadoda
11/13/2015 5:21:54 PM

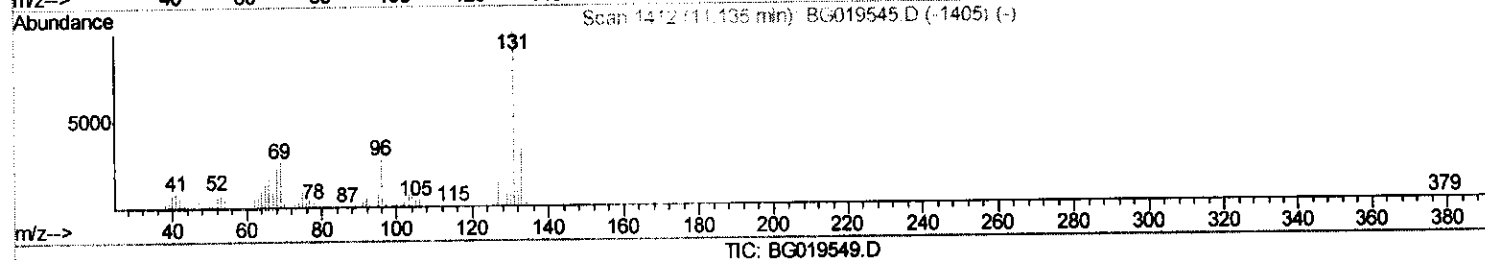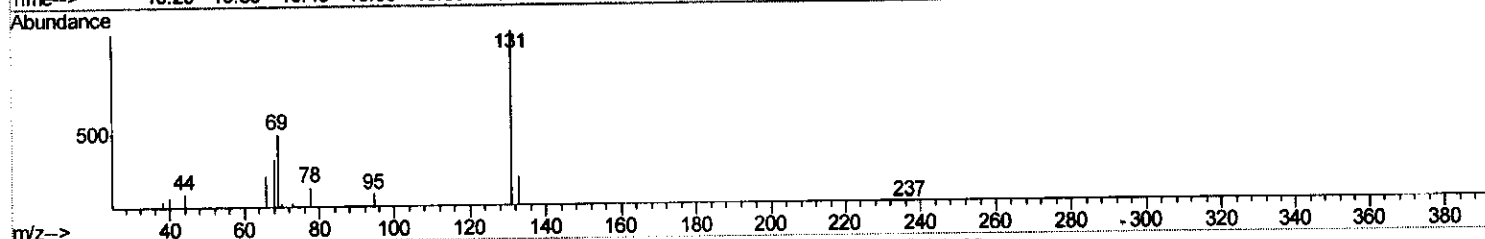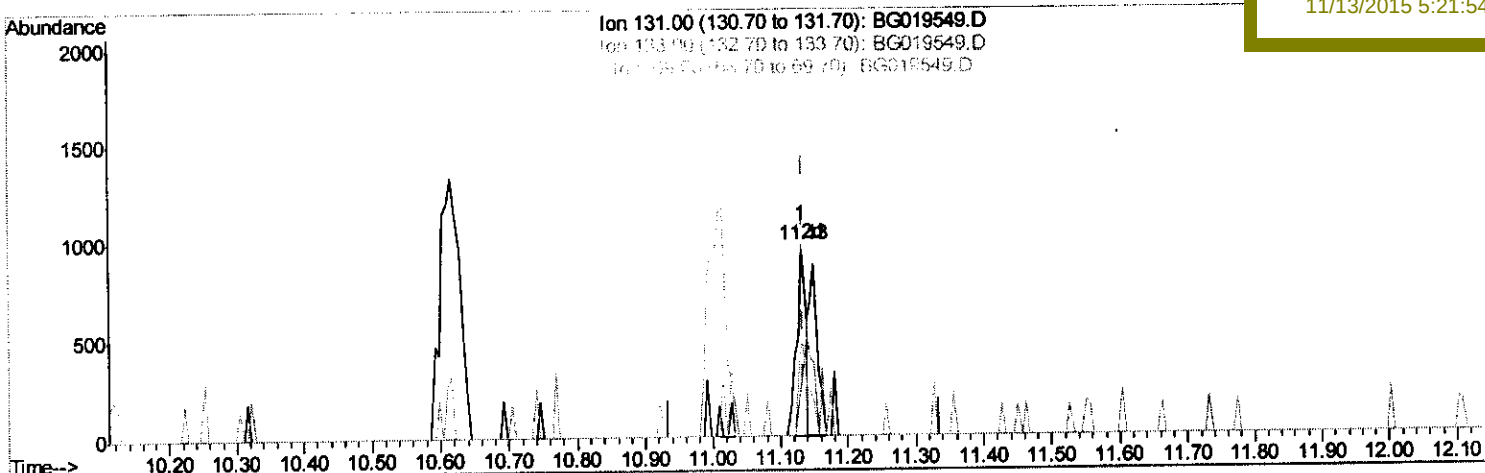

(29) 4-Chloroaniline-d4 (S)

11.133min (-0.002) 0.28ng/ul

response 926

Ion	Exp%	Act%
131.00	100	100
133.00	29.30	30.34
69.00	23.70	50.88#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG111015\
Data File : BG019549.D
Acq On : 10 Nov 2015 17:40
Operator : UM/NP
Sample : G4308-05
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
D9KR4

Quant Time: Nov 13 08:49:56 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG102815.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Nov 13 08:28:14 2015
Response via : Initial Calibration

Manual Integrations
APPROVED

Mmdadoda
11/13/2015 5:21:54 PM

