

Quantitation Report (QT/LSC Reviewed)

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG111015\
 Data File : BG019551.D
 Acq On : 10 Nov 2015 18:57
 Operator : UM/NP
 Sample : G4308-07
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 D9KR6

Quant Time: Nov 13 08:54:44 2015
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG102815.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Nov 13 08:28:14 2015
 Response via : Initial Calibration

Manual Integrations
 APPROVED

Mmdadoda
 11/13/2015 5:21:55 PM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.18	152	38711	20.00	ng/ul	0.00
18) Naphthalene-d8	11.00	136	168110	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.80	164	142727	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.55	188	404675	20.00	ng/ul	0.00
78) Chrysene-d12	21.82	240	523901	20.00	ng/ul	0.00
86) Perylene-d12	25.17	264	504914	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.47	96	1170	1.45	ng/uL	0.00
5) Phenol-d5	7.32	99	21880	6.16	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.48	67	65528	29.09	ng/ul	0.00
9) 2-Chlorophenol-d4	7.70	132	48367	21.80	ng/ul	0.00
13) 4-Methylphenol-d8	8.88	113	41813	14.77	ng/ul	0.00
19) Nitrobenzene-d5	9.34	128	33074	26.77	ng/ul	0.00
22) 2-Nitrophenol-d4	10.07	143	39102	26.66	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.62	165	77016	24.21	ng/ul	0.00
29) 4-Chloroaniline-d4	11.13	131	1395m	0.43	ng/ul	0.00
44) Dimethylphthalate-d6	14.20	166	344547	29.28	ng/ul	0.00
47) Acenaphthylene-d8	14.50	160	350583	26.90	ng/ul	0.00
52) 4-Nitrophenol-d4	14.98	143	10215	5.46	ng/ul	0.00
58) Fluorene-d10	15.79	176	292152	26.84	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.90	200	59846	22.85	ng/ul	0.00
71) Anthracene-d10	17.65	188	511386	27.72	ng/ul	0.00
79) Pyrene-d10	19.92	212	608518	26.54	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.94	264	689840	27.23	ng/ul	0.00

U.M.
 11/23/15

Target Compounds					Qvalue
45) Dimethylphthalate	14.24	163	55257	4.59 ng/ul#	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_G\DATA\BG111015\
 Data File : BG019551.D
 Acq On : 10 Nov 2015 18:57
 Operator : UM/NP
 Sample : G4308-07
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 D9KR6

Quant Time: Nov 13 08:38:04 2015
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG102815.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Nov 13 08:28:14 2015
 Response via : Initial Calibration

Manual Integrations
 APPROVED

Mmdadoda
 11/13/2015 5:21:55 PM

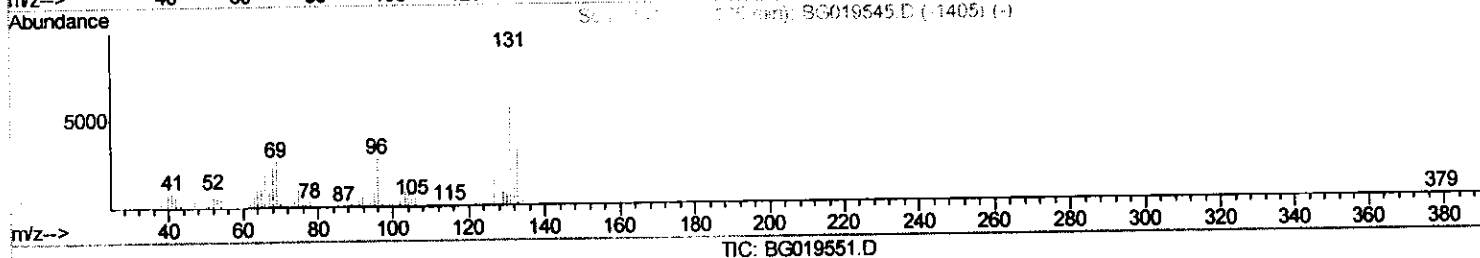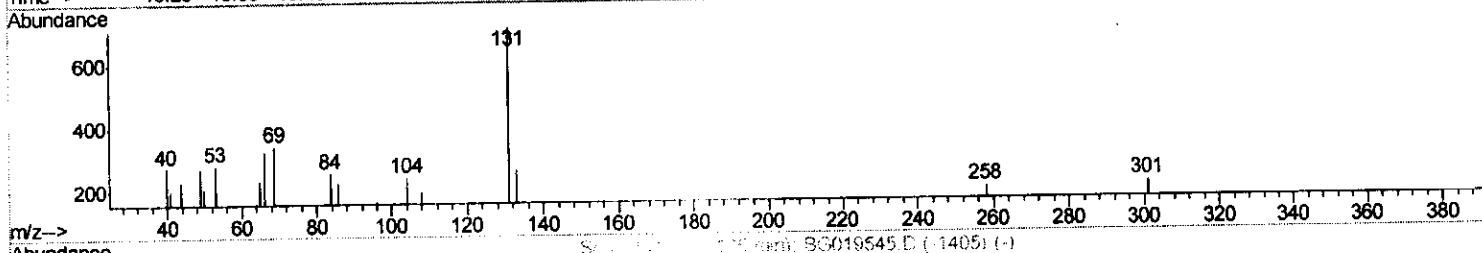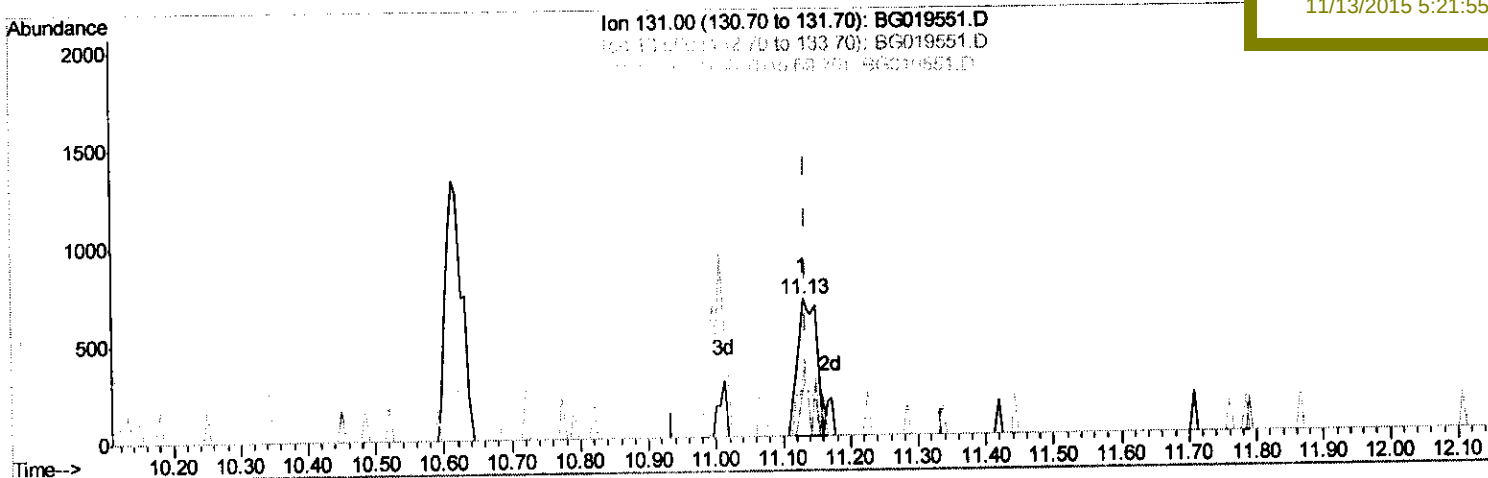

(29) 4-Chloroaniline-d4 (S)

11.131min (-0.004) 0.43ng/ul m

response 1395

Ion Exp% Act%

131.00 100 100

133.00 29.30 36.67#

69.00 23.70 48.24#

0.00 0.00 0.00

U.M.
 11/23/15

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_G\DATA\BG111015\
 Data File : BG019551.D
 Acq On : 10 Nov 2015 18:57
 Operator : UM/NP
 Sample : G4308-07
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 D9KR6

Quant Time: Nov 13 08:38:04 2015
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG102815.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Nov 13 08:28:14 2015
 Response via : Initial Calibration

Manual Integrations
 APPROVED

Mmdadoda
 11/13/2015 5:21:55 PM

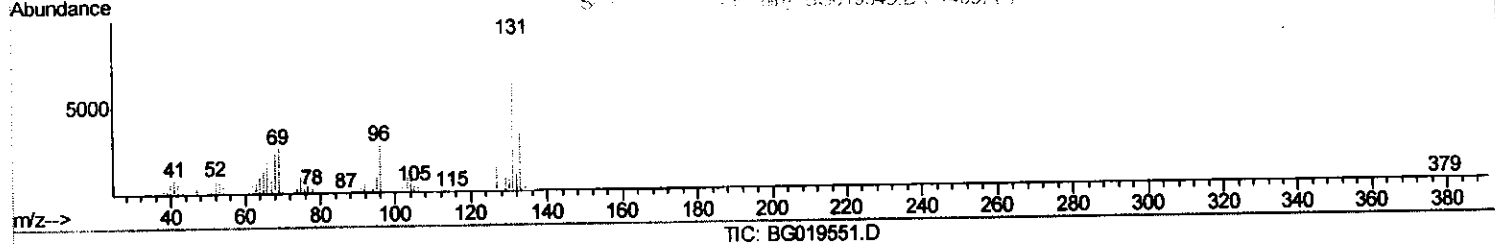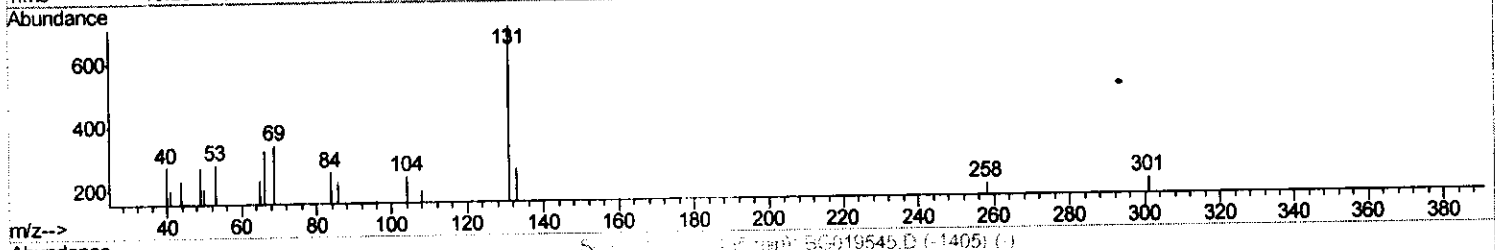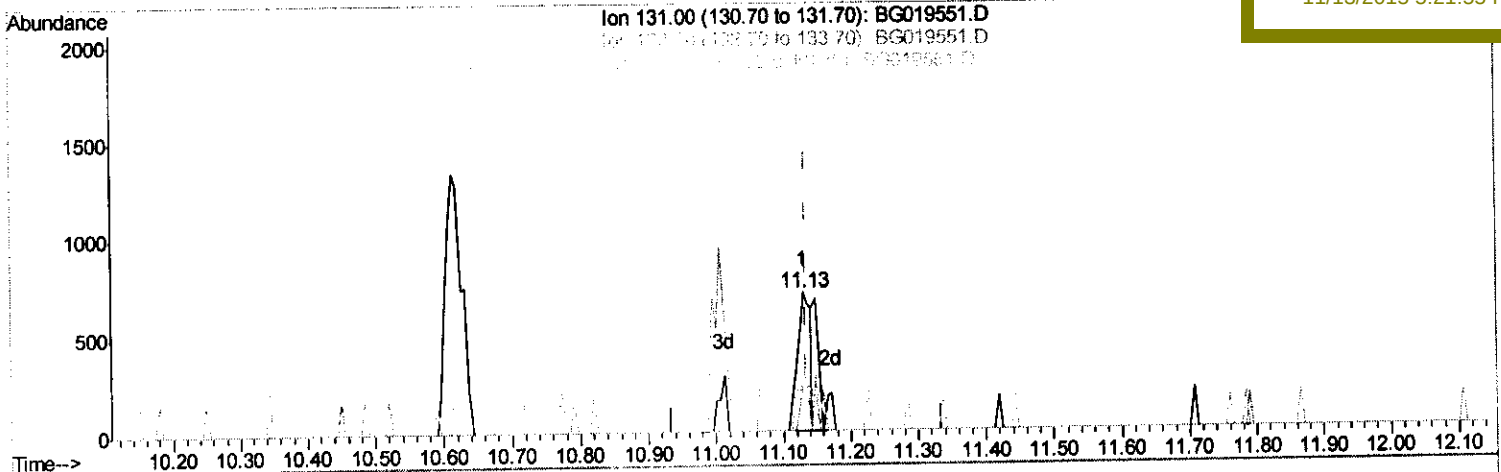

(29) 4-Chloroaniline-d4 (S)
 11.131min (-0.004) 0.32ng/ul
 response 1042

Ion	Exp%	Act%
131.00	100	100
133.00	29.30	36.67#
69.00	23.70	48.24#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG111015\
Data File : BG019551.D
Acq On : 10 Nov 2015 18:57
Operator : UM/NP
Sample : G4308-07
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
D9KR6

Quant Time: Nov 13 08:54:44 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG102815.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Nov 13 08:28:14 2015
Response via : Initial Calibration

Manual Integrations
APPROVED

Mmdadoda
11/13/2015 5:21:55 PM

