

Data Path : Z:\HPCHEM1\BNA G\DATA\BG111015\
 Data File : BG019562.D
 Acq On : 11 Nov 2015 1:59
 Operator : UM/NP
 Sample : G4308-18
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 D9KR9

Quant Time: Nov 13 08:39:22 2015
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG102815.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Nov 13 08:28:14 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.17	152	41169	20.00	ng/ul	0.00
18) Naphthalene-d8	11.01	136	169594	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.81	164	136927	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.54	188	397950	20.00	ng/ul	0.00
78) Chrysene-d12	21.83	240	524409	20.00	ng/ul	0.00
86) Perylene-d12	25.18	264	494638	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.48	96	875	1.02	ng/uL	0.00
5) Phenol-d5	7.32	99	17343	4.59	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.49	67	56059	23.40	ng/ul	0.00
9) 2-Chlorophenol-d4	7.70	132	39738	16.84	ng/ul	0.00
13) 4-Methylphenol-d8	8.88	113	34405	11.43	ng/ul	0.00
19) Nitrobenzene-d5	9.35	128	28545	22.90	ng/ul	0.00
22) 2-Nitrophenol-d4	10.07	143	32731	22.12	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.62	165	62521	19.48	ng/ul	0.00
29) 4-Chloroaniline-d4	11.14	131	3169	0.98	ng/ul	0.00
44) Dimethylphthalate-d6	14.20	166	277831	24.61	ng/ul	0.00
47) Acenaphthylene-d8	14.50	160	280087	22.40	ng/ul	0.00
52) 4-Nitrophenol-d4	14.99	143	8066	4.50	ng/ul	0.00
58) Fluorene-d10	15.79	176	230497	22.07	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.91	200	49895	19.37	ng/ul	0.00
71) Anthracene-d10	17.64	188	401801	22.15	ng/ul	0.00
79) Pyrene-d10	19.92	212	499247	21.75	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.94	264	551310	22.21	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
45) Dimethylphthalate	14.25	163	77841	6.74	ng/ul#	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG111015\
Data File : BG019562.D
Acq On : 11 Nov 2015 1:59
Operator : UM/NP
Sample : G4308-18
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
D9KR9

Quant Time: Nov 13 08:39:22 2015
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG102815.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Nov 13 08:28:14 2015
Response via : Initial Calibration

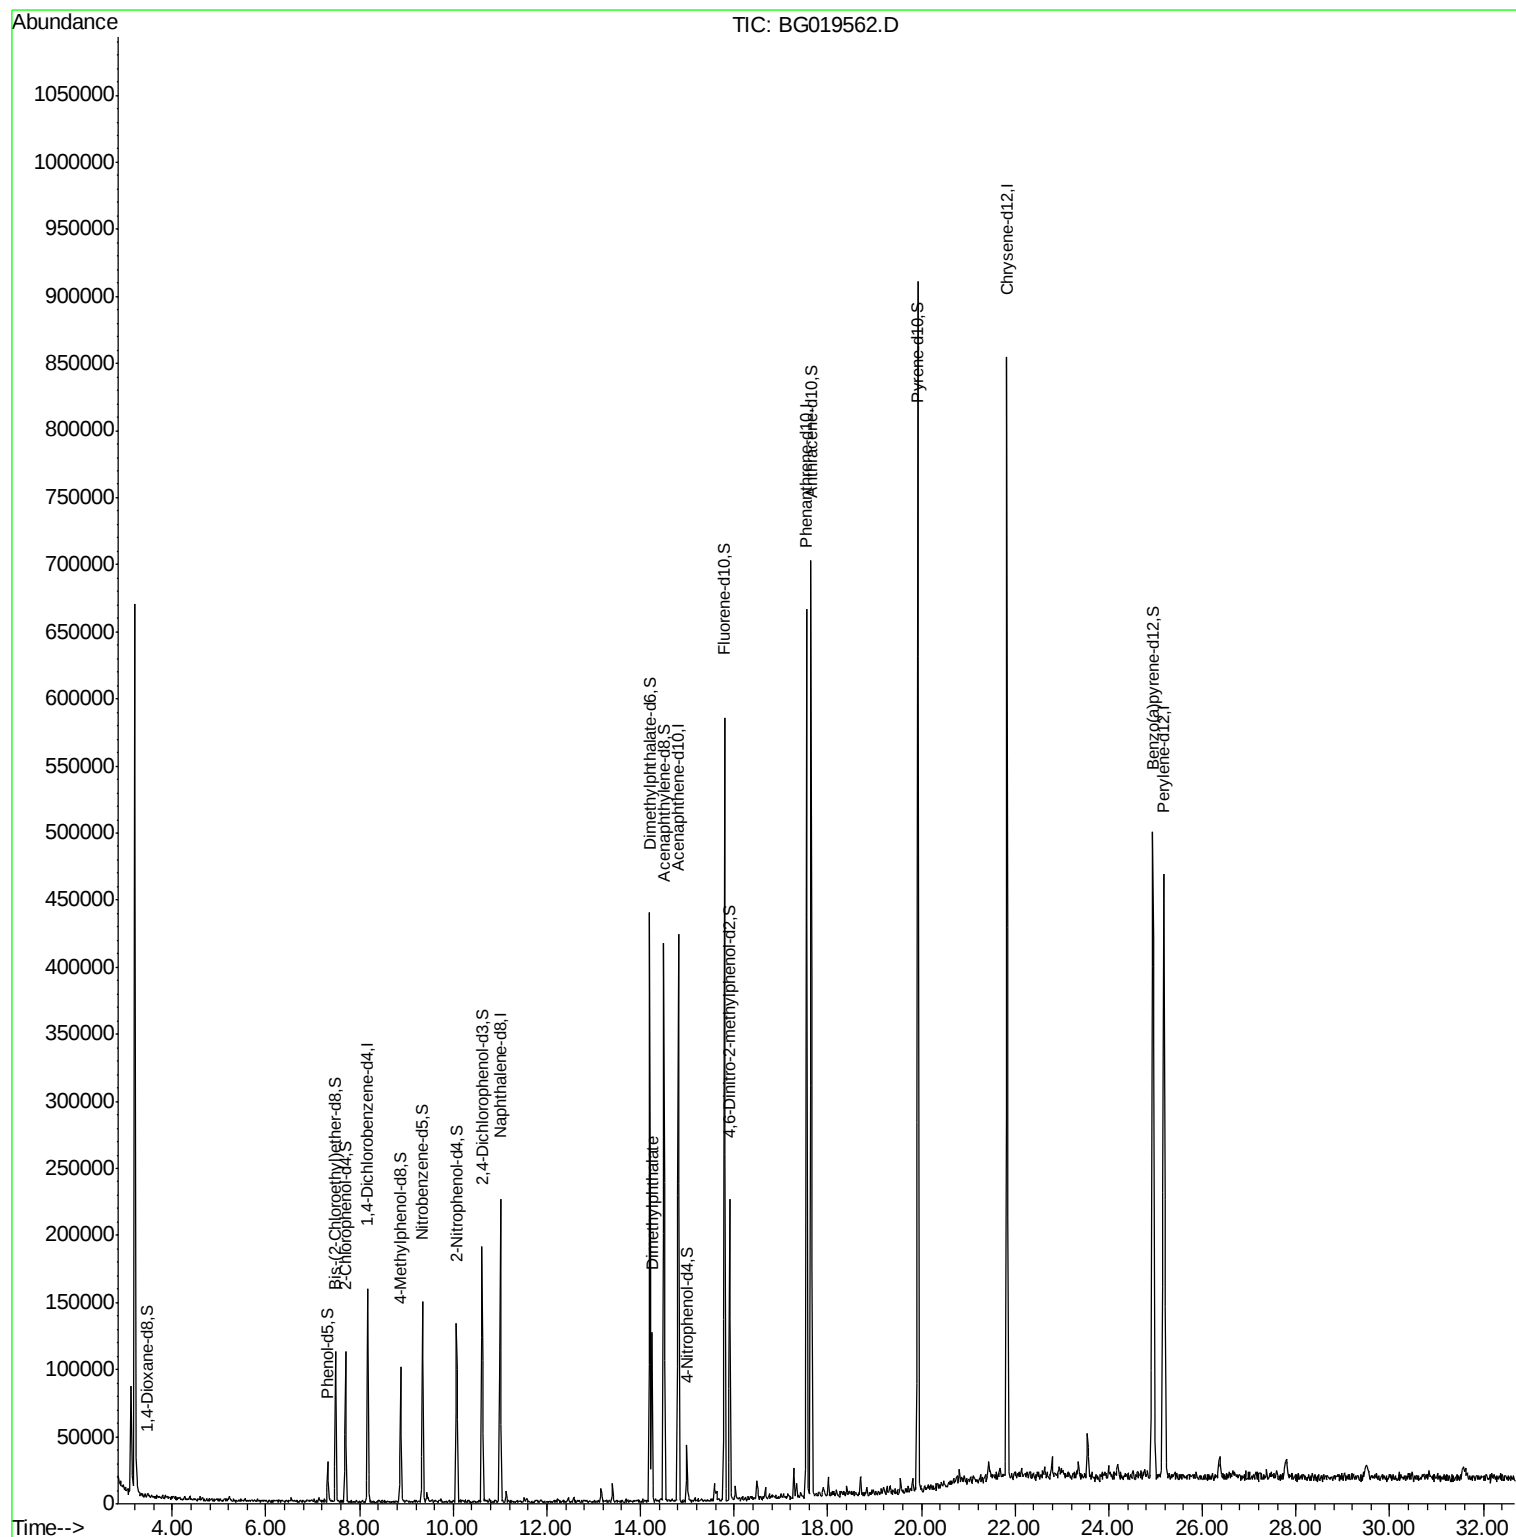

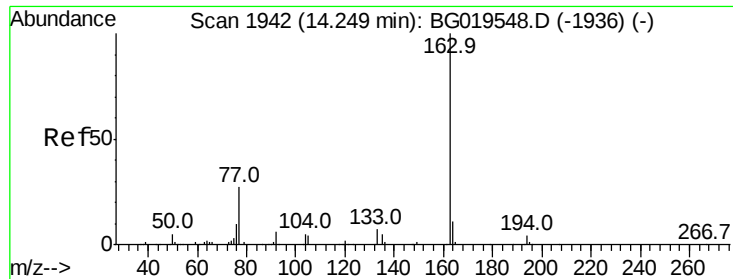

#45

Dimethylphthalate

Concen: 6.74 ng/ul

RT: 14.25 min Scan# 1942

Delta R.T. -0.00 min

Lab File: BG019562.D

Acq: 11 Nov 2015 1:59

Instrument :

BNA_G

ClientSampleId :

D9KR9


Tot Ion:163 Resp: 77841

Ion Ratio Lower Upper

163 100

194 4.3 4.3 6.5#

164 9.9 7.5 11.3

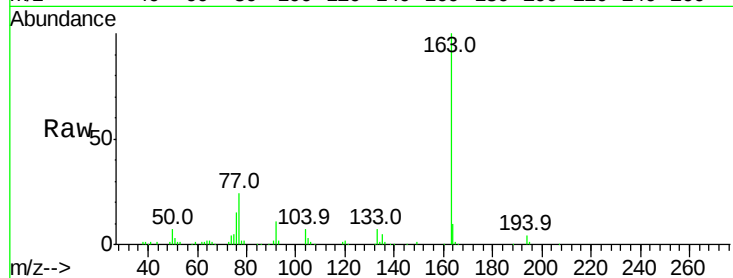

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

