



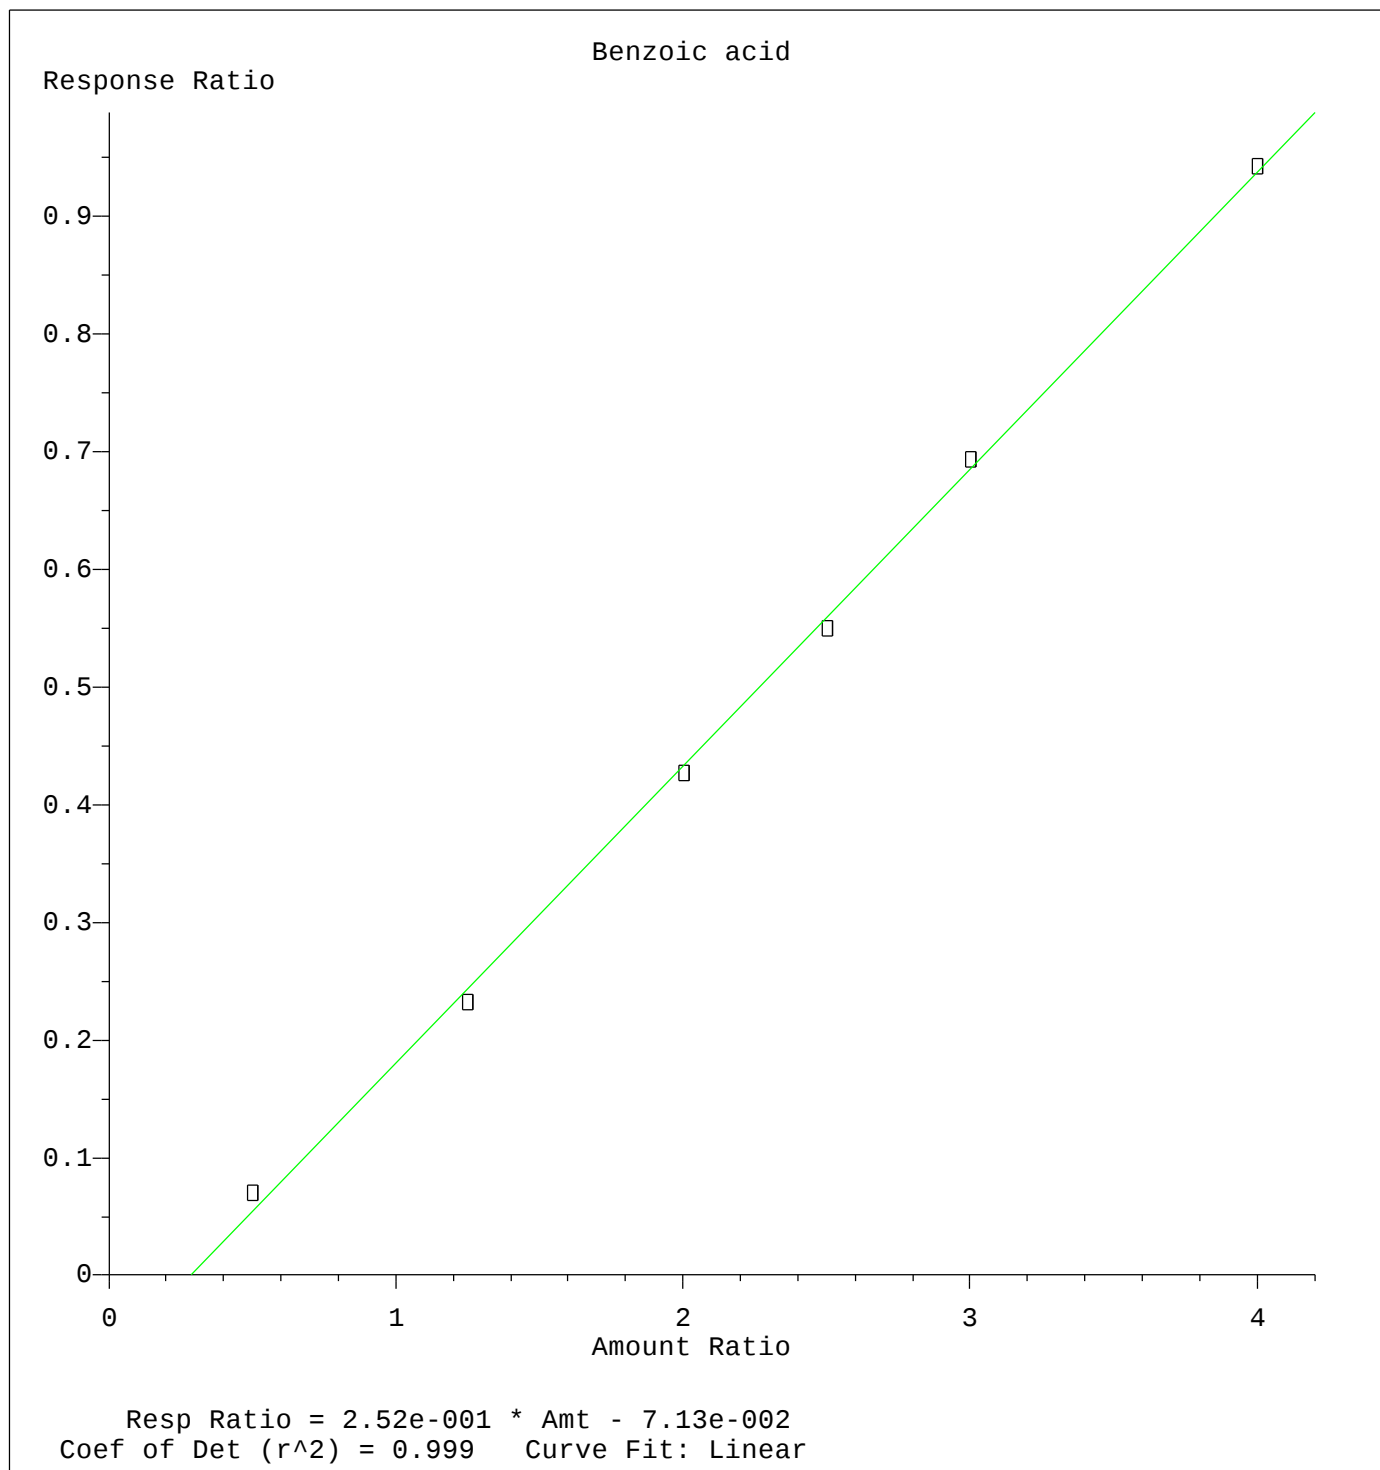

Method Name: Z:\HPCHEM1\BNA_G\METHODS\8270-BG111017.M
Calibration Table Last Updated: Fri Nov 10 15:38:25 2017


Hexachlorocyclopentadiene

Response Ratio

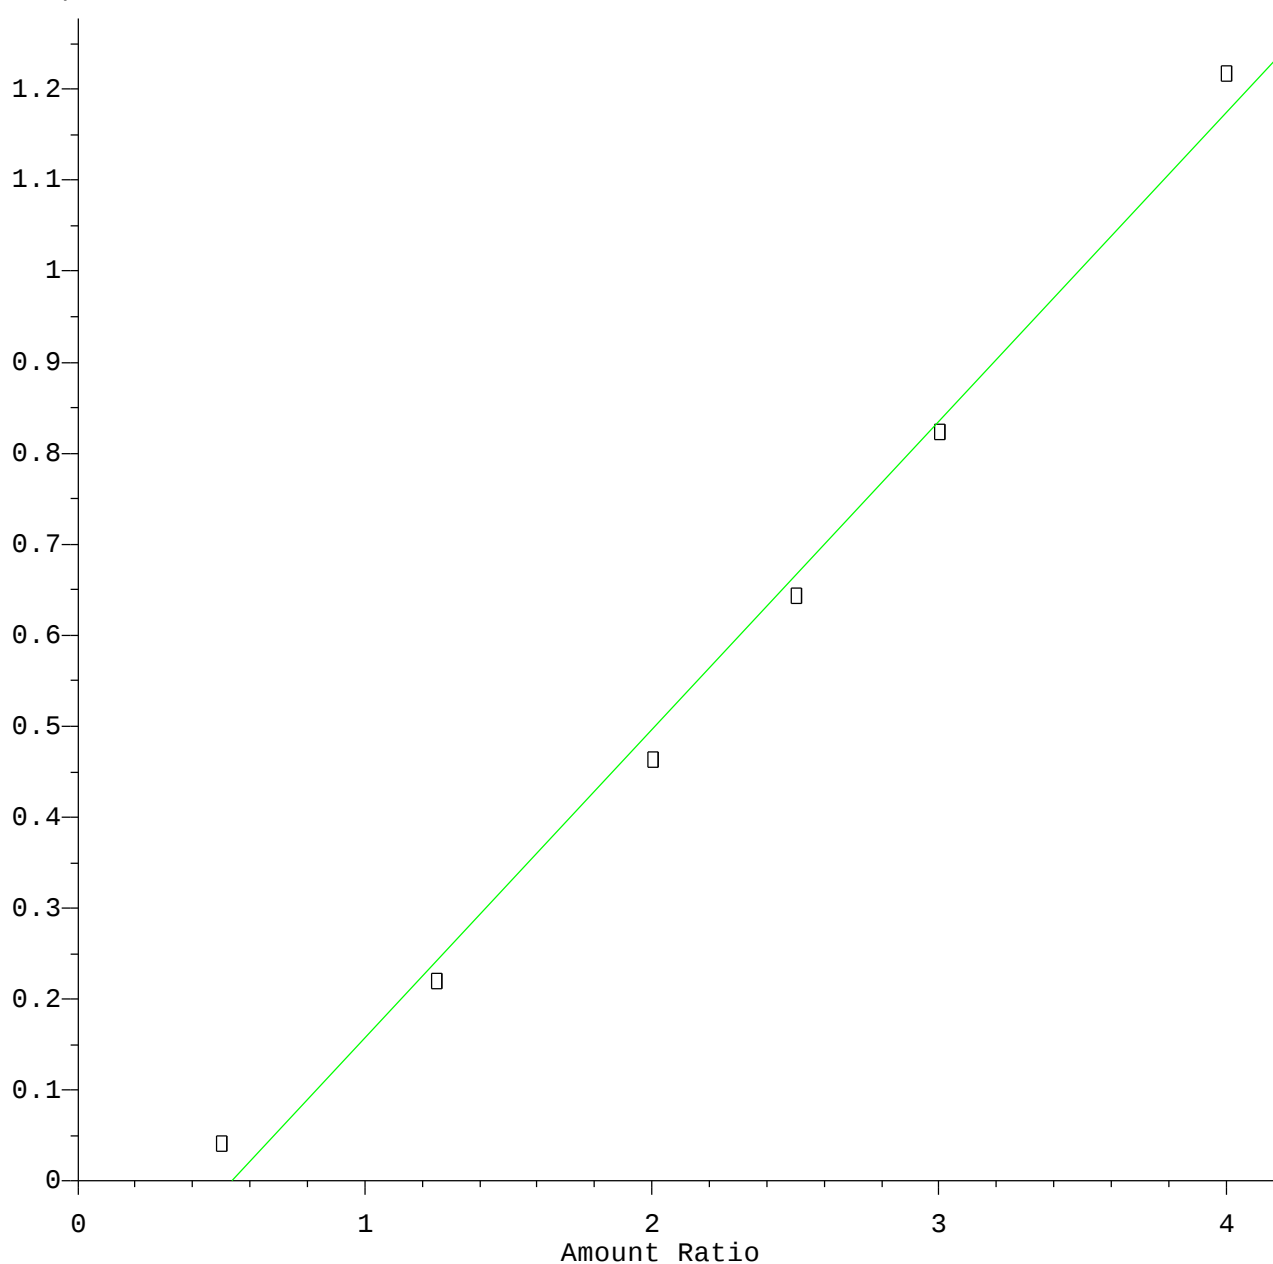

Resp Ratio = $3.39 \times 10^{-1} \times \text{Amt} - 1.80 \times 10^{-1}$
Coef of Det (r^2) = 0.992 Curve Fit: Linear

Method Name: Z:\HPCHEM1\BNA_G\METHODS\8270-BG111017.M
Calibration Table Last Updated: Fri Nov 10 15:38:25 2017

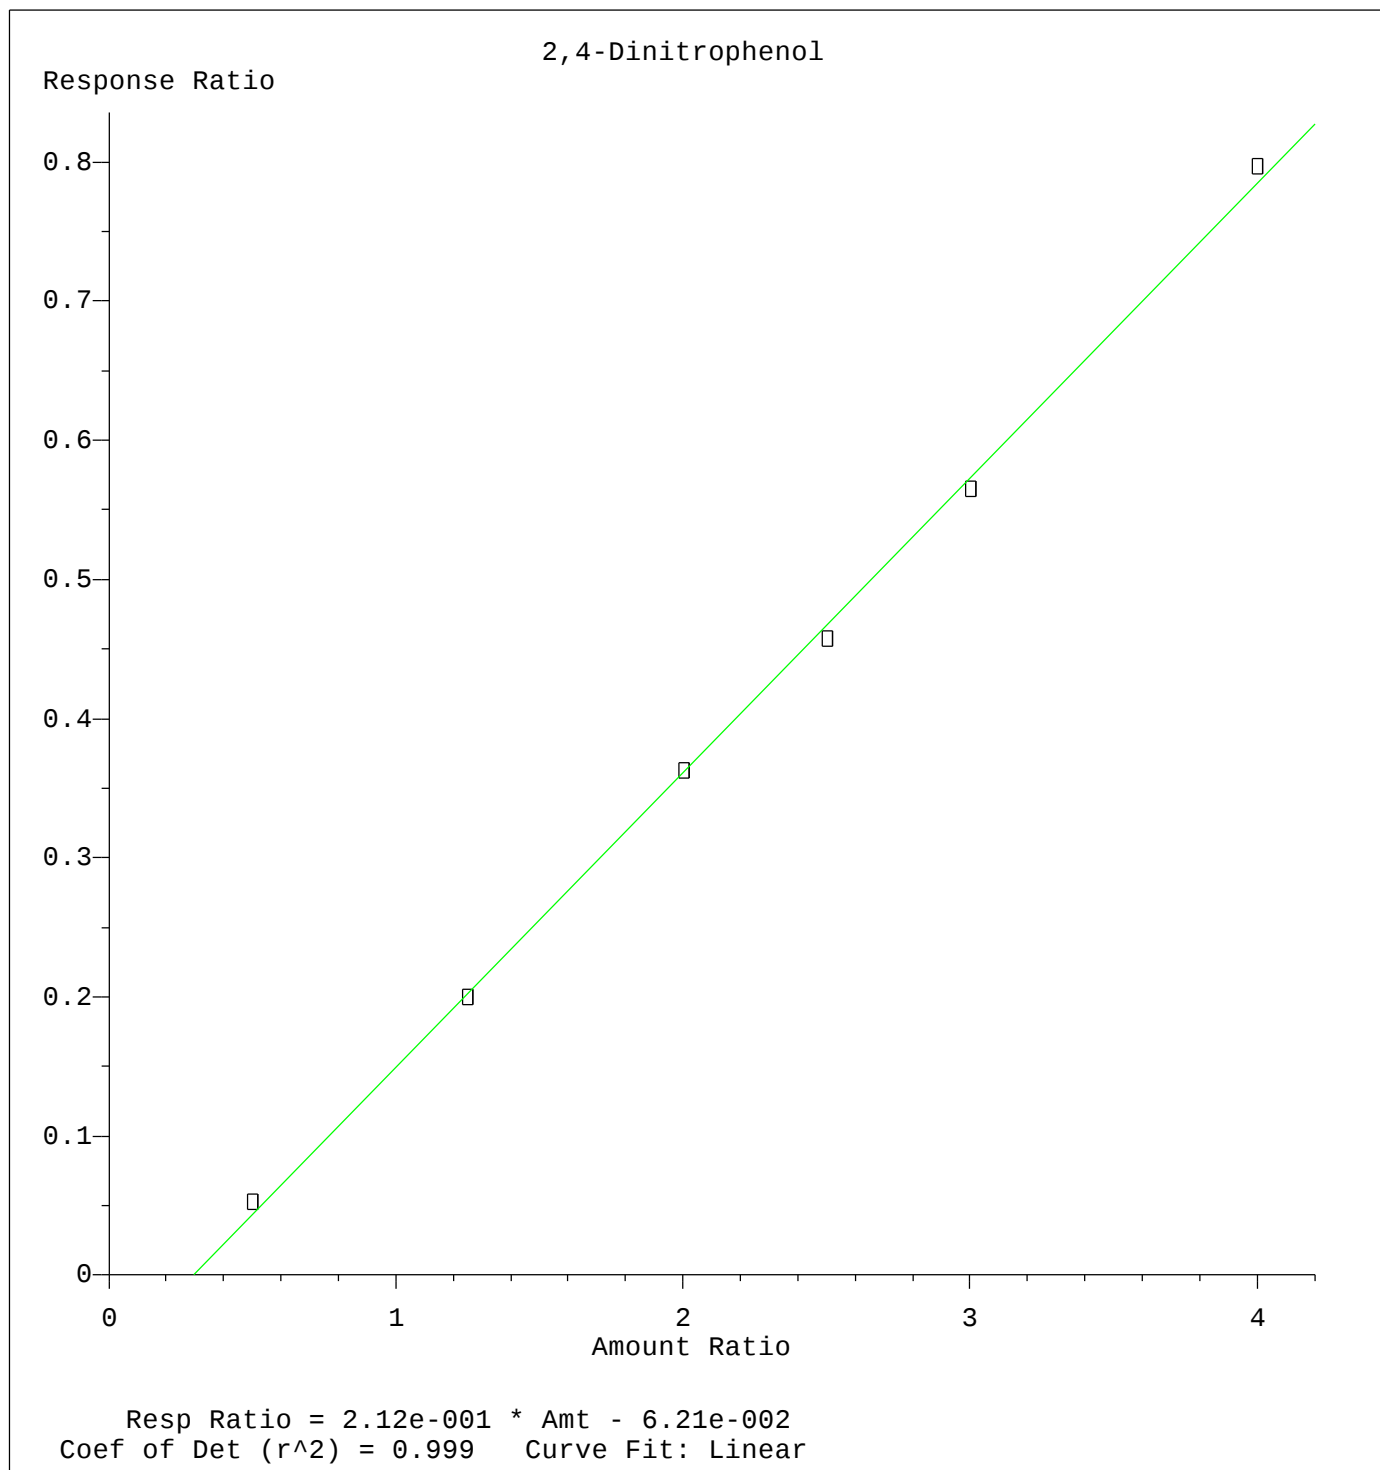

Method Name: Z:\HPCHEM1\BNA_G\METHODS\8270-BG111017.M
Calibration Table Last Updated: Fri Nov 10 15:38:25 2017