


Data Path : \\74.0.250.170\svoasrv\HPCHEM1\BNA G\Data\BG111017\
 Data File : BG030913.D
 Acq On : 10 Nov 2017 19:16
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG111017.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Nov 10 15:38:25 2017

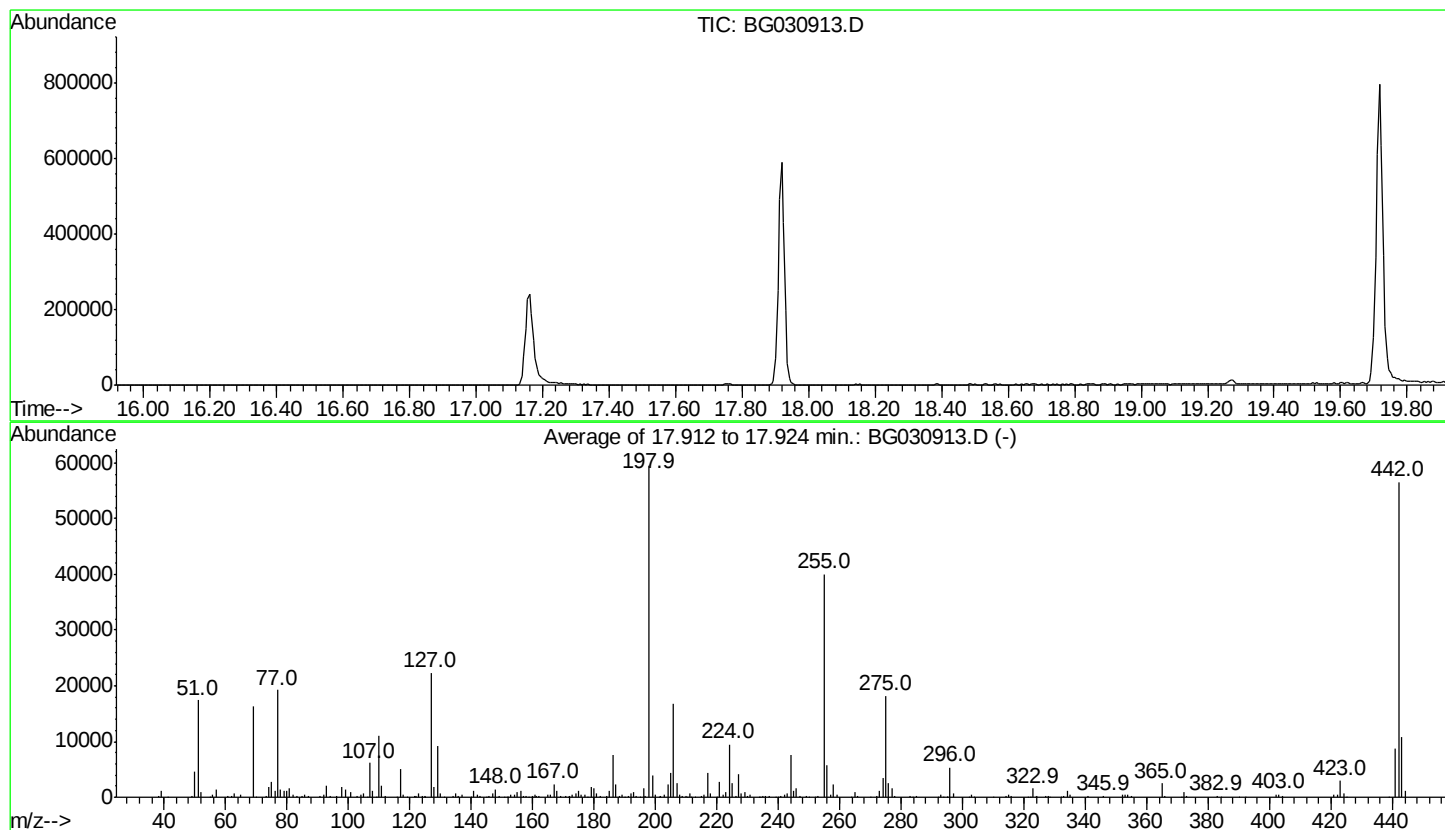

AutoFind: Scans 2489, 2490, 2491; Background Corrected with Scan 2482

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.2	17401	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	27.5	16397	PASS
70	69	0.00	2	0.3	51	PASS
127	198	10	80	37.5	22314	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	59533	PASS
199	198	5	9	6.5	3869	PASS
275	198	10	60	30.6	18227	PASS
365	198	1	100	4.2	2484	PASS
441	442	0.01	24	15.3	8642	PASS
442	198	50	100	95.0	56576	PASS
443	442	15	24	19.3	10897	PASS