

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111022\
 Data File : BG055547.D
 Acq On : 10 Nov 2022 20:16
 Operator : CG/JU
 Sample : N5474-01
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 5592-3

Quant Time: Nov 11 02:02:22 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG110922.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 10 03:39:46 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.270	152	44481	20.000	ng	0.00
21) Naphthalene-d8	11.096	136	179097	20.000	ng	0.00
39) Acenaphthene-d10	14.886	164	121709	20.000	ng	0.00
64) Phenanthrene-d10	17.624	188	285167	20.000	ng	0.00
76) Chrysene-d12	21.919	240	299520	20.000	ng	-0.01
86) Perylene-d12	25.338	264	315526	20.000	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.797	112	117151	50.165	ng	0.00
7) Phenol-d6	7.395	99	101612	31.500	ng	0.00
23) Nitrobenzene-d5	9.439	82	276336	104.599	ng	0.00
42) 2,4,6-Tribromophenol	16.361	330	155046	130.563	ng	0.00
45) 2-Fluorobiphenyl	13.517	172	615006	76.221	ng	0.00
79) Terphenyl-d14	20.215	244	914829	61.348	ng	0.00
Target Compounds						
						Qvalue
19) n-Nitroso-di-n-propyla...	9.439	70	37448	14.047	ng	# 82
48) 2-Nitroaniline	13.511	65	1206	4.414	ng	# 15
51) 2,6-Dinitrotoluene	14.886	165	15971	12.331	ng	# 21
57) 2,4-Dinitrotoluene	14.886	165	15971	10.499	ng	# 22
65) 4,6-Dinitro-2-methylph...	16.355	198	180	2.147	ng	# 1
67) 4-Bromophenyl-phenylether	16.361	248	10194	3.504	ng	# 1
80) Butylbenzylphthalate	20.897	149	503	3.425	ng	# 64


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111022\
Data File : BG055547.D
Acq On : 10 Nov 2022 20:16
Operator : CG/JU
Sample : N5474-01
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
5592-3

Quant Time: Nov 11 02:02:22 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG110922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 10 03:39:46 2022
Response via : Initial Calibration




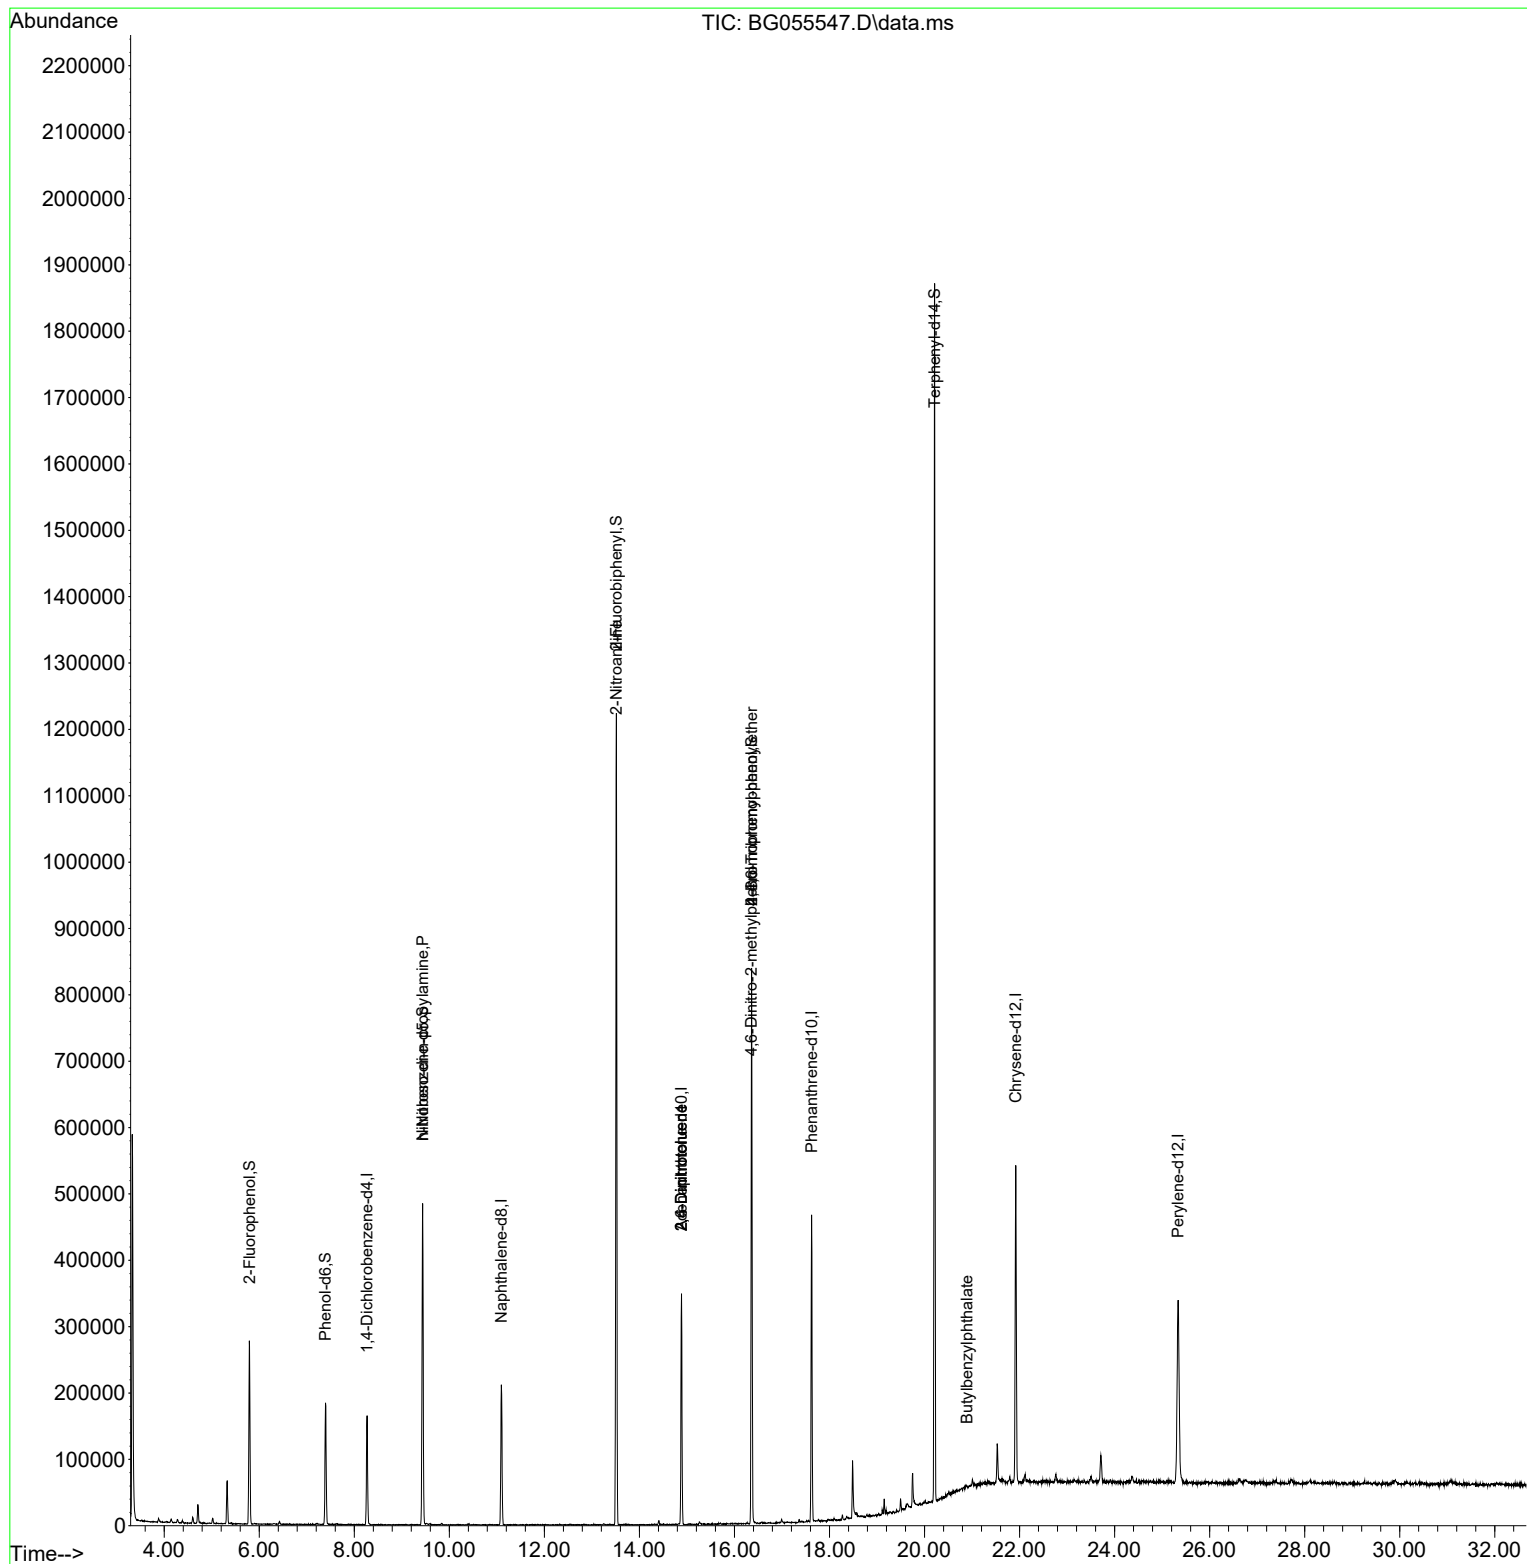




#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.270 min Scan# 84
Delta R.T. 0.000 min
Lab File: BG055547.D
Acq: 10 Nov 2022 20:16




Instrument :
BNA_G
ClientSampleId :
5592-3

Tgt Ion:152 Resp: 44481
Ion Ratio Lower Upper
152 100
150 165.0 121.0 181.4
115 66.6 47.8 71.8

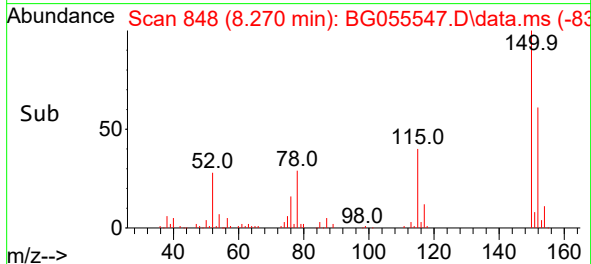

#5
2-Fluorophenol
Concen: 50.165 ng
RT: 5.797 min Scan# 427
Delta R.T. 0.006 min
Lab File: BG055547.D
Acq: 10 Nov 2022 20:16

Tgt Ion:112 Resp: 117151
Ion Ratio Lower Upper
112 100
64 64.8 52.6 78.8
63 34.6 28.3 42.5


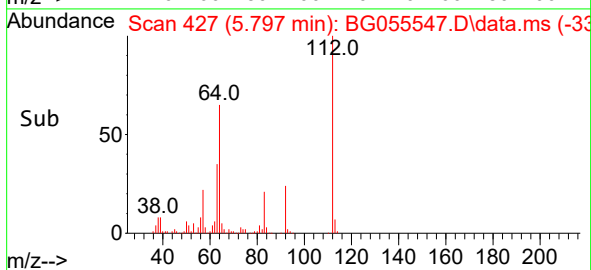

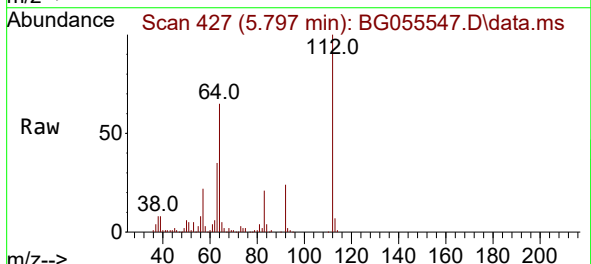




#7
Phenol-d6
Concen: 31.500 ng
RT: 7.395 min Scan# 61
Delta R.T. -0.006 min
Lab File: BG055547.D
Acq: 10 Nov 2022 20:16




Instrument :
BNA_G
ClientSampleId :
5592-3


Tgt Ion: 99 Resp: 101612
Ion Ratio Lower Upper
99 100
42 24.3 17.5 26.3
71 35.8 28.3 42.5

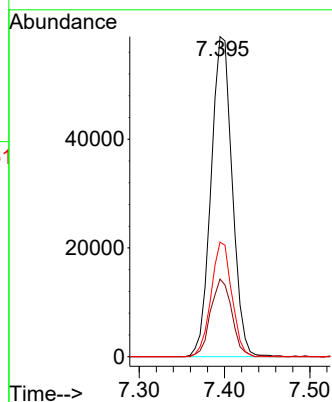

#19
n-Nitroso-di-n-propylamine
Concen: 14.047 ng
RT: 9.439 min Scan# 1047
Delta R.T. 0.364 min
Lab File: BG055547.D
Acq: 10 Nov 2022 20:16

Tgt Ion: 70 Resp: 37448
Ion Ratio Lower Upper
70 100
42 58.9 54.8 82.2
101 0.0 6.8 10.2#
130 1.8 14.9 22.3#


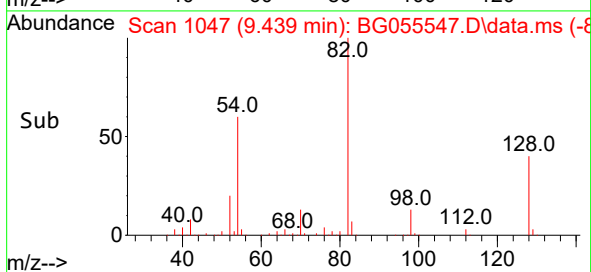






#21
Naphthalene-d8
Concen: 20.000 ng
RT: 11.096 min Scan# 11
Delta R.T. -0.006 min
Lab File: BG055547.D
Acq: 10 Nov 2022 20:16




Instrument :
BNA_G
ClientSampleId :
5592-3


Tgt Ion:136 Resp: 179097
Ion Ratio Lower Upper
136 100
137 11.3 8.6 12.8
54 10.1 8.6 12.8
68 6.5 4.6 6.8

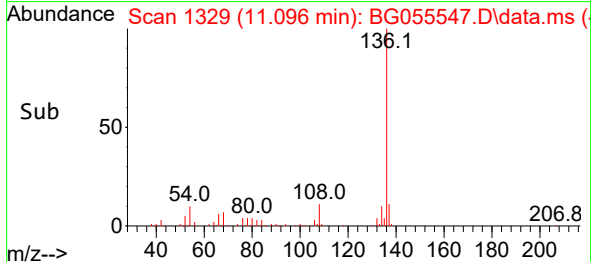

#23
Nitrobenzene-d5
Concen: 104.599 ng
RT: 9.439 min Scan# 1047
Delta R.T. -0.006 min
Lab File: BG055547.D
Acq: 10 Nov 2022 20:16

Tgt Ion: 82 Resp: 276336
Ion Ratio Lower Upper
82 100
128 39.6 32.6 49.0
54 59.7 47.3 70.9


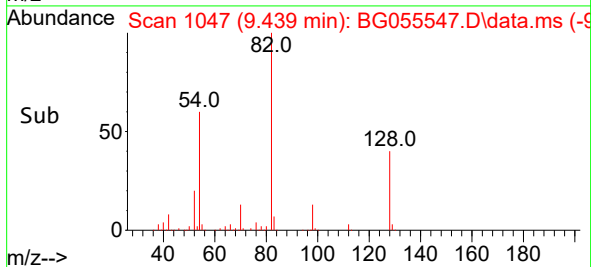

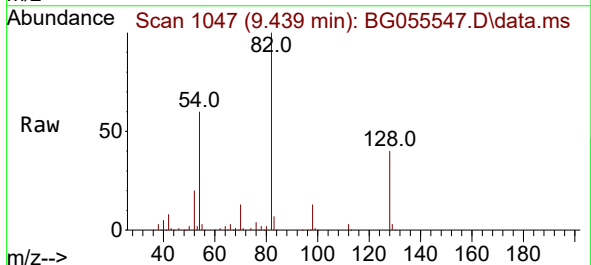




#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.886 min Scan# 1975
Delta R.T. -0.006 min
Lab File: BG055547.D
Acq: 10 Nov 2022 20:16




Instrument :
BNA_G
ClientSampleId :
5592-3


Tgt Ion:164 Resp: 121709
Ion Ratio Lower Upper
164 100
162 103.7 81.3 121.9
160 44.7 35.9 53.9

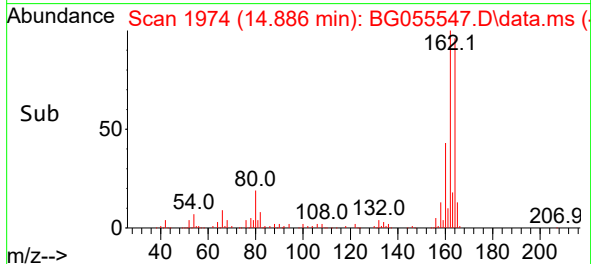

#42
2,4,6-Tribromophenol
Concen: 130.563 ng
RT: 16.361 min Scan# 2225
Delta R.T. -0.006 min
Lab File: BG055547.D
Acq: 10 Nov 2022 20:16

Tgt Ion:330 Resp: 155046
Ion Ratio Lower Upper
330 100
332 96.7 77.4 116.2
141 33.7 25.4 38.2


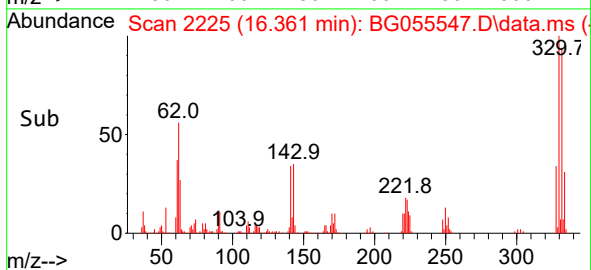

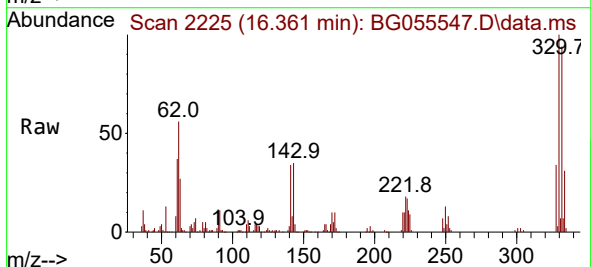




#45
2-Fluorobiphenyl
Concen: 76.221 ng
RT: 13.517 min Scan# 1740
Delta R.T. -0.000 min
Lab File: BG055547.D
Acq: 10 Nov 2022 20:16




Instrument :
BNA_G
ClientSampleId :
5592-3


Tgt Ion:172 Resp: 615006
Ion Ratio Lower Upper
172 100
171 36.6 29.7 44.5
170 24.3 19.8 29.6

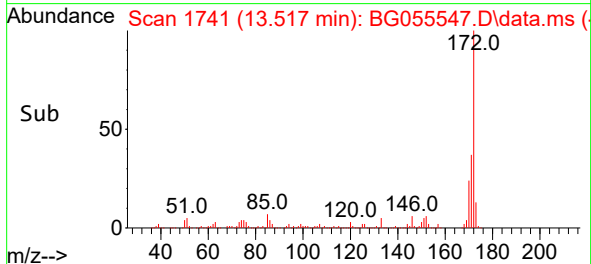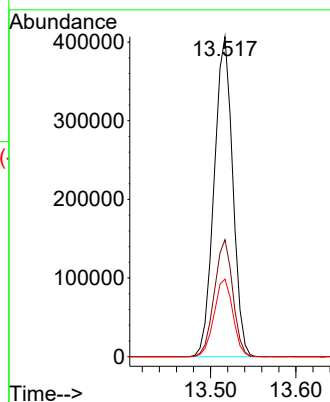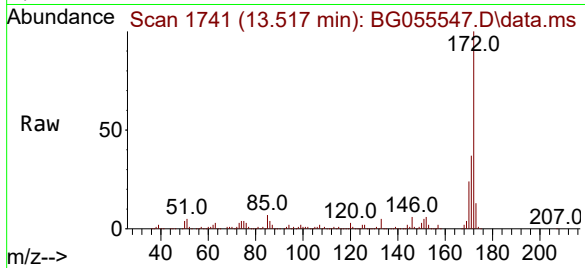

#48
2-Nitroaniline
Concen: 4.414 ng
RT: 13.511 min Scan# 1740
Delta R.T. -0.453 min
Lab File: BG055547.D
Acq: 10 Nov 2022 20:16

Tgt Ion: 65 Resp: 1206
Ion Ratio Lower Upper
65 100
92 159.8 51.6 77.4#
138 37.3 77.0 115.4#


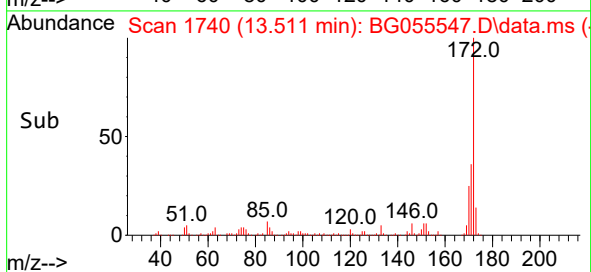
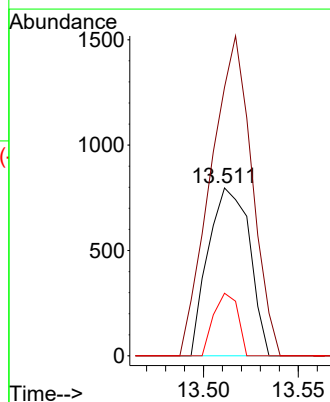
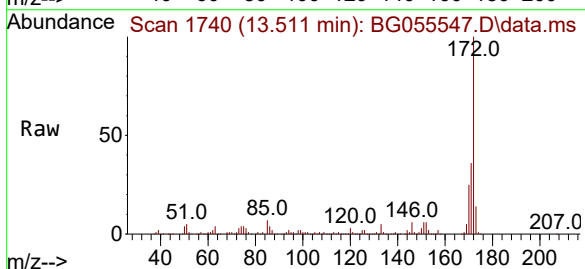




#51
2,6-Dinitrotoluene
Concen: 12.331 ng
RT: 14.886 min Scan# 1900
Delta R.T. 0.435 min
Lab File: BG055547.D
Acq: 10 Nov 2022 20:16




Instrument :
BNA_G
ClientSampleId :
5592-3


Tgt Ion:165 Resp: 15971
Ion Ratio Lower Upper
165 100
63 0.0 50.1 75.1#
89 1.7 46.5 69.7#

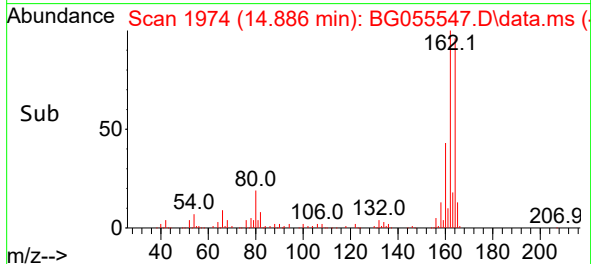

#57
2,4-Dinitrotoluene
Concen: 10.499 ng
RT: 14.886 min Scan# 1974
Delta R.T. -0.347 min
Lab File: BG055547.D
Acq: 10 Nov 2022 20:16

Tgt Ion:165 Resp: 15971
Ion Ratio Lower Upper
165 100
63 0.0 37.0 55.4#
89 1.7 58.6 87.8#
182 0.0 2.2 3.2#


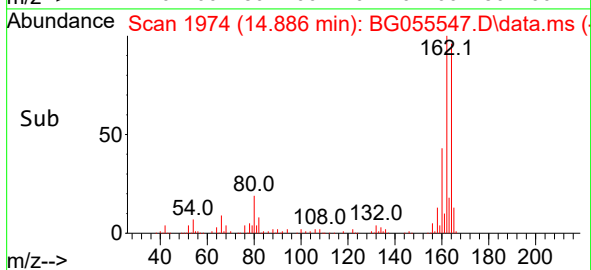

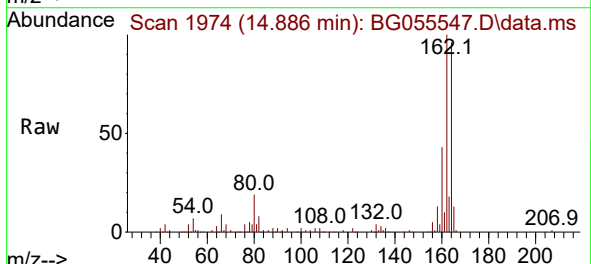




#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.624 min Scan# 2441
Delta R.T. -0.006 min
Lab File: BG055547.D
Acq: 10 Nov 2022 20:16




Instrument :
BNA_G
ClientSampleId :
5592-3


Tgt Ion:188 Resp: 285167
Ion Ratio Lower Upper
188 100
94 8.3 6.4 9.6
80 9.1 7.6 11.4

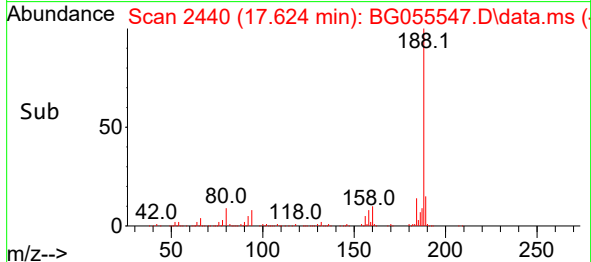

#65
4,6-Dinitro-2-methylphenol
Concen: 2.147 ng
RT: 16.355 min Scan# 2224
Delta R.T. 0.364 min
Lab File: BG055547.D
Acq: 10 Nov 2022 20:16

Tgt Ion:198 Resp: 180
Ion Ratio Lower Upper
198 100
51 164.4 24.7 64.7#
105 151.6 17.6 57.6#


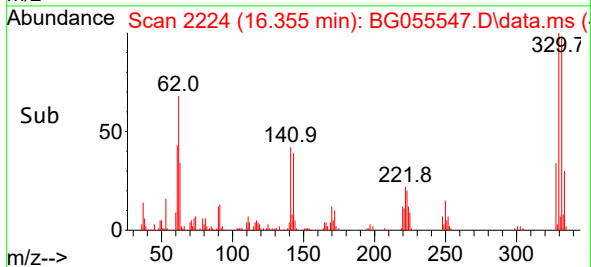

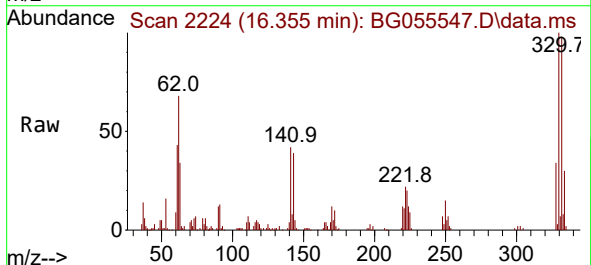




#67
4-Bromophenyl-phenylether
Concen: 3.504 ng
RT: 16.361 min Scan# 21
Delta R.T. -0.452 min
Lab File: BG055547.D
Acq: 10 Nov 2022 20:16




Instrument :
BNA_G
ClientSampleId :
5592-3


Tgt Ion:248 Resp: 10194
Ion Ratio Lower Upper
248 100
250 178.6 76.9 115.3#
141 473.4 54.3 81.5#

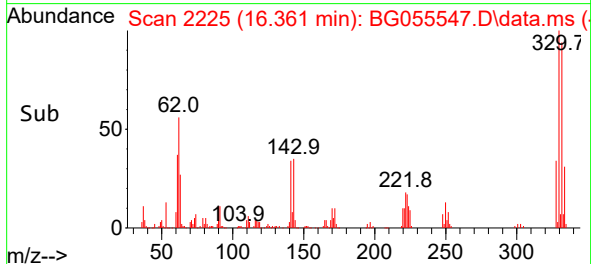

#76
Chrysene-d12
Concen: 20.000 ng
RT: 21.919 min Scan# 3171
Delta R.T. -0.012 min
Lab File: BG055547.D
Acq: 10 Nov 2022 20:16

Tgt Ion:240 Resp: 299520
Ion Ratio Lower Upper
240 100
120 8.5 6.1 9.1
236 25.7 21.4 32.0



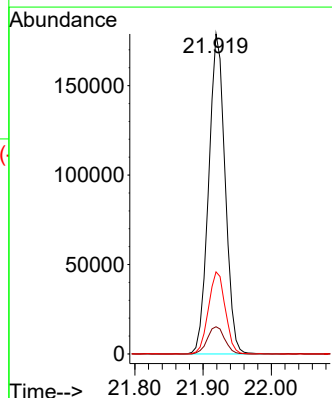
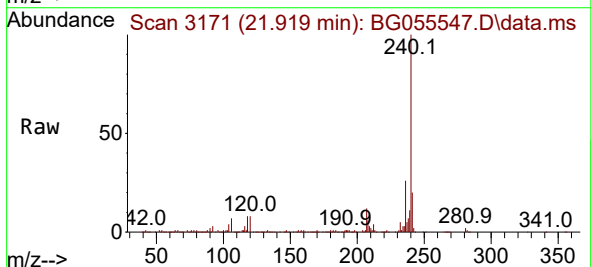




#79
 Terphenyl-d14
 Concen: 61.348 ng
 RT: 20.215 min Scan# 2881
 Delta R.T. -0.000 min
 Lab File: BG055547.D
 Acq: 10 Nov 2022 20:16




Instrument :
 BNA_G
 ClientSampleId :
 5592-3


Tgt Ion:244 Resp: 914829
 Ion Ratio Lower Upper
 244 100
 212 7.7 6.5 9.7
 122 8.6 7.7 11.5

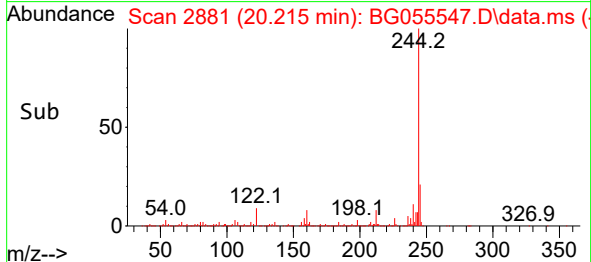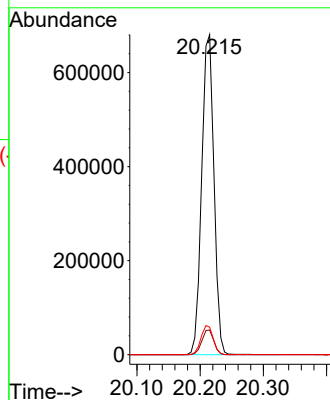

#80
 Butylbenzylphthalate
 Concen: 3.425 ng
 RT: 20.897 min Scan# 2997
 Delta R.T. -0.006 min
 Lab File: BG055547.D
 Acq: 10 Nov 2022 20:16

Tgt Ion:149 Resp: 503
 Ion Ratio Lower Upper
 149 100
 91 43.2 56.8 85.2#
 206 0.0 17.3 25.9#

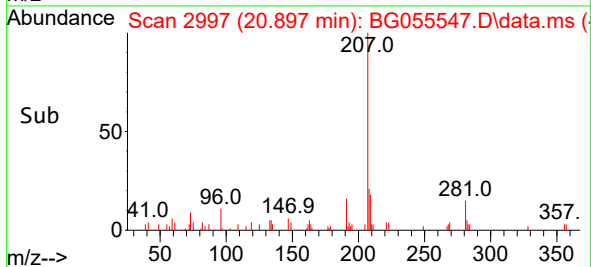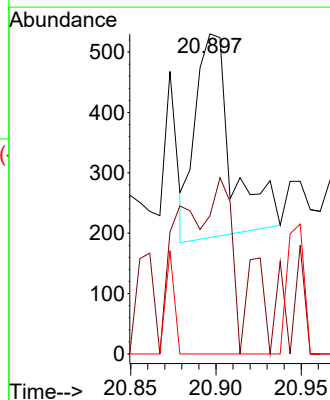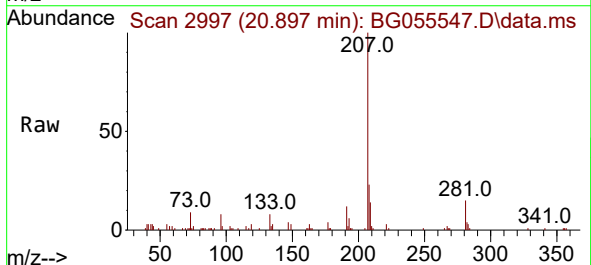



#86
Perylene-d12
Concen: 20.000 ng
RT: 25.338 min Scan# 31
Delta R.T. -0.012 min
Lab File: BG055547.D
Acq: 10 Nov 2022 20:16

Instrument :
BNA_G
ClientSampleId :
5592-3

Tgt Ion:264 Resp: 315526

Ion	Ratio	Lower	Upper
264	100		
260	22.3	19.4	29.2
265	21.5	17.1	25.7

