

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111022\
 Data File : BG055557.D
 Acq On : 11 Nov 2022 3:09
 Operator : CG/JU
 Sample : N5494-05
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SB-17

Quant Time: Nov 11 04:43:37 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG110922.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 10 03:39:46 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.271	152	47028	20.000	ng	0.00
21) Naphthalene-d8	11.097	136	195417	20.000	ng	0.00
39) Acenaphthene-d10	14.887	164	132479	20.000	ng	0.00
64) Phenanthrene-d10	17.625	188	312347	20.000	ng	0.00
76) Chrysene-d12	21.920	240	312825	20.000	ng	#-0.01
86) Perylene-d12	25.339	264	324704	20.000	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.797	112	314112	127.221	ng	0.00
7) Phenol-d6	7.401	99	415607	121.860	ng	0.00
23) Nitrobenzene-d5	9.434	82	244850	84.941	ng	-0.01
42) 2,4,6-Tribromophenol	16.367	330	177360	137.211	ng	0.00
45) 2-Fluorobiphenyl	13.512	172	587232	66.862	ng	0.00
79) Terphenyl-d14	20.210	244	1042030	66.906	ng	0.00
Target Compounds						
						Qvalue
19) n-Nitroso-di-n-propyla...	9.434	70	32741	11.616	ng	# 85
48) 2-Nitroaniline	13.518	65	1100	4.312	ng	# 1
51) 2,6-Dinitrotoluene	14.887	165	16949	12.101	ng	# 21
57) 2,4-Dinitrotoluene	14.887	165	16949	10.327	ng	# 22
65) 4,6-Dinitro-2-methylph...	16.362	198	495	2.549	ng	# 1
67) 4-Bromophenyl-phenylether	16.367	248	11358	3.564	ng	# 1
80) Butylbenzylphthalate	20.892	149	732	3.449	ng	# 58


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111022\
Data File : BG055557.D
Acq On : 11 Nov 2022 3:09
Operator : CG/JU
Sample : N5494-05
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SB-17

Quant Time: Nov 11 04:43:37 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG110922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 10 03:39:46 2022
Response via : Initial Calibration




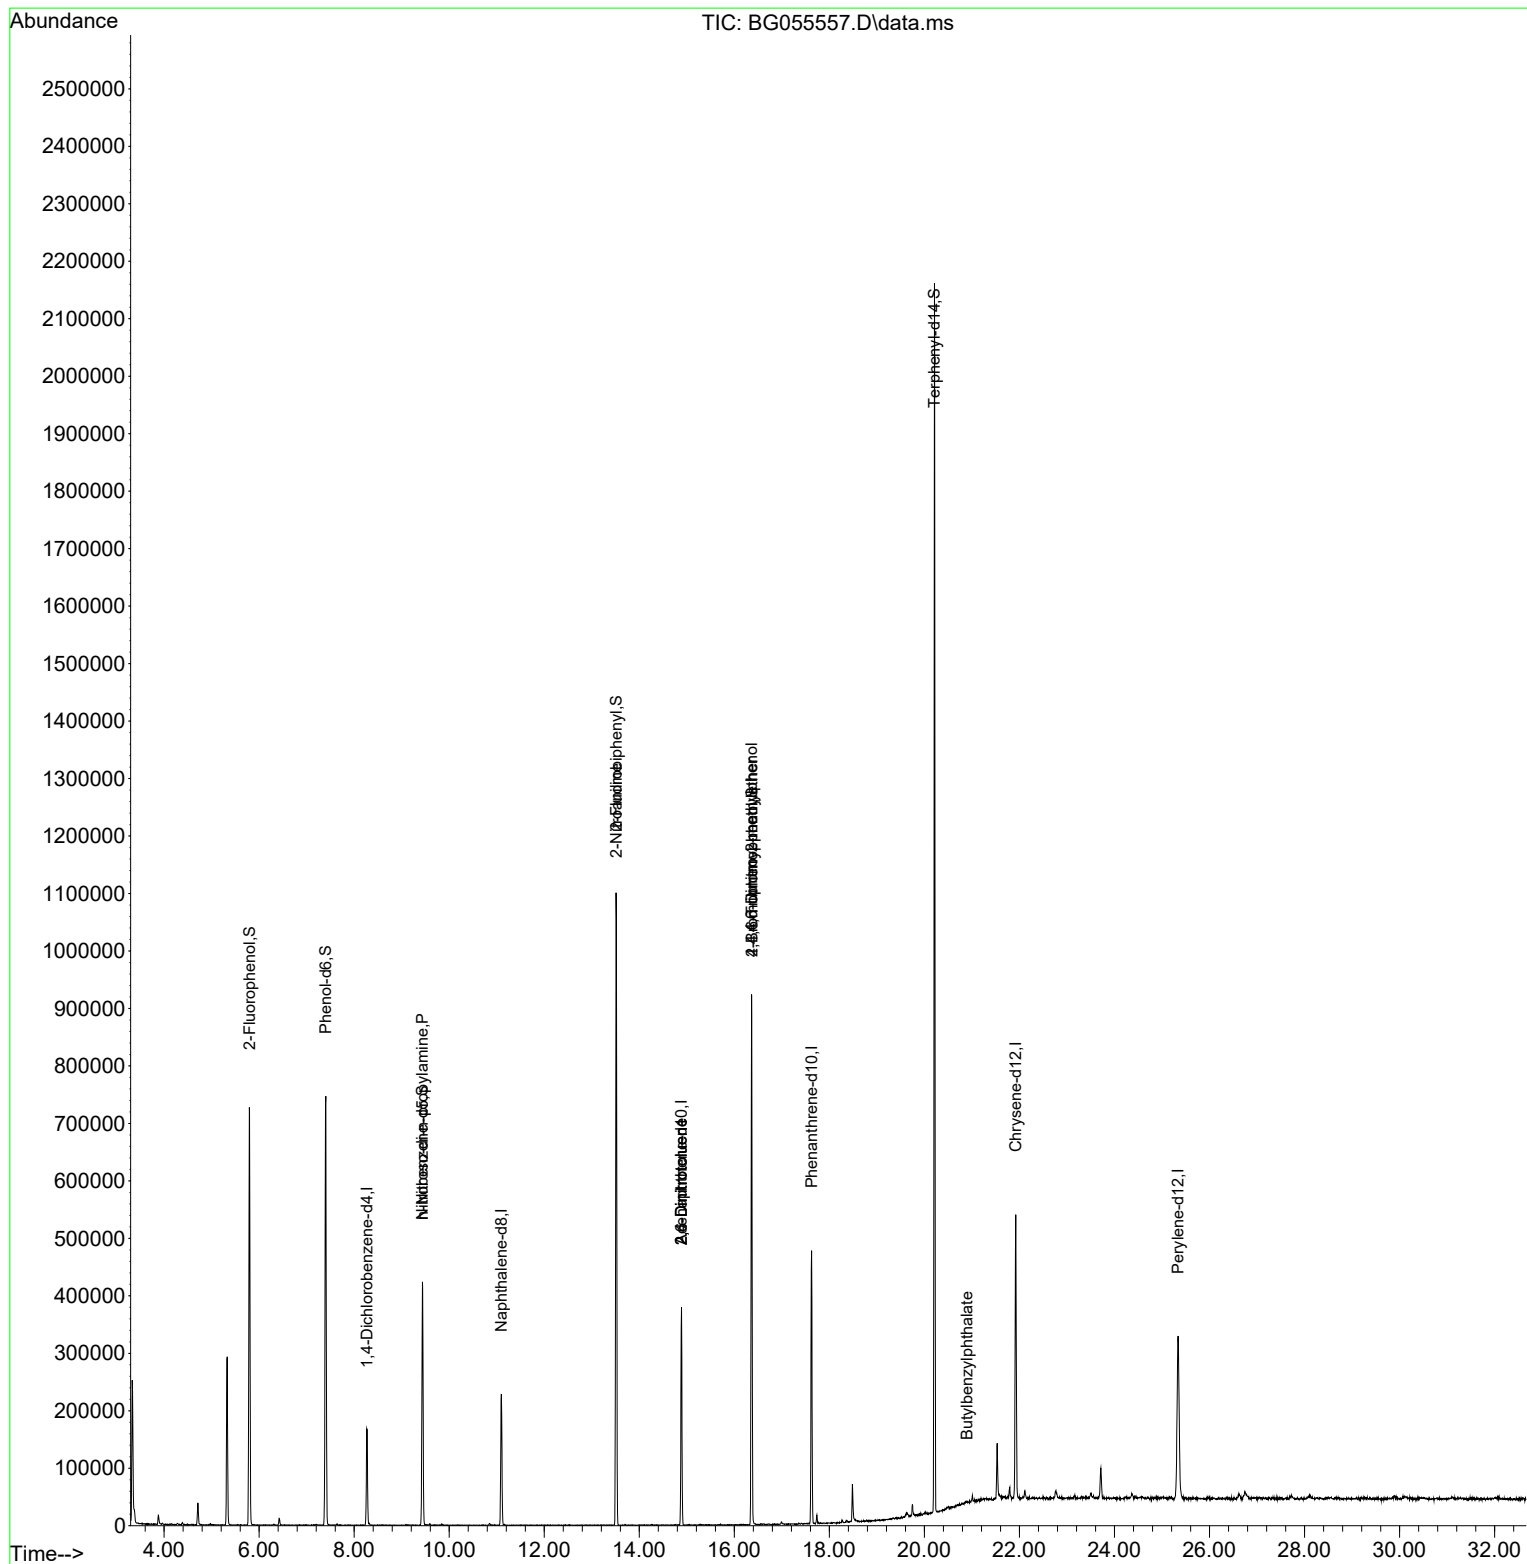




#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.271 min Scan# 84
Delta R.T. 0.001 min
Lab File: BG055557.D
Acq: 11 Nov 2022 3:09




Instrument :
BNA_G
ClientSampleId :
SB-17


Tgt Ion:152 Resp: 47028
Ion Ratio Lower Upper
152 100
150 148.1 121.0 181.4
115 56.4 47.8 71.8

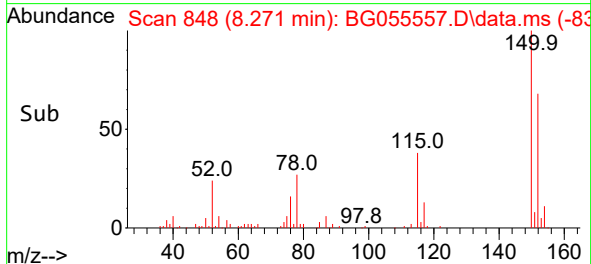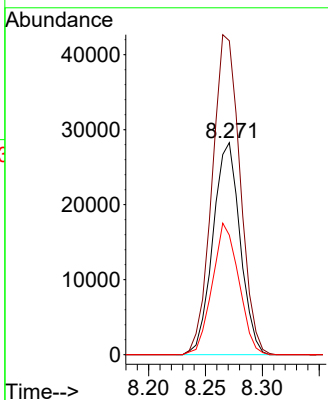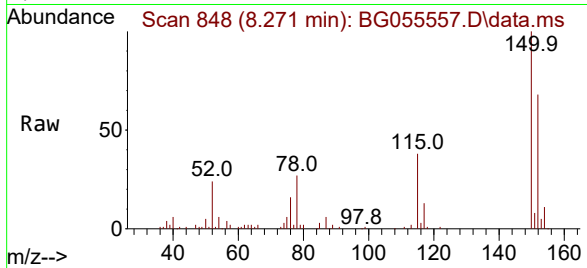

#5
2-Fluorophenol
Concen: 127.221 ng
RT: 5.797 min Scan# 427
Delta R.T. 0.006 min
Lab File: BG055557.D
Acq: 11 Nov 2022 3:09

Tgt Ion:112 Resp: 314112
Ion Ratio Lower Upper
112 100
64 66.7 52.6 78.8
63 35.2 28.3 42.5


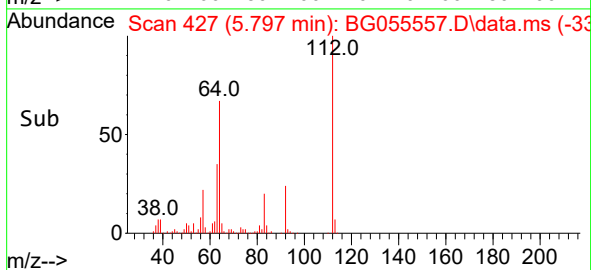
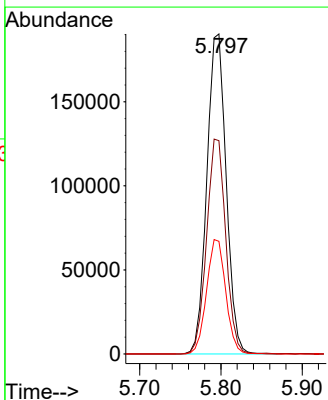
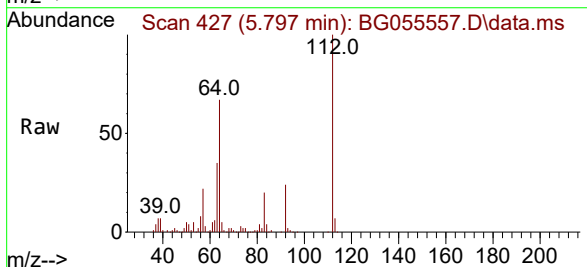


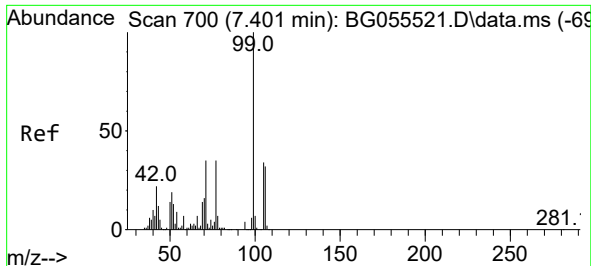

#7
Phenol-d6
Concen: 121.860 ng
RT: 7.401 min Scan# 700
Delta R.T. 0.000 min
Lab File: BG055557.D
Acq: 11 Nov 2022 3:09




Instrument :
BNA_G
ClientSampleId :
SB-17


Tgt Ion: 99 Resp: 415607
Ion Ratio Lower Upper
99 100
42 21.9 17.5 26.3
71 35.1 28.3 42.5

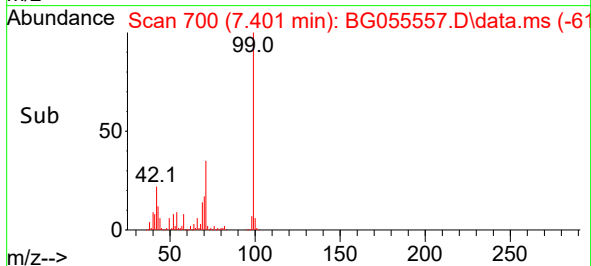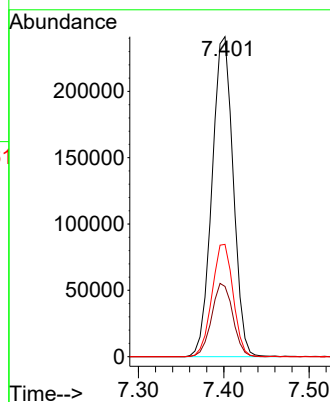

#19
n-Nitroso-di-n-propylamine
Concen: 11.616 ng
RT: 9.434 min Scan# 1046
Delta R.T. 0.359 min
Lab File: BG055557.D
Acq: 11 Nov 2022 3:09

Tgt Ion: 70 Resp: 32741
Ion Ratio Lower Upper
70 100
42 61.8 54.8 82.2
101 0.0 6.8 10.2#
130 1.8 14.9 22.3#


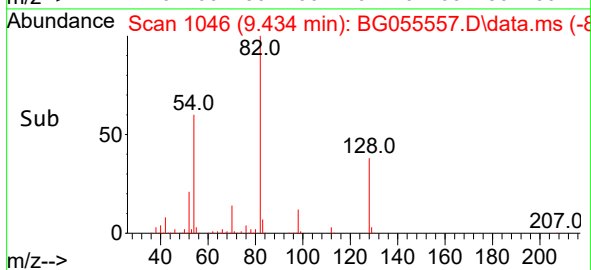
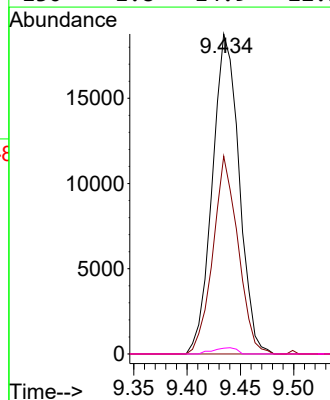
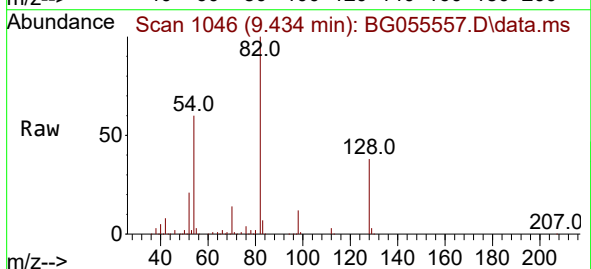


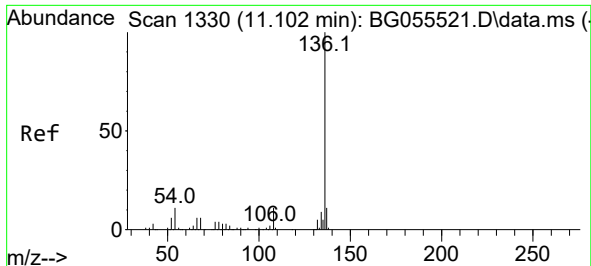

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 11.097 min Scan# 11
Delta R.T. -0.005 min
Lab File: BG055557.D
Acq: 11 Nov 2022 3:09




Instrument :
BNA_G
ClientSampleId :
SB-17


Tgt Ion:	136	Resp:	195417
Ion Ratio	Lower	Upper	
136	100		
137	11.6	8.6	12.8
54	10.3	8.6	12.8
68	6.1	4.6	6.8

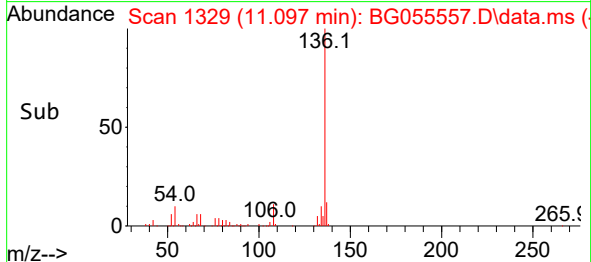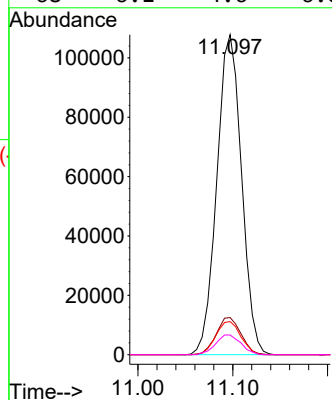

#23
Nitrobenzene-d5
Concen: 84.941 ng
RT: 9.434 min Scan# 1046
Delta R.T. -0.011 min
Lab File: BG055557.D
Acq: 11 Nov 2022 3:09

Tgt Ion:	82	Resp:	244850
Ion Ratio	Lower	Upper	
82	100		
128	38.4	32.6	49.0
54	59.8	47.3	70.9


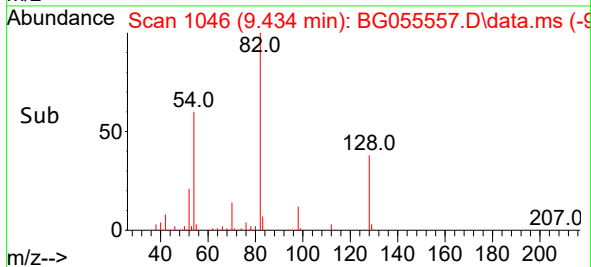
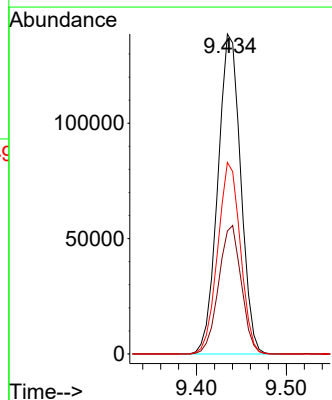
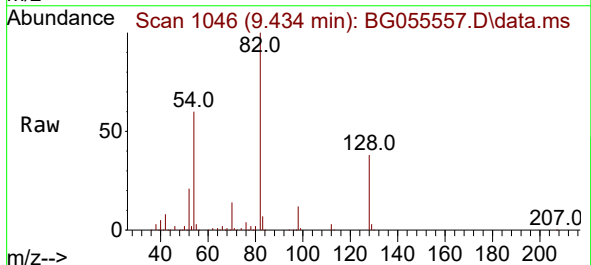


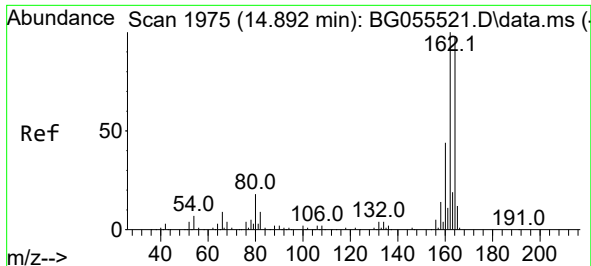

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.887 min Scan# 1974
Delta R.T. -0.005 min
Lab File: BG055557.D
Acq: 11 Nov 2022 3:09




Instrument :
BNA_G
ClientSampleId :
SB-17


Tgt Ion:164 Resp: 132479
Ion Ratio Lower Upper
164 100
162 101.5 81.3 121.9
160 43.9 35.9 53.9

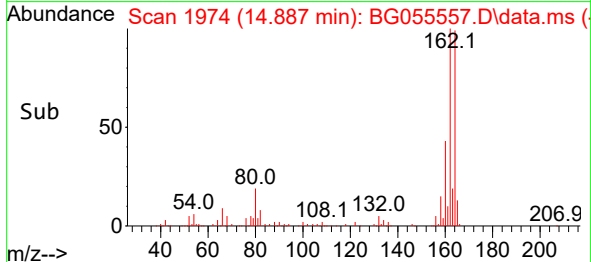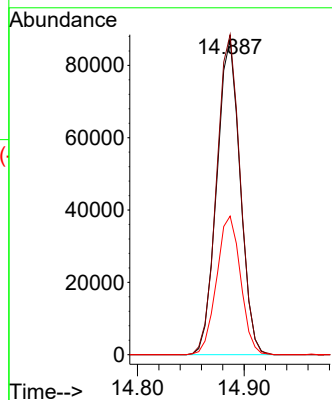

#42
2,4,6-Tribromophenol
Concen: 137.211 ng
RT: 16.367 min Scan# 2226
Delta R.T. 0.000 min
Lab File: BG055557.D
Acq: 11 Nov 2022 3:09

Tgt Ion:330 Resp: 177360
Ion Ratio Lower Upper
330 100
332 95.4 77.4 116.2
141 33.1 25.4 38.2


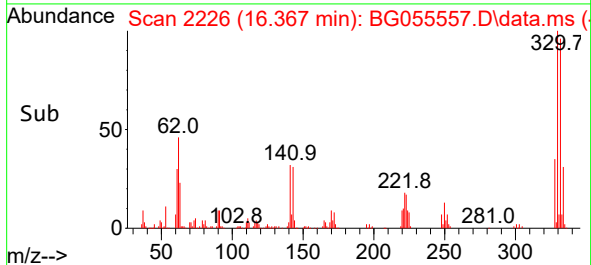
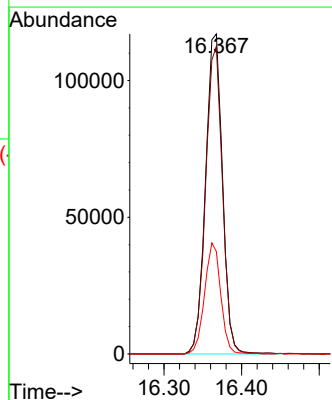
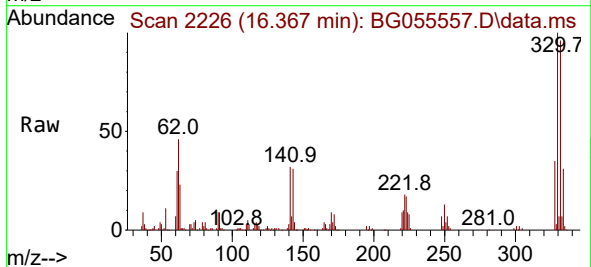


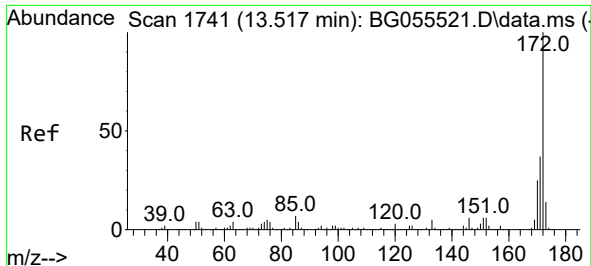

#45
2-Fluorobiphenyl
Concen: 66.862 ng
RT: 13.512 min Scan# 1741
Delta R.T. -0.005 min
Lab File: BG055557.D
Acq: 11 Nov 2022 3:09




Instrument :
BNA_G
ClientSampleId :
SB-17


Tgt Ion:172 Resp: 587232
Ion Ratio Lower Upper
172 100
171 37.5 29.7 44.5
170 25.0 19.8 29.6

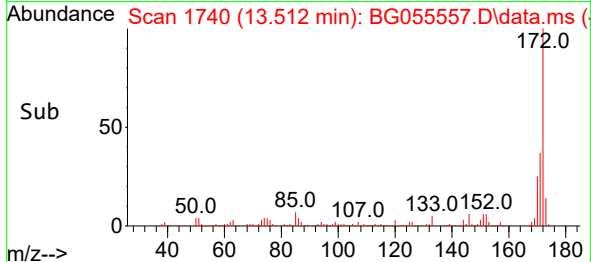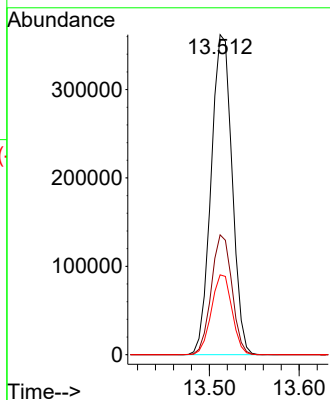

#48
2-Nitroaniline
Concen: 4.312 ng
RT: 13.518 min Scan# 1741
Delta R.T. -0.446 min
Lab File: BG055557.D
Acq: 11 Nov 2022 3:09

Tgt Ion: 65 Resp: 1100
Ion Ratio Lower Upper
65 100
92 198.1 51.6 77.4#
138 23.1 77.0 115.4#


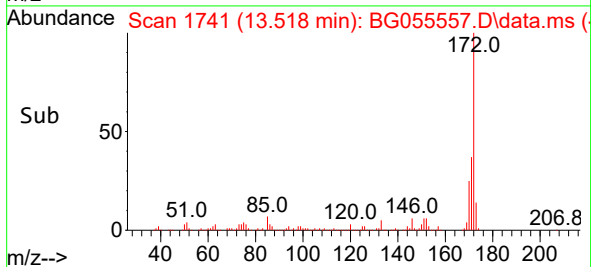
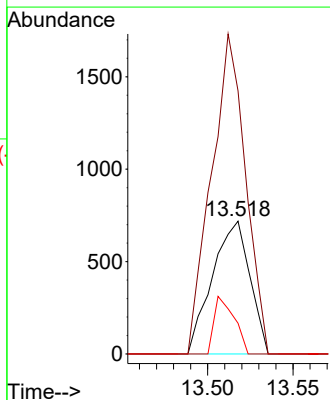
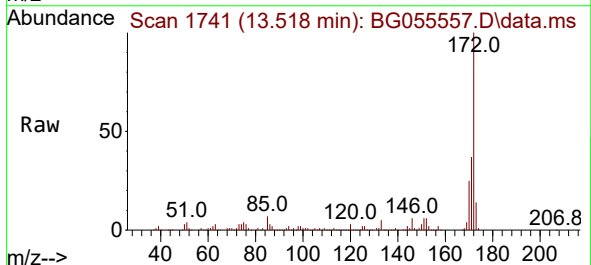


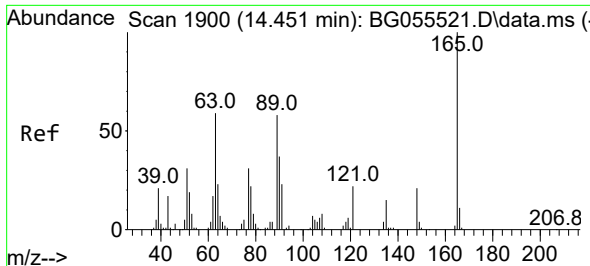

#51
2,6-Dinitrotoluene
Concen: 12.101 ng
RT: 14.887 min Scan# 1900
Delta R.T. 0.436 min
Lab File: BG055557.D
Acq: 11 Nov 2022 3:09




Instrument :
BNA_G
ClientSampleId :
SB-17


Tgt Ion:165 Resp: 16949
Ion Ratio Lower Upper
165 100
63 0.0 50.1 75.1#
89 1.4 46.5 69.7#

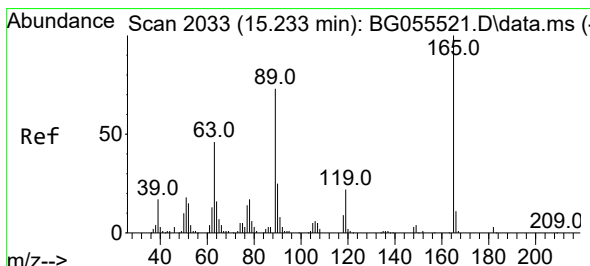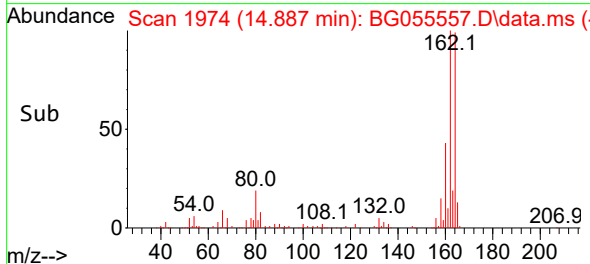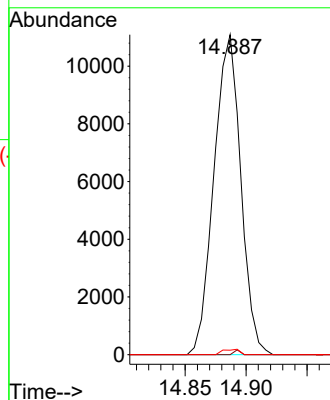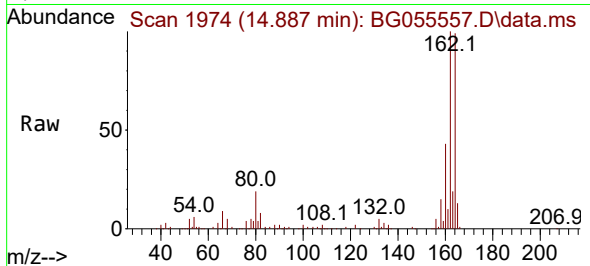

#57
2,4-Dinitrotoluene
Concen: 10.327 ng
RT: 14.887 min Scan# 1974
Delta R.T. -0.346 min
Lab File: BG055557.D
Acq: 11 Nov 2022 3:09

Tgt Ion:165 Resp: 16949
Ion Ratio Lower Upper
165 100
63 0.0 37.0 55.4#
89 1.4 58.6 87.8#
182 0.0 2.2 3.2#


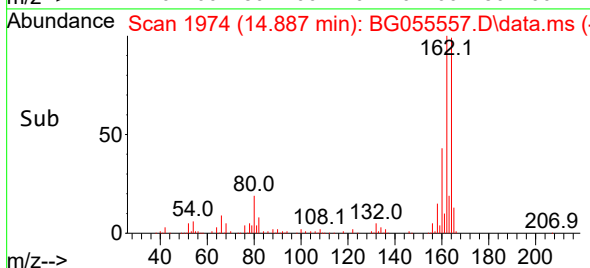
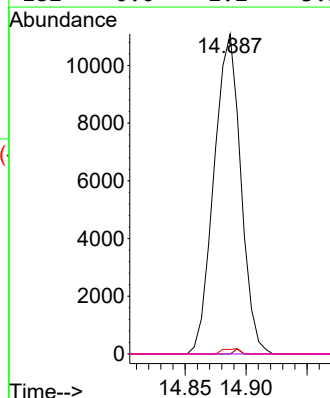
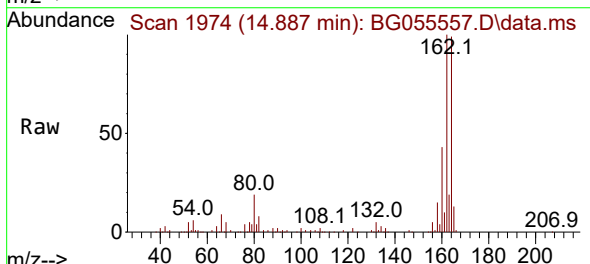


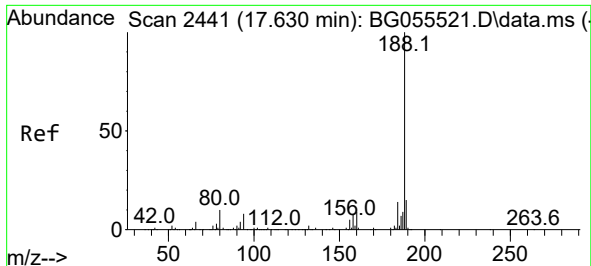

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.625 min Scan# 2441
Delta R.T. -0.005 min
Lab File: BG055557.D
Acq: 11 Nov 2022 3:09




Instrument :
BNA_G
ClientSampleId :
SB-17


Tgt Ion:188 Resp: 312347
Ion Ratio Lower Upper
188 100
94 7.5 6.4 9.6
80 9.3 7.6 11.4

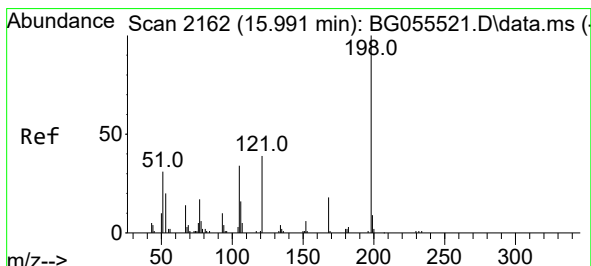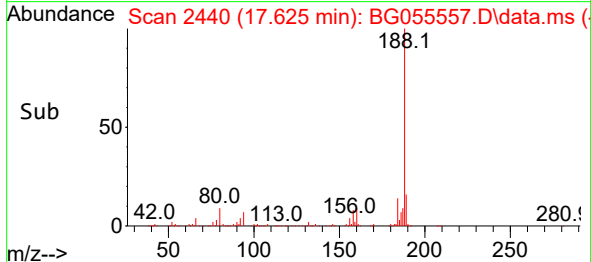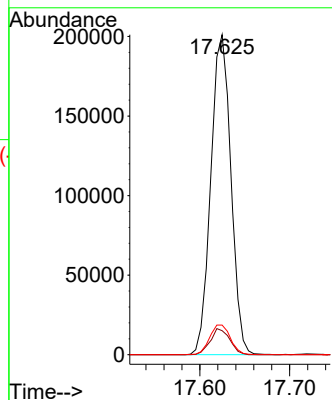

#65
4,6-Dinitro-2-methylphenol
Concen: 2.549 ng
RT: 16.362 min Scan# 2225
Delta R.T. 0.371 min
Lab File: BG055557.D
Acq: 11 Nov 2022 3:09

Tgt Ion:198 Resp: 495
Ion Ratio Lower Upper
198 100
51 101.9 24.7 64.7#
105 106.8 17.6 57.6#


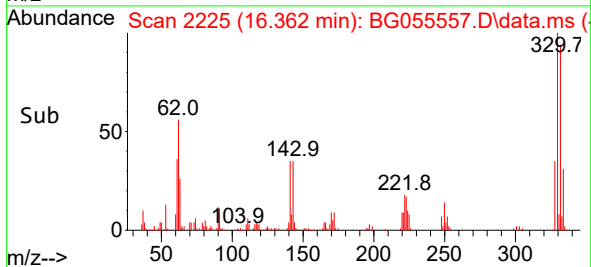
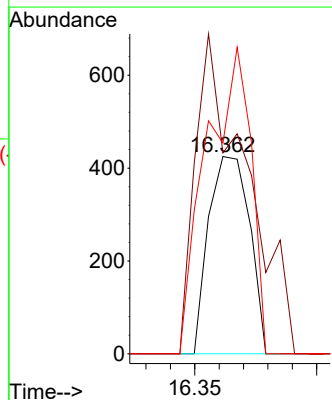
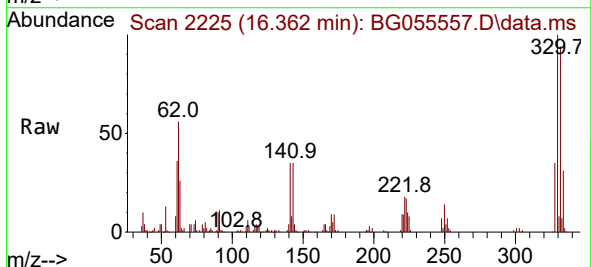


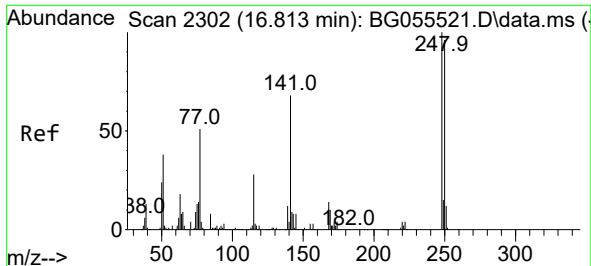

#67
4-Bromophenyl-phenylether
Concen: 3.564 ng
RT: 16.367 min Scan# 211
Delta R.T. -0.446 min
Lab File: BG055557.D
Acq: 11 Nov 2022 3:09




Instrument :
BNA_G
ClientSampleId :
SB-17


Tgt Ion:248 Resp: 11358
Ion Ratio Lower Upper
248 100
250 199.6 76.9 115.3#
141 492.1 54.3 81.5#

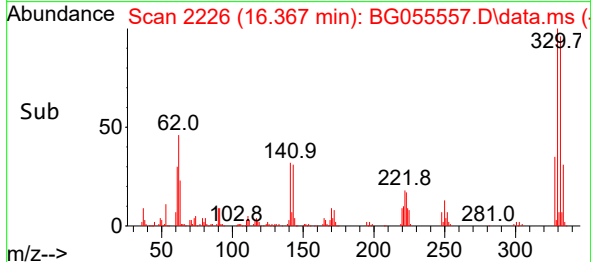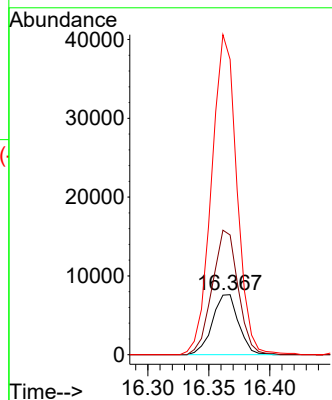

#76
Chrysene-d12
Concen: 20.000 ng
RT: 21.920 min Scan# 3171
Delta R.T. -0.011 min
Lab File: BG055557.D
Acq: 11 Nov 2022 3:09

Tgt Ion:240 Resp: 312825
Ion Ratio Lower Upper
240 100
120 9.3 6.1 9.1#
236 26.7 21.4 32.0

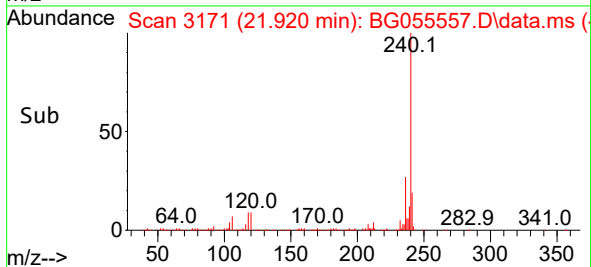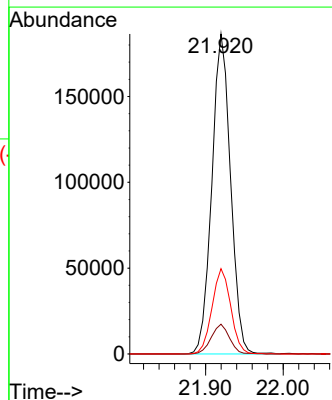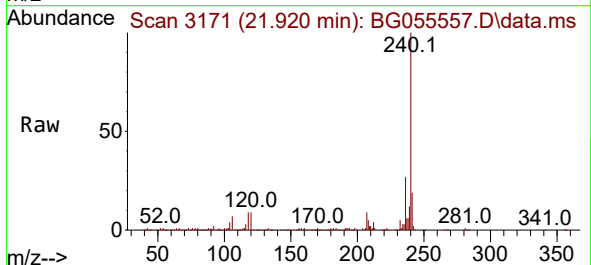



#79

Terphenyl-d14

Concen: 66.906 ng

RT: 20.210 min Scan# 21

Delta R.T. -0.005 min

Lab File: BG055557.D

Acq: 11 Nov 2022 3:09

Instrument :

BNA_G

ClientSampleId :

SB-17





Tgt Ion:244 Resp: 1042030

Ion Ratio Lower Upper

244 100

212 7.6 6.5 9.7

122 9.8 7.7 11.5

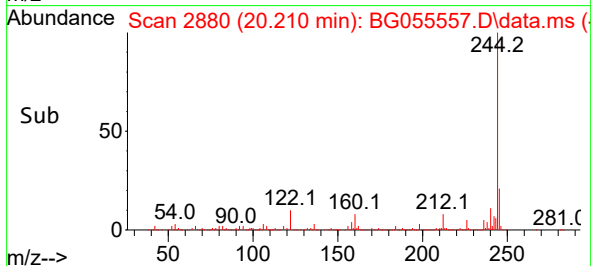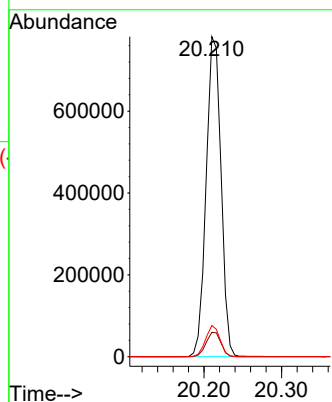

#80

Butylbenzylphthalate

Concen: 3.449 ng

RT: 20.892 min Scan# 2996

Delta R.T. -0.011 min

Lab File: BG055557.D

Acq: 11 Nov 2022 3:09




Tgt Ion:149 Resp: 732


Ion Ratio Lower Upper

149 100

91 36.2 56.8 85.2#

206 41.6 17.3 25.9#

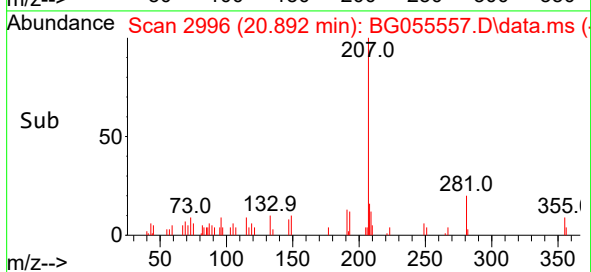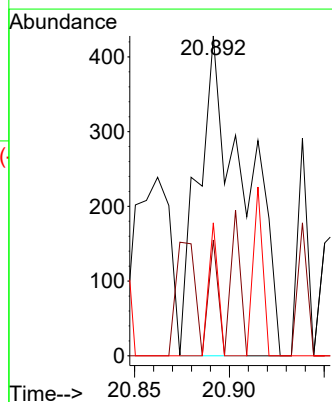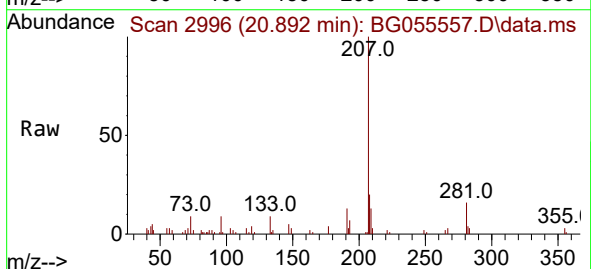



#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 25.339 min Scan# 31
 Delta R.T. -0.011 min
 Lab File: BG055557.D
 Acq: 11 Nov 2022 3:09

Instrument :
 BNA_G
 ClientSampleId :
 SB-17

Tgt Ion:264 Resp: 324704
 Ion Ratio Lower Upper
 264 100
 260 23.4 19.4 29.2
 265 22.5 17.1 25.7

