
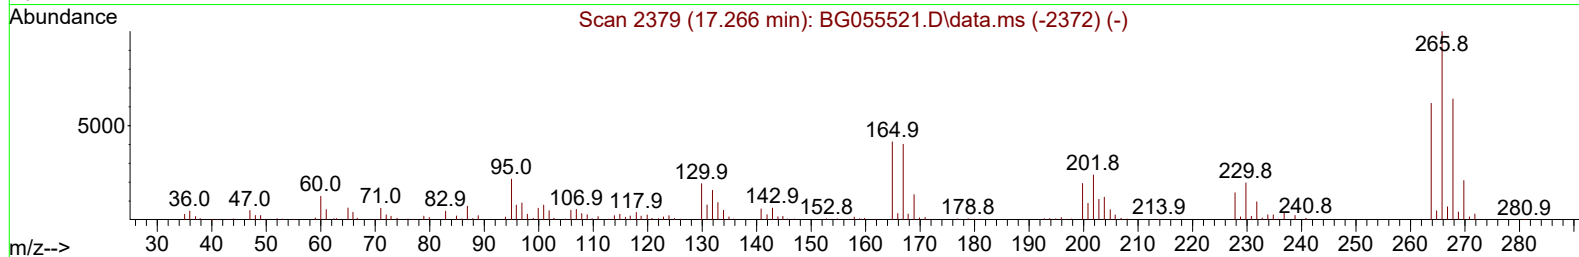
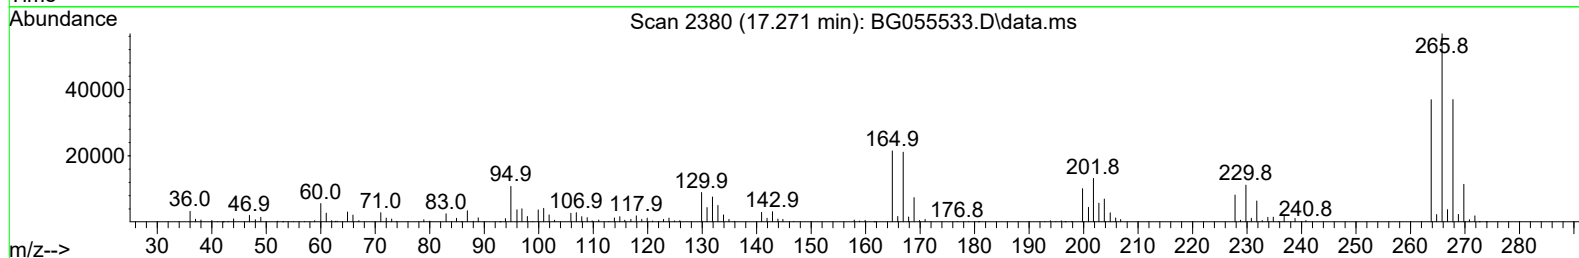


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111022\
Data File : BG055533.D
Acq On : 10 Nov 2022 10:21
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 11 04:58:32 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG110922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 10 03:39:46 2022
Response via : Initial Calibration

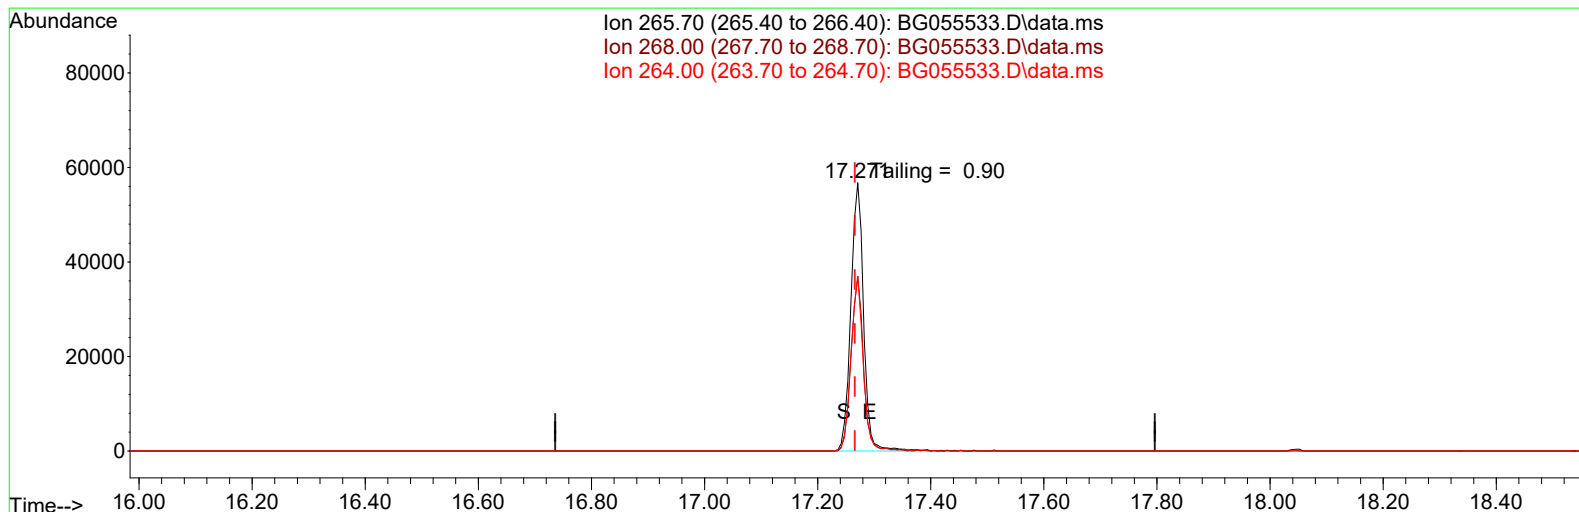

TIC: BG055533.D\data.ms

(70) Pentachlorophenol (C)




17.271min (+ 0.005) 17168.58 ng

response 89095

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.20	65.11
264.00	61.90	65.05
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111022\
Data File : BG055533.D
Acq On : 10 Nov 2022 10:21
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 11 04:58:32 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG110922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 10 03:39:46 2022
Response via : Initial Calibration

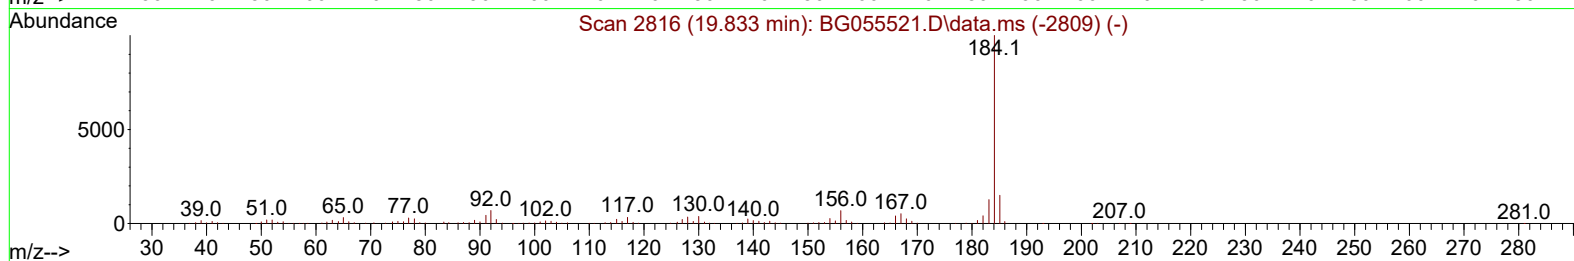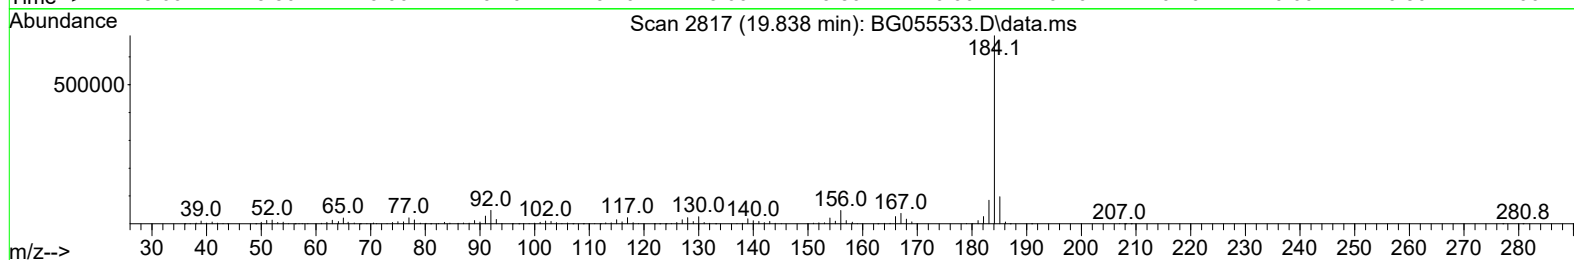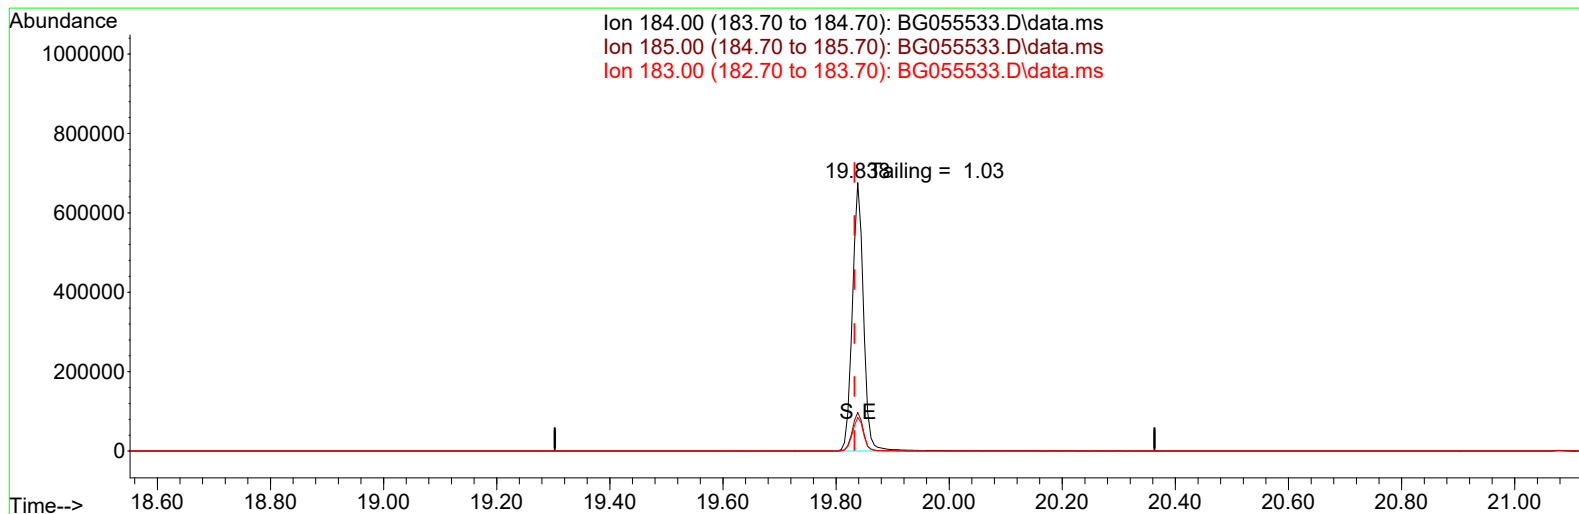

TIC: BG055533.D\data.ms

(77) Benzidine

19.838min (+ 0.005) 0.00 ng

response 931044

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.00	14.38
183.00	12.70	12.55
0.00	0.00	0.00