
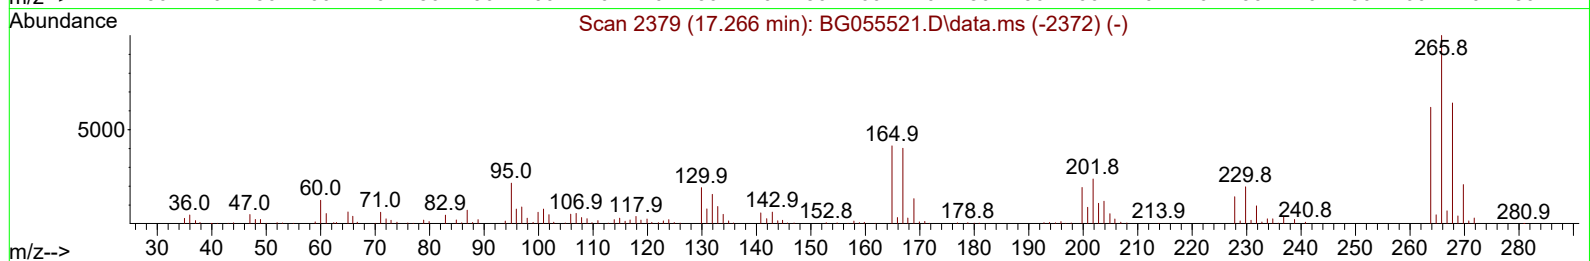
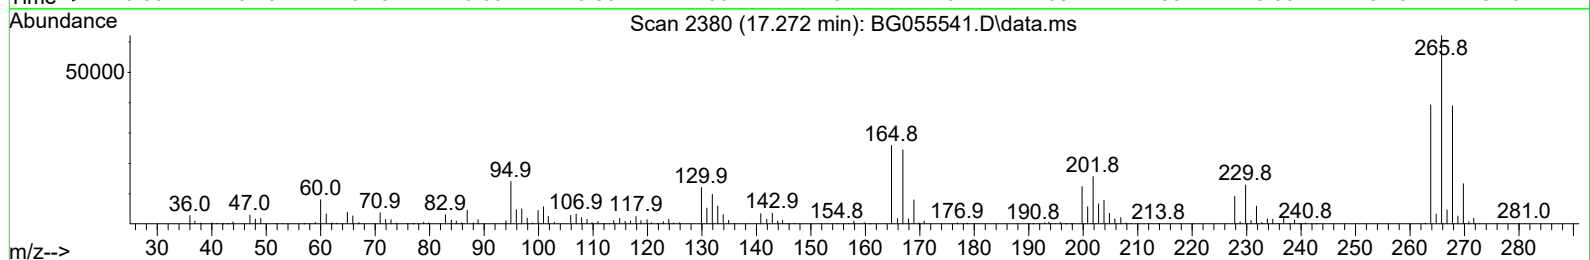


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111022\
Data File : BG055541.D
Acq On : 10 Nov 2022 16:01
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 10 16:36:13 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG110922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 10 03:39:46 2022
Response via : Initial Calibration

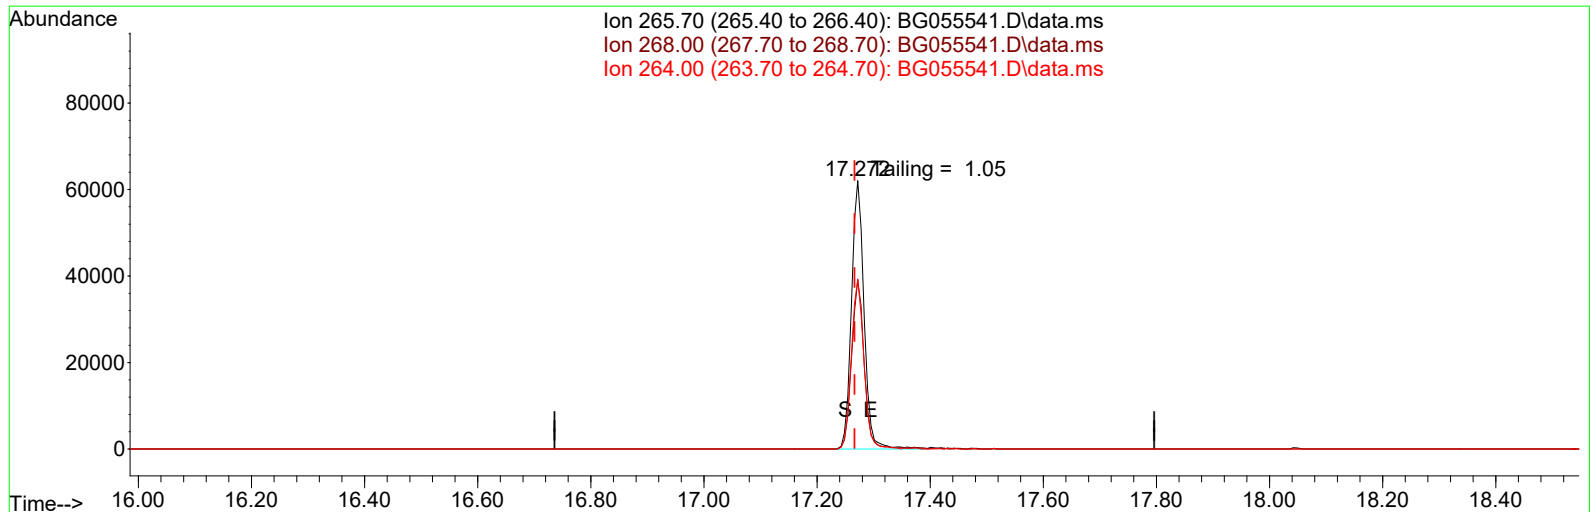

TIC: BG055541.D\data.ms

(70) Pentachlorophenol (C)




17.272min (+ 0.006) 25960.17 ng

response 95217

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.20	62.83
264.00	61.90	63.35
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111022\
Data File : BG055541.D
Acq On : 10 Nov 2022 16:01
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 10 16:36:13 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG110922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 10 03:39:46 2022
Response via : Initial Calibration

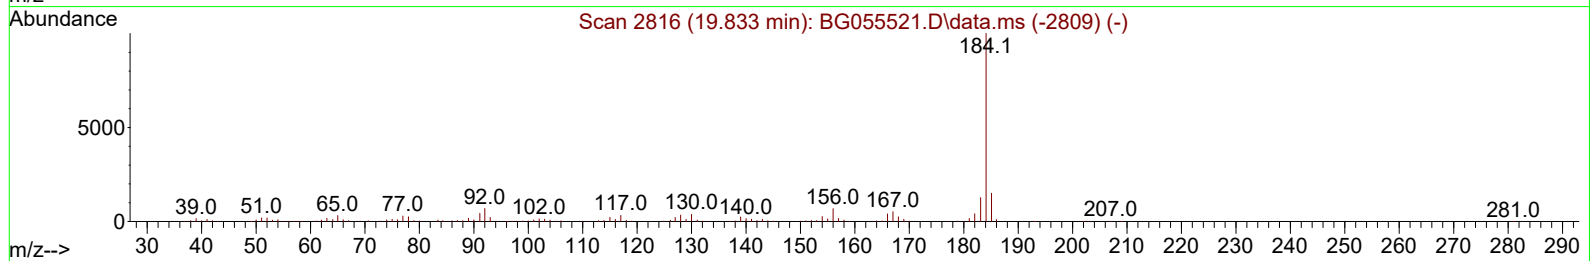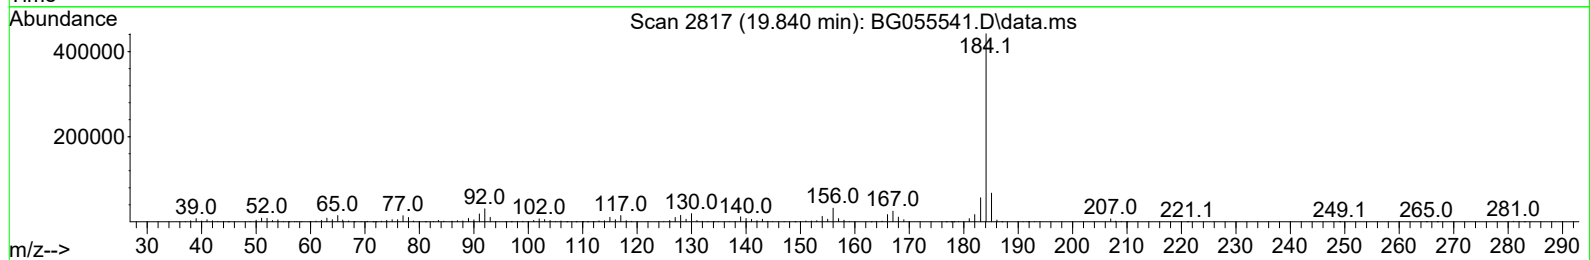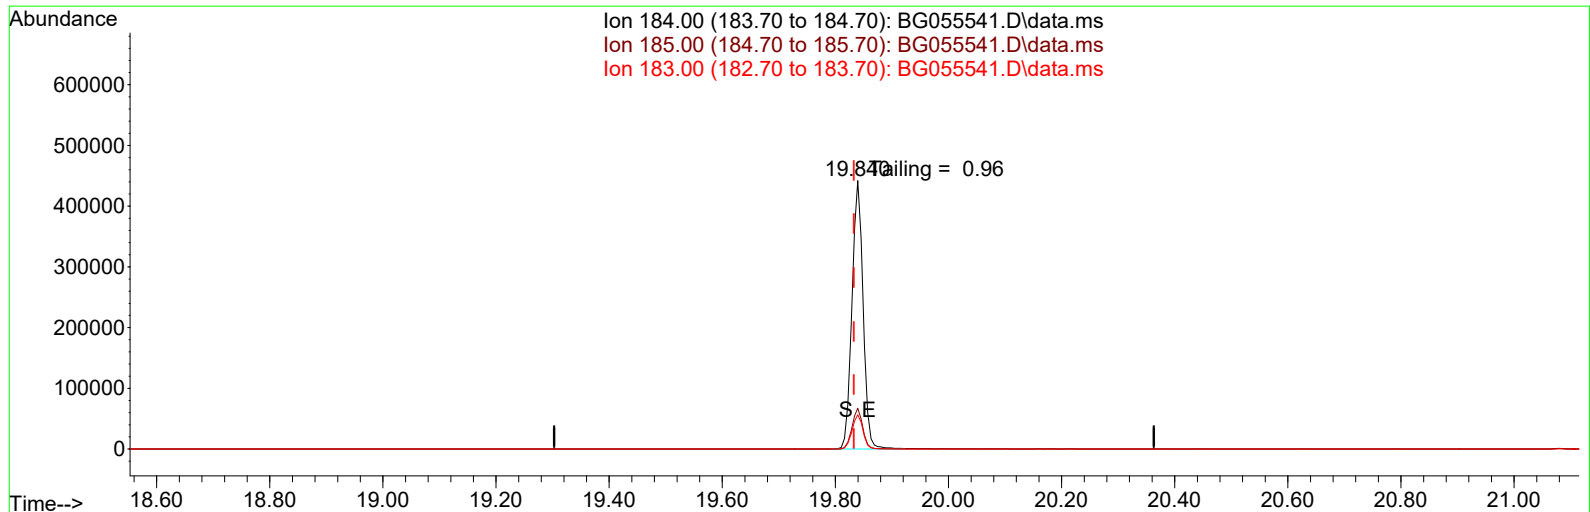

TIC: BG055541.D\data.ms

(77) Benzidine

19.840min (+ 0.007) 0.00 ng

response 609062

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.00	15.23
183.00	12.70	12.76
0.00	0.00	0.00