
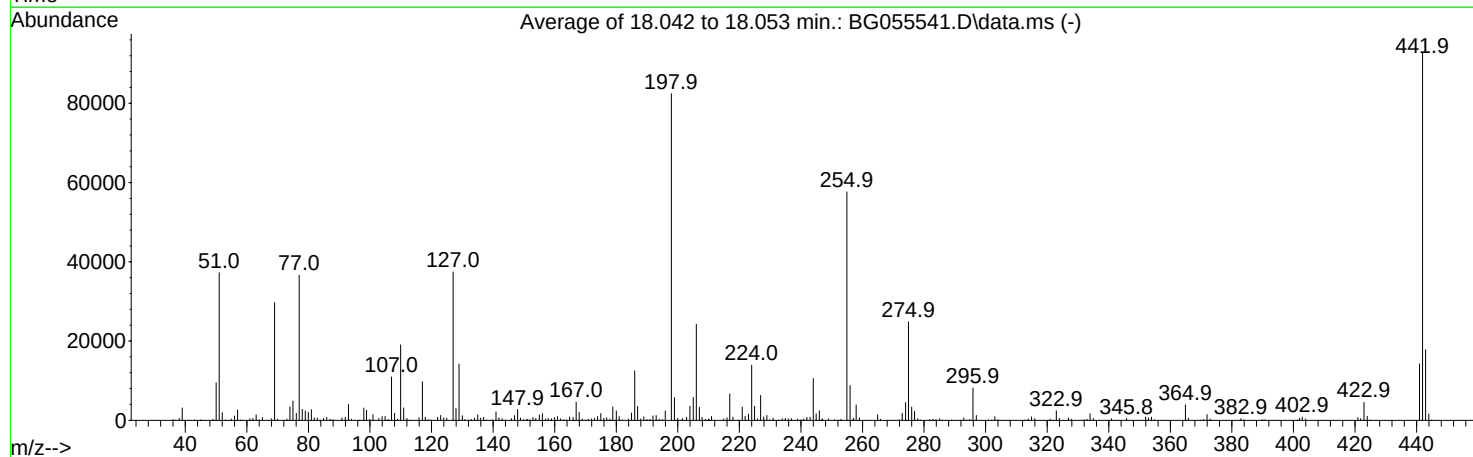


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111022\
Data File : BG055541.D
Acq On : 10 Nov 2022 16:01
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG110922.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Nov 10 03:39:46 2022

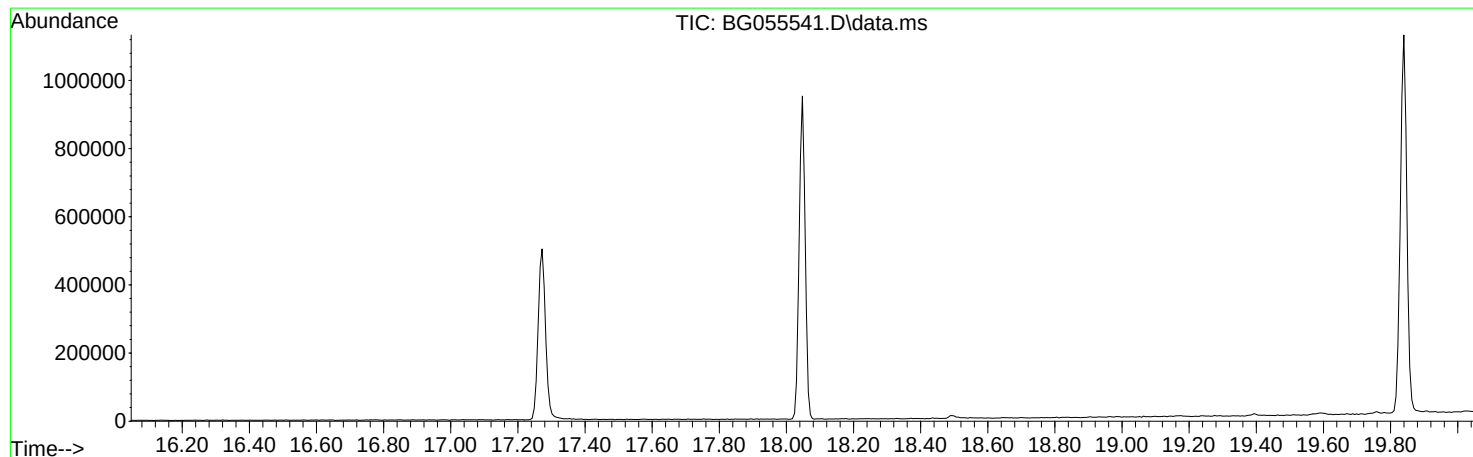




AutoFind: Scans 2511, 2512, 2513; Background Corrected with Scan 2504

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	45.2	37243	PASS
68	69	0.00	2	1.3	400	PASS
69	198	0.00	100	36.0	29685	PASS
70	69	0.00	2	1.0	284	PASS
127	198	10	80	45.4	37435	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	82459	PASS
199	198	5	9	7.0	5760	PASS
275	198	10	60	30.1	24803	PASS
365	198	1	100	4.7	3910	PASS
441	198	0.01	100	17.2	14222	PASS
442	442	50	100	100.0	92835	PASS
443	442	15	24	19.2	17799	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111022\
Data File : BG055541.D
Acq On : 10 Nov 2022 16:01
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Nov 10 16:36:13 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG110922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 10 03:39:46 2022
Response via : Initial Calibration

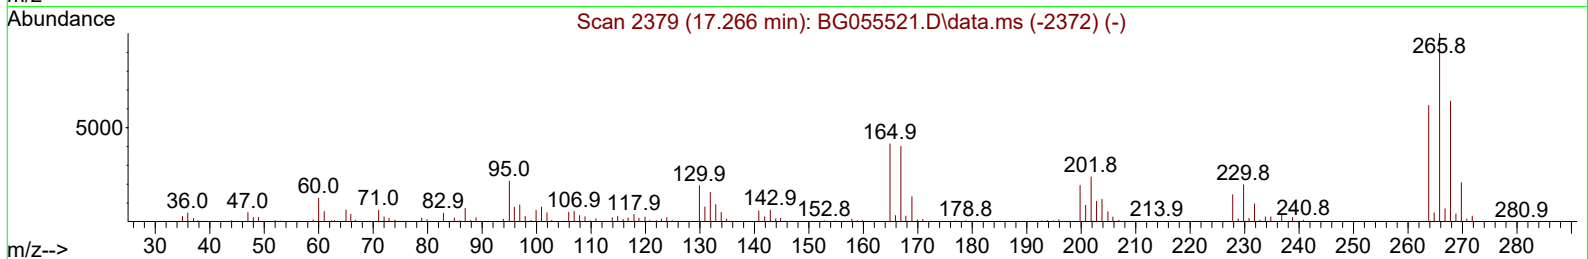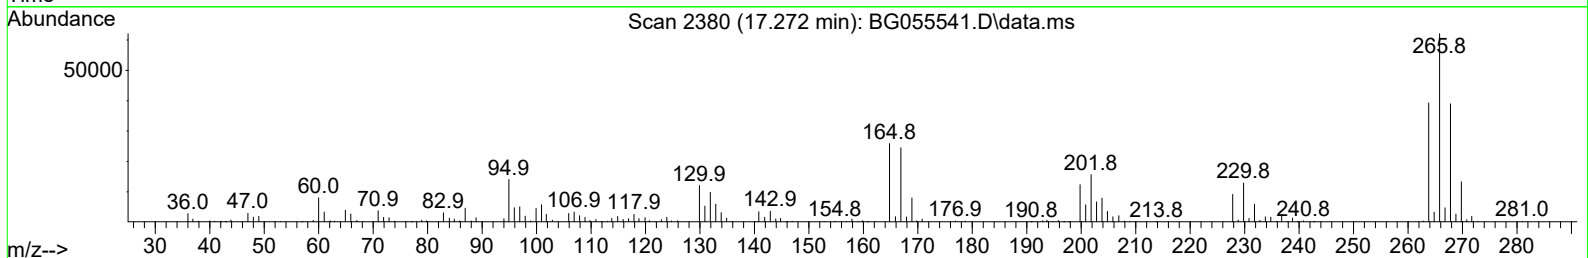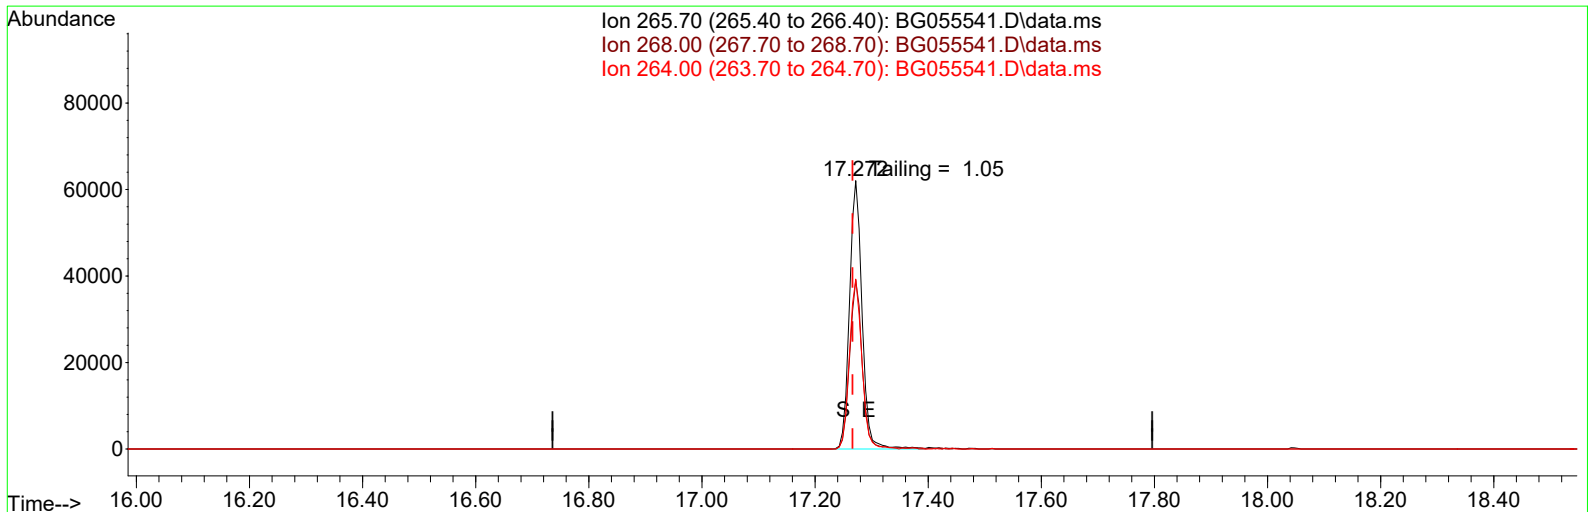

TIC: BG055541.D\data.ms

(70) Pentachlorophenol (C)

17.272min (+ 0.006) 25960.17 ng




response 95217

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.20	62.83
264.00	61.90	63.35
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111022\
Data File : BG055541.D
Acq On : 10 Nov 2022 16:01
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Nov 10 16:36:13 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG110922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 10 03:39:46 2022
Response via : Initial Calibration

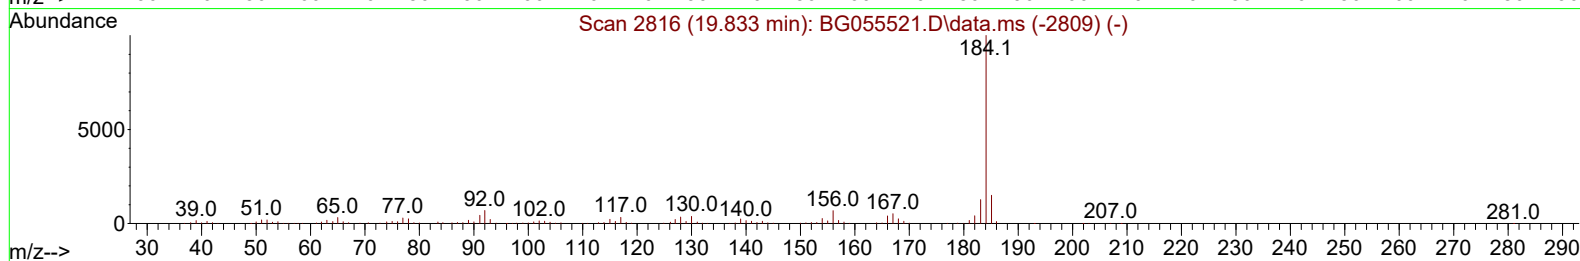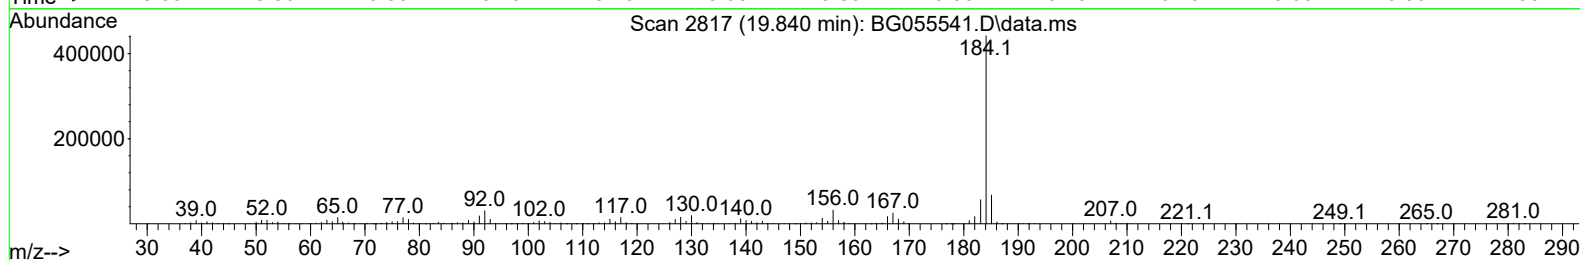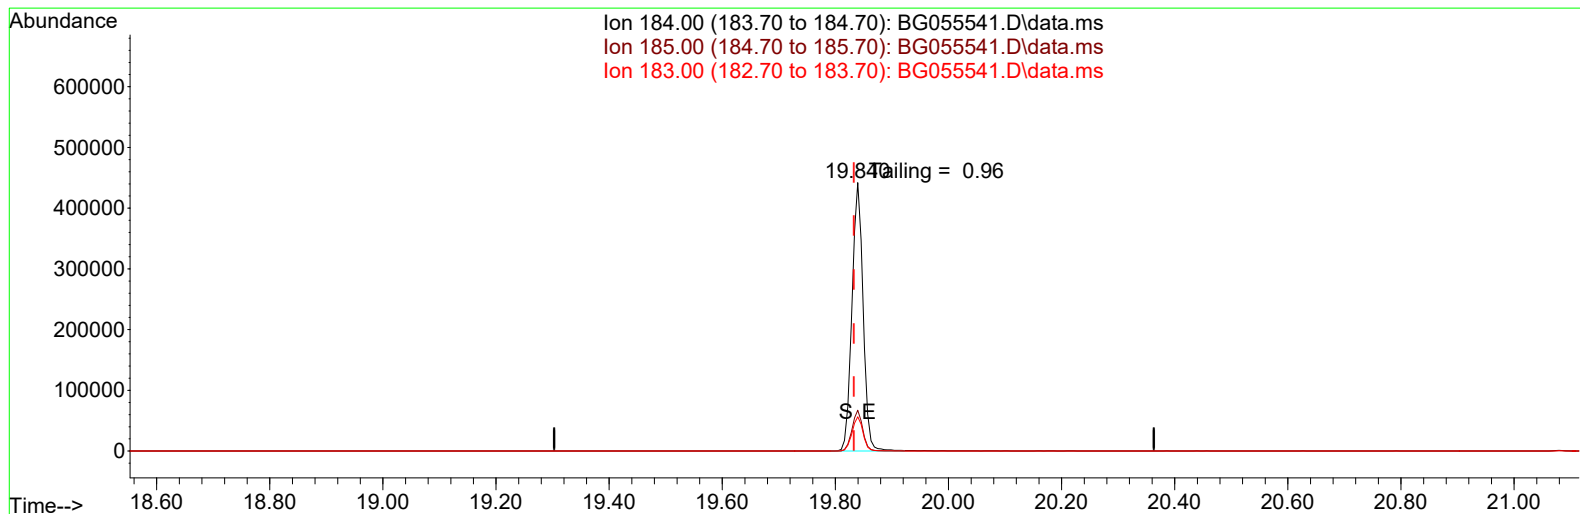

TIC: BG055541.D\data.ms

(77) Benzidine

19.840min (+ 0.007) 0.00 ng

response 609062

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.00	15.23
183.00	12.70	12.76
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/10/2022	BNA_G	<u>BG055541.D</u>
Compound Name	Response	Retention Time
DDT	246956	21.079
DDD	12671	20.621
DDE	329	20.128
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
13000	259956	5.00

Instrument :
BNA_G
ClientSampleId :
DFTPP