


Data Path : \\74.0.250.170\svoasrv\HPCHEM1\BNA G\Data\BG111117\
 Data File : BG030931.D
 Acq On : 11 Nov 2017 7:07
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG111017.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Nov 10 15:38:25 2017

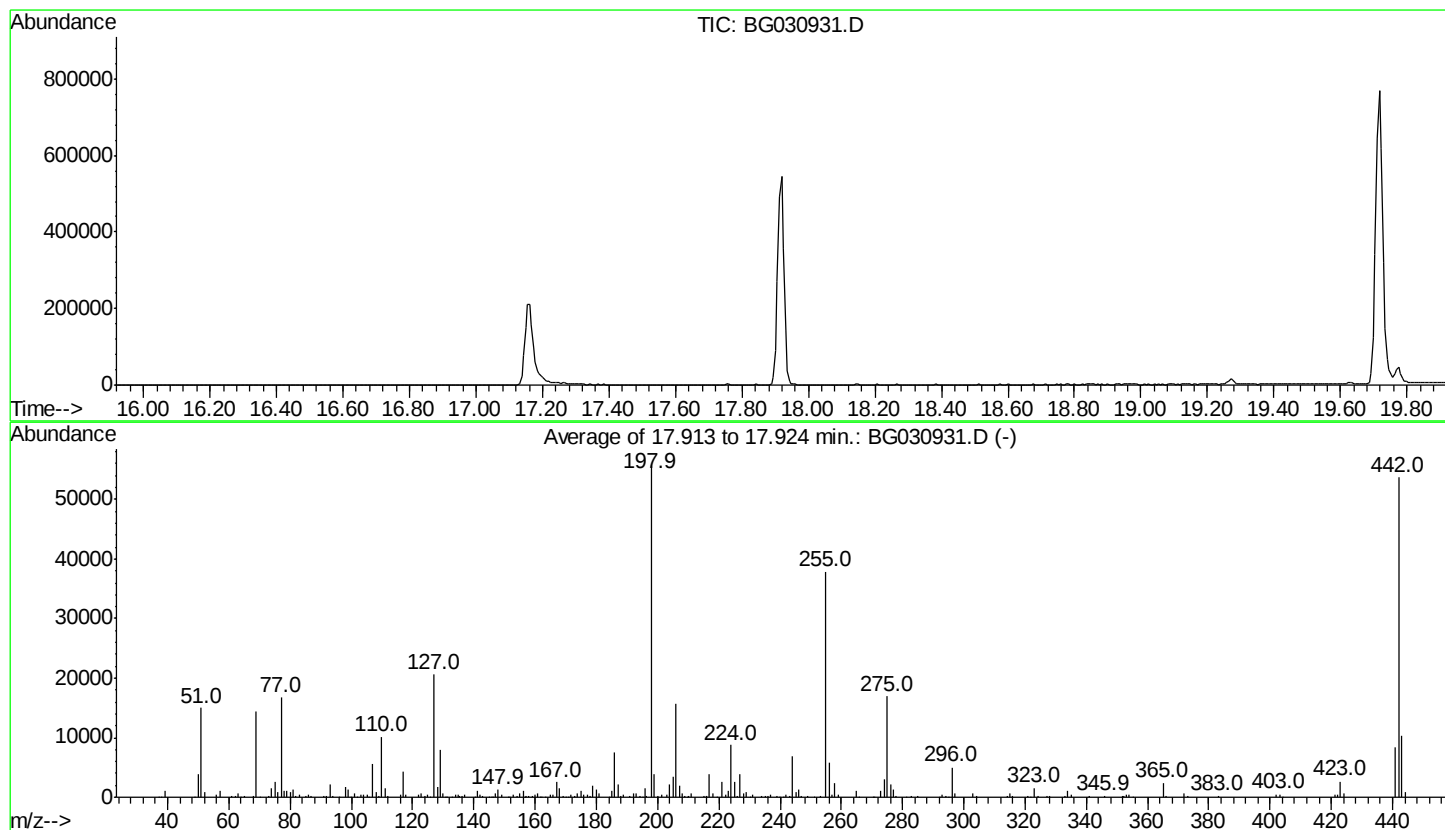

AutoFind: Scans 2489, 2490, 2491; Background Corrected with Scan 2482

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	26.9	14951	PASS
68	69	0.00	2	1.6	236	PASS
69	198	0.00	100	26.0	14477	PASS
70	69	0.00	2	0.4	54	PASS
127	198	10	80	36.9	20556	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	55674	PASS
199	198	5	9	7.0	3896	PASS
275	198	10	60	30.5	16969	PASS
365	198	1	100	4.3	2379	PASS
441	442	0.01	24	15.8	8484	PASS
442	198	50	100	96.4	53688	PASS
443	442	15	24	19.2	10334	PASS