
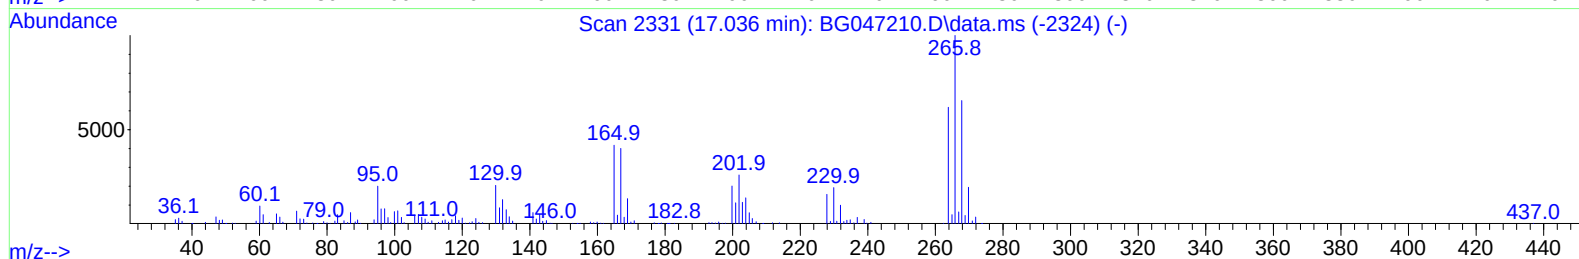
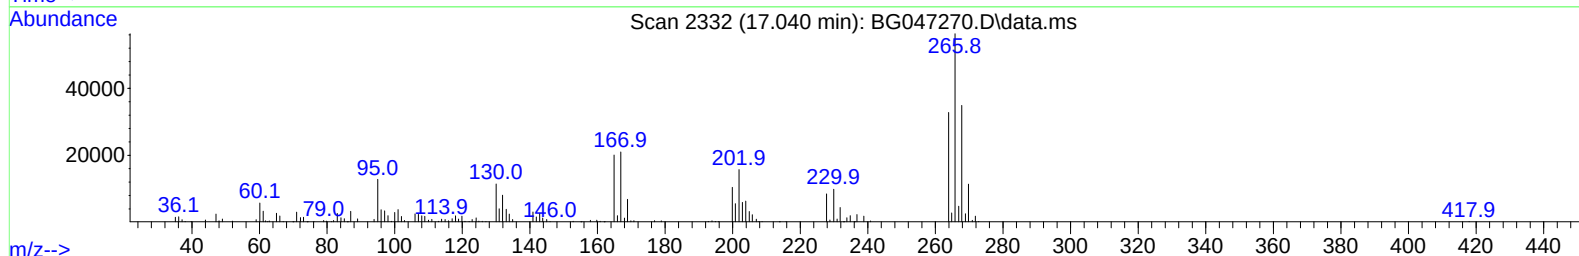


Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG111120\  
Data File : BG047270.D  
Acq On : 10 Nov 2020 15:40  
Operator : CG/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 11 04:02:39 2020  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_G\METHODS\8270-BG110420.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Wed Nov 04 16:19:40 2020  
Response via : Initial Calibration

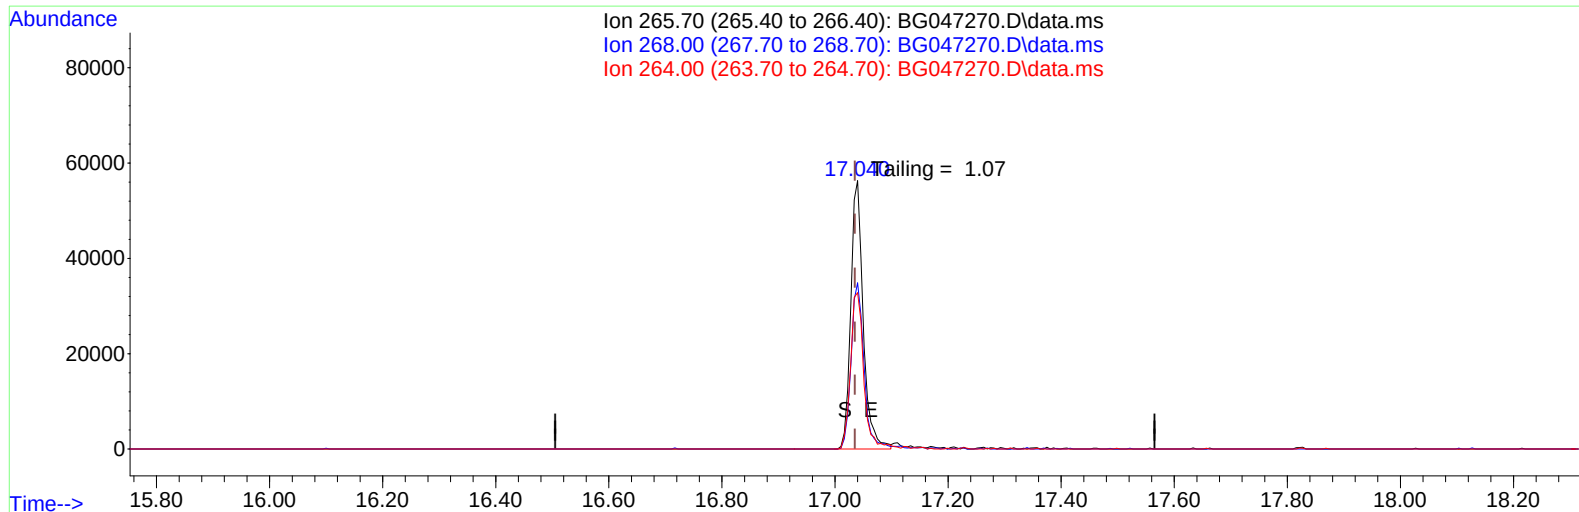

TIC: BG047270.D\data.ms

**(70) Pentachlorophenol (C)**




17.040min (+ 0.004) 25219.03 ng

response 85920

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 62.20  | 61.98  |
| 264.00 | 61.60  | 58.28  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG111120\  
Data File : BG047270.D  
Acq On : 10 Nov 2020 15:40  
Operator : CG/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 11 04:02:39 2020  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_G\METHODS\8270-BG110420.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Wed Nov 04 16:19:40 2020  
Response via : Initial Calibration

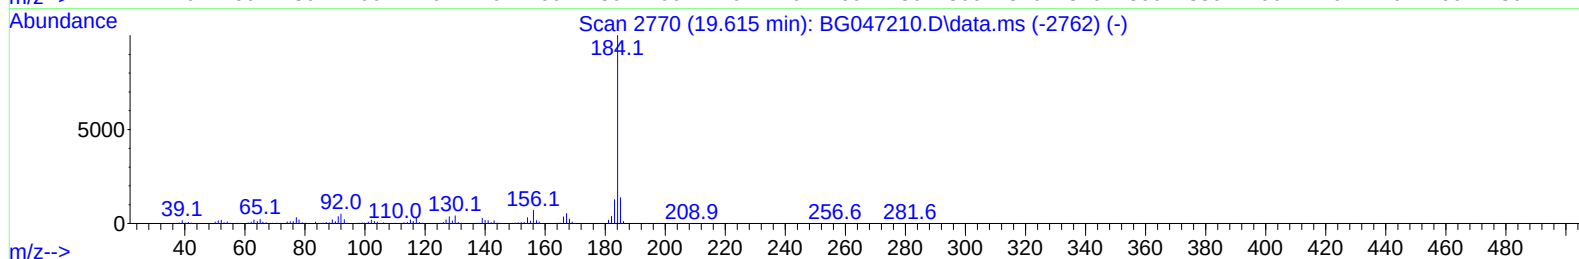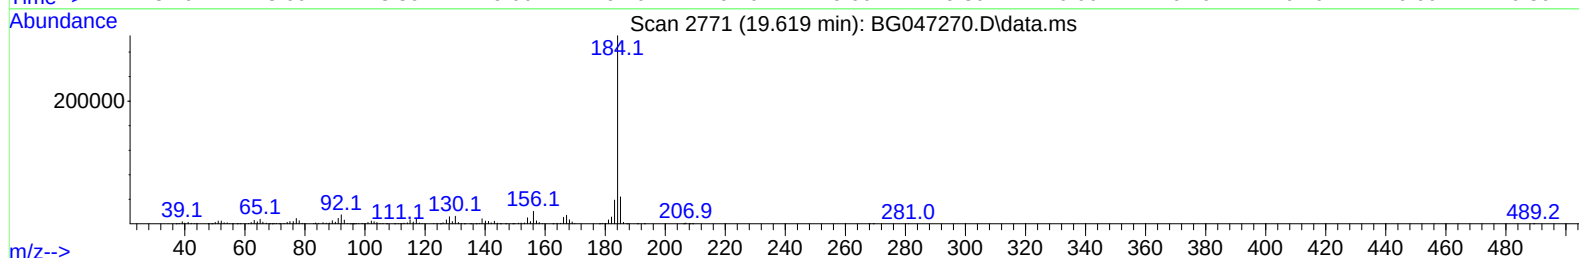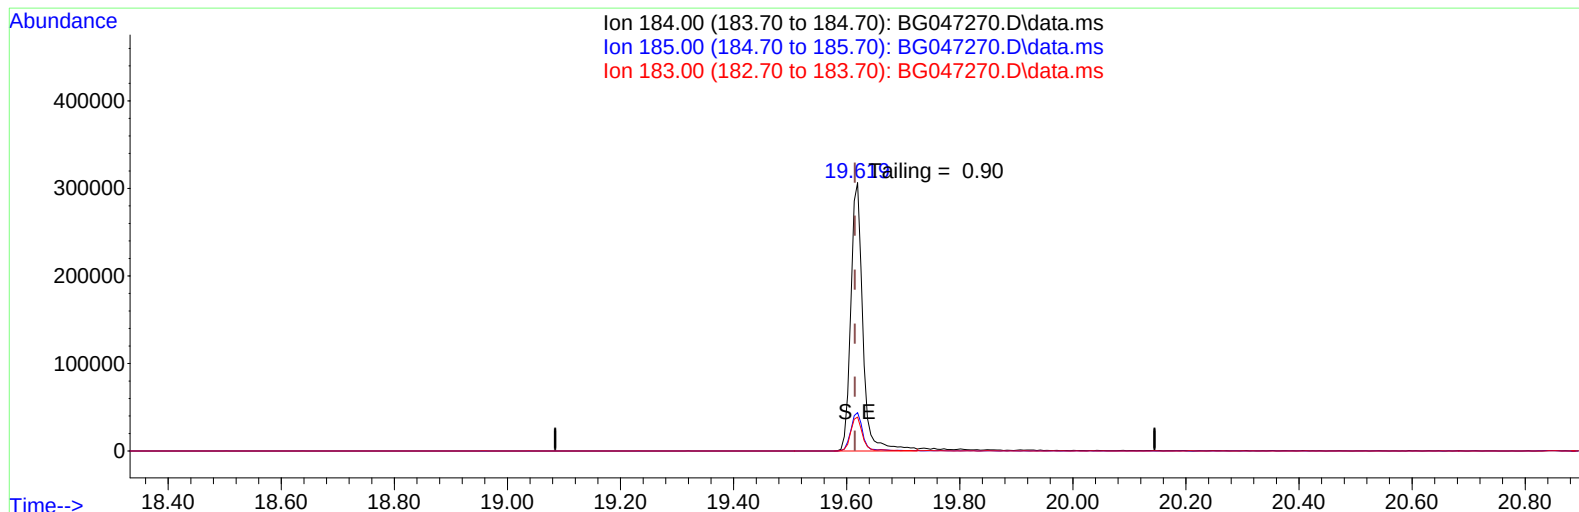

TIC: BG047270.D\data.ms

**(77) Benzidine****19.619min (+ 0.004) 218377.27 ng****response 454092**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 15.50  | 14.33  |
| 183.00 | 13.20  | 12.67  |
| 0.00   | 0.00   | 0.00   |