
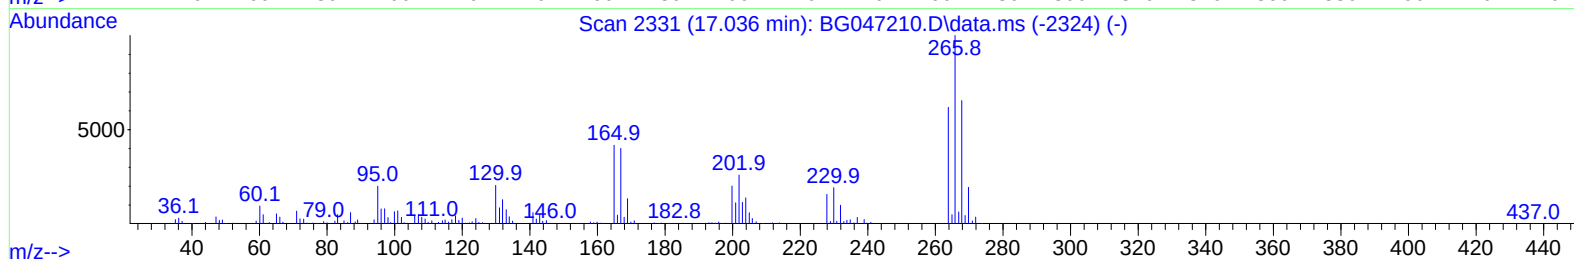
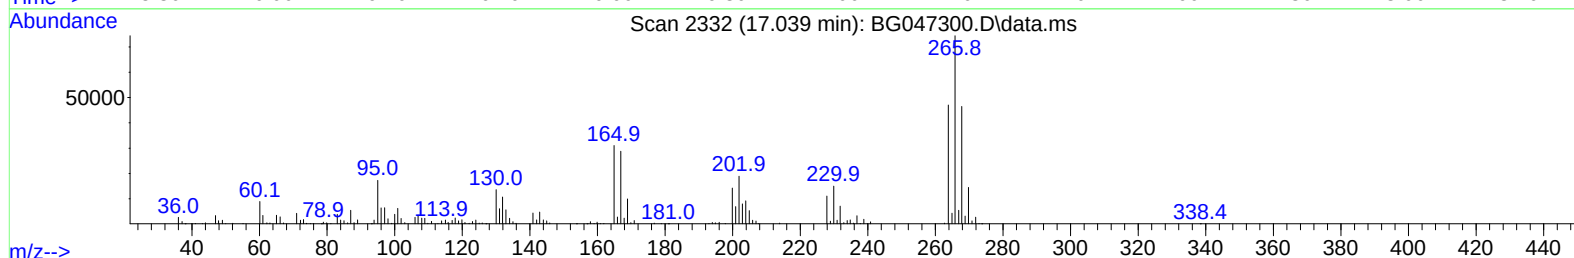


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111120\
Data File : BG047300.D
Acq On : 12 Nov 2020 2:51
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 12 05:26:54 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG110420.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 04 16:19:40 2020
Response via : Initial Calibration

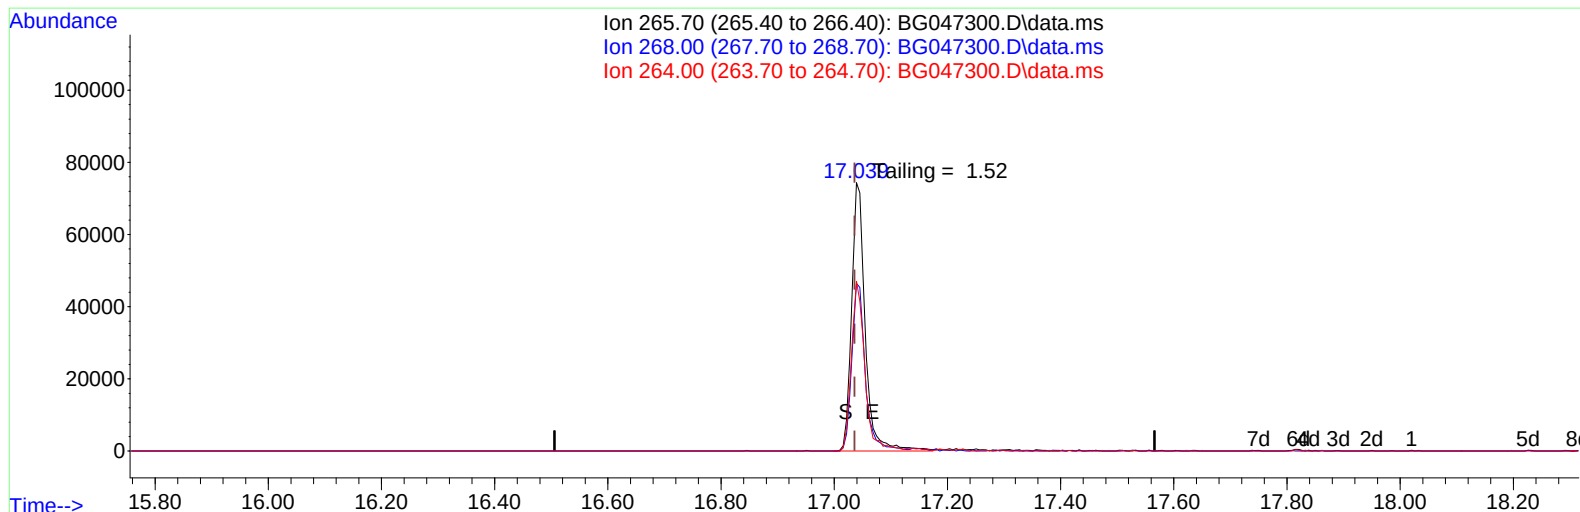

TIC: BG047300.D\data.ms

(70) Pentachlorophenol (C)




17.039min (+ 0.004) 239721.46 ng m

response 126869

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	62.48
264.00	61.60	63.21
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111120\
Data File : BG047300.D
Acq On : 12 Nov 2020 2:51
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 12 05:26:54 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG110420.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 04 16:19:40 2020
Response via : Initial Calibration

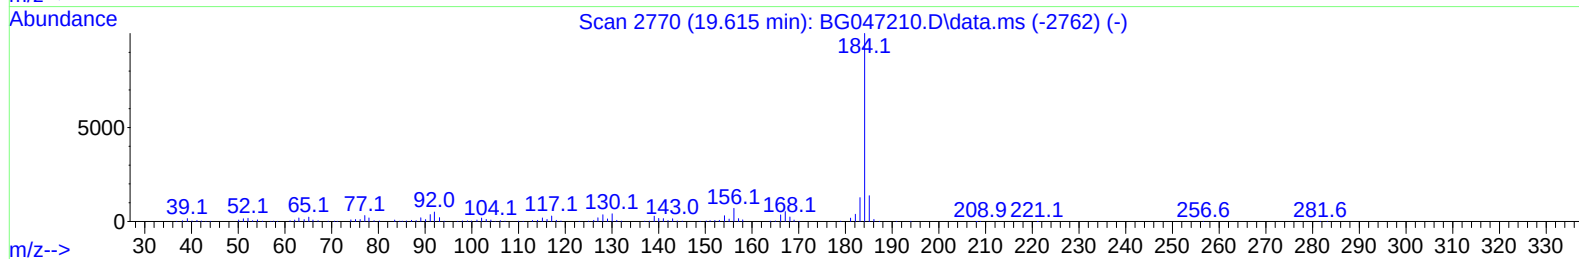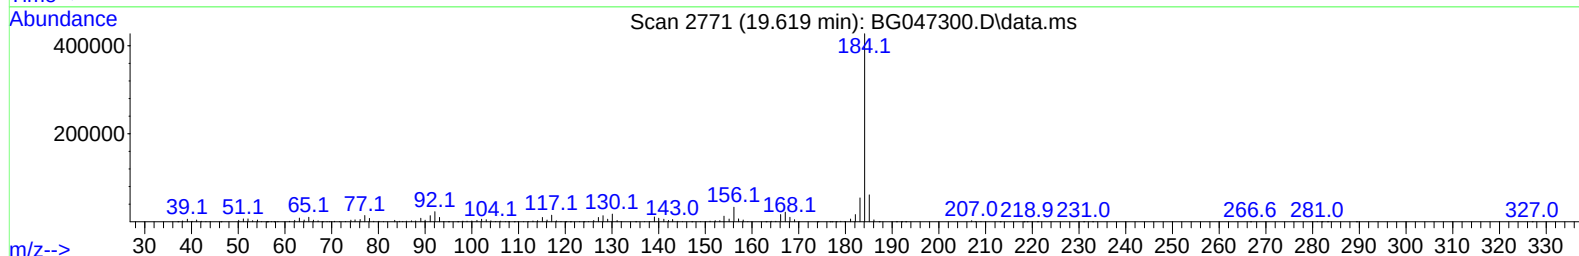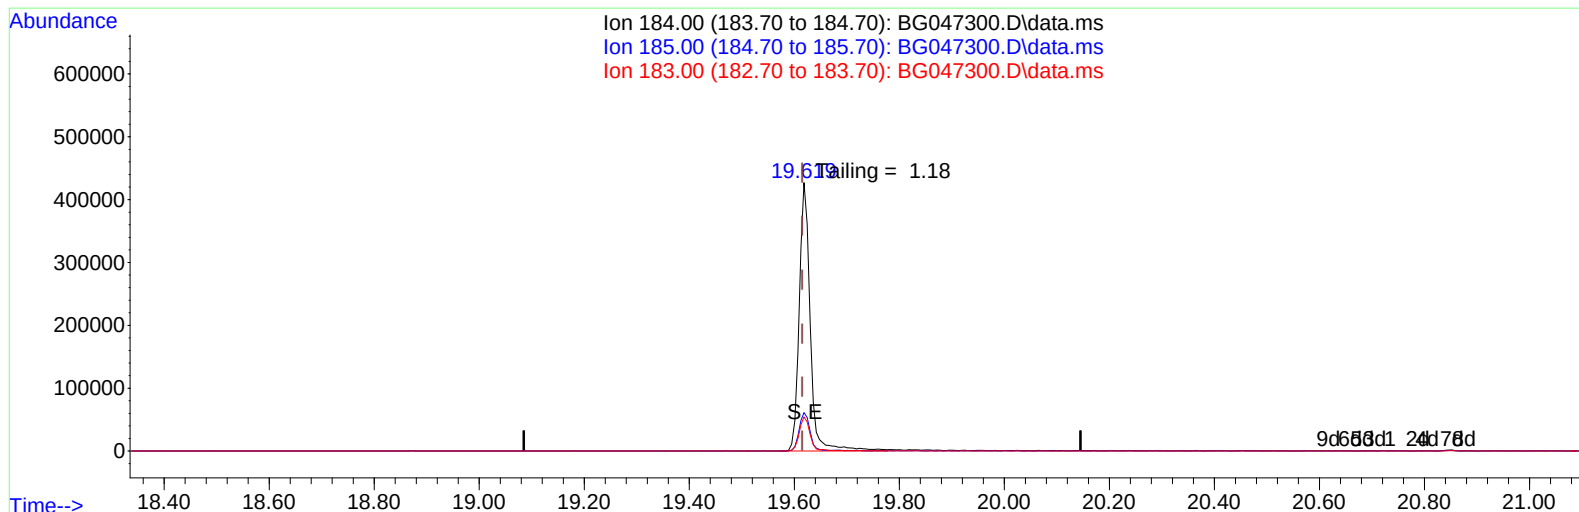

TIC: BG047300.D\data.ms

(77) Benzidine

19.619min (+ 0.004) 156428.98 ng m

response 645308

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.31
183.00	13.20	12.71
0.00	0.00	0.00