

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111120\
 Data File : BG047277.D
 Acq On : 10 Nov 2020 20:24
 Operator : CG/JU
 Sample : L4680-05
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 PAV-B7-110920-10-20

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG110420.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG047277.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.565	372	379	389	rBV	817608	1268559	39.83%	6.845%
2	7.163	644	651	664	rBV	868194	1462475	45.91%	7.891%
3	7.586	714	723	734	rBV2	38944	67023	2.10%	0.362%
4	8.009	787	795	802	rBV	237689	409695	12.86%	2.211%
5	9.167	985	992	1000	rBV	532792	928195	29.14%	5.008%
6	10.818	1266	1273	1284	rBV	326795	574300	18.03%	3.099%
7	13.262	1680	1689	1697	rBV	1420645	2153340	67.60%	11.619%
8	13.526	1728	1734	1741	rBV3	30724	41401	1.30%	0.223%
9	14.084	1824	1829	1839	rBV	249602	365989	11.49%	1.975%
10	14.643	1917	1924	1932	rBV	576906	875690	27.49%	4.725%
11	16.129	2170	2177	2188	rBV	1283059	1924217	60.41%	10.383%
12	17.386	2384	2391	2396	rBV	717643	1107166	34.76%	5.974%
13	17.428	2396	2398	2403	rVB2	59899	70276	2.21%	0.379%
14	18.268	2535	2541	2546	rBV3	198707	286821	9.00%	1.548%
15	18.450	2567	2572	2577	rBV5	16995	36629	1.15%	0.198%
16	19.178	2691	2696	2699	rBV5	23112	40806	1.28%	0.220%
17	19.214	2699	2702	2709	rVB8	37418	48609	1.53%	0.262%
18	19.437	2735	2740	2745	rVB	119417	171509	5.38%	0.925%
19	19.537	2752	2757	2765	rBV5	67805	106854	3.35%	0.577%
20	19.678	2776	2781	2786	rVB4	28759	49818	1.56%	0.269%
21	19.766	2792	2796	2797	rBV	30581	33699	1.06%	0.182%
22	19.795	2797	2801	2809	rVB	104251	167729	5.27%	0.905%
23	19.995	2829	2835	2841	rBV	2475145	3185195	100.00%	17.187%
24	20.289	2881	2885	2891	rVB6	24376	41418	1.30%	0.223%
25	20.671	2946	2950	2954	rVB	135960	156797	4.92%	0.846%
26	21.288	3049	3055	3066	rBV4	162529	383239	12.03%	2.068%
27	21.646	3108	3116	3121	rBV2	710508	1213163	38.09%	6.546%
28	23.826	3480	3487	3495	rBV4	31244	105257	3.30%	0.568%
29	24.537	3604	3608	3615	rVB4	18390	40016	1.26%	0.216%
30	24.678	3626	3632	3633	rBV	26966	37348	1.17%	0.202%
31	24.842	3649	3660	3669	rBV	416849	1179441	37.03%	6.364%




Sum of corrected areas: 18532674

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111120\
Data File : BG047277.D
Acq On : 10 Nov 2020 20:24
Operator : CG/JU
Sample : L4680-05
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PAV-B7-110920-10-20

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG110420.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

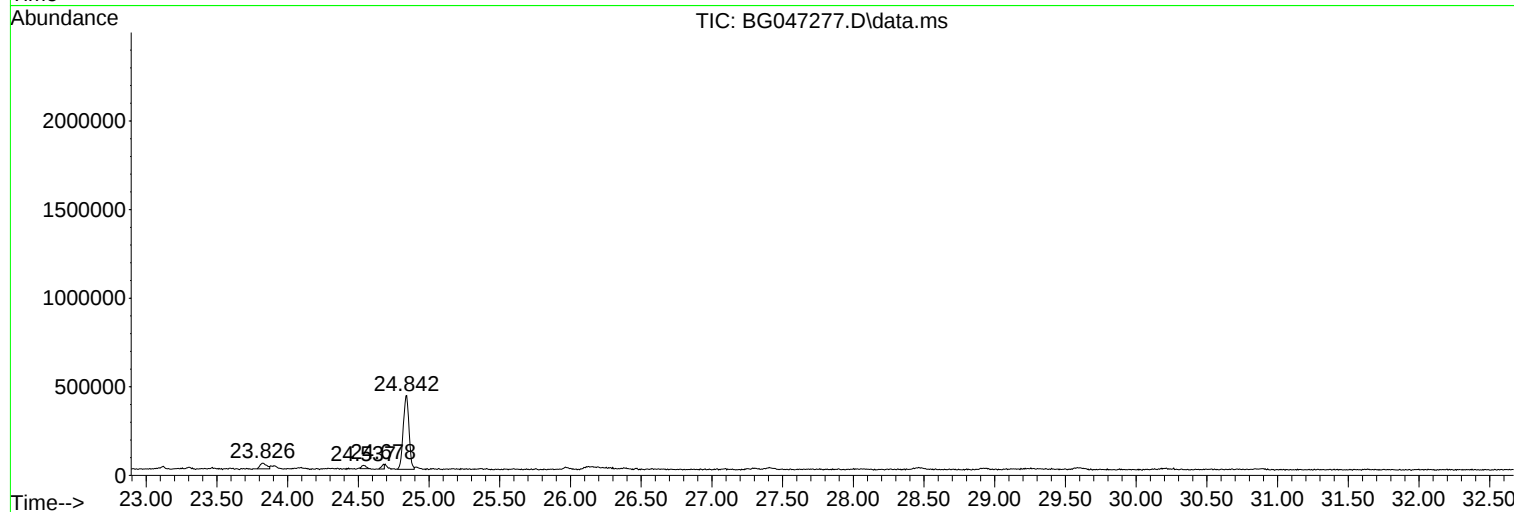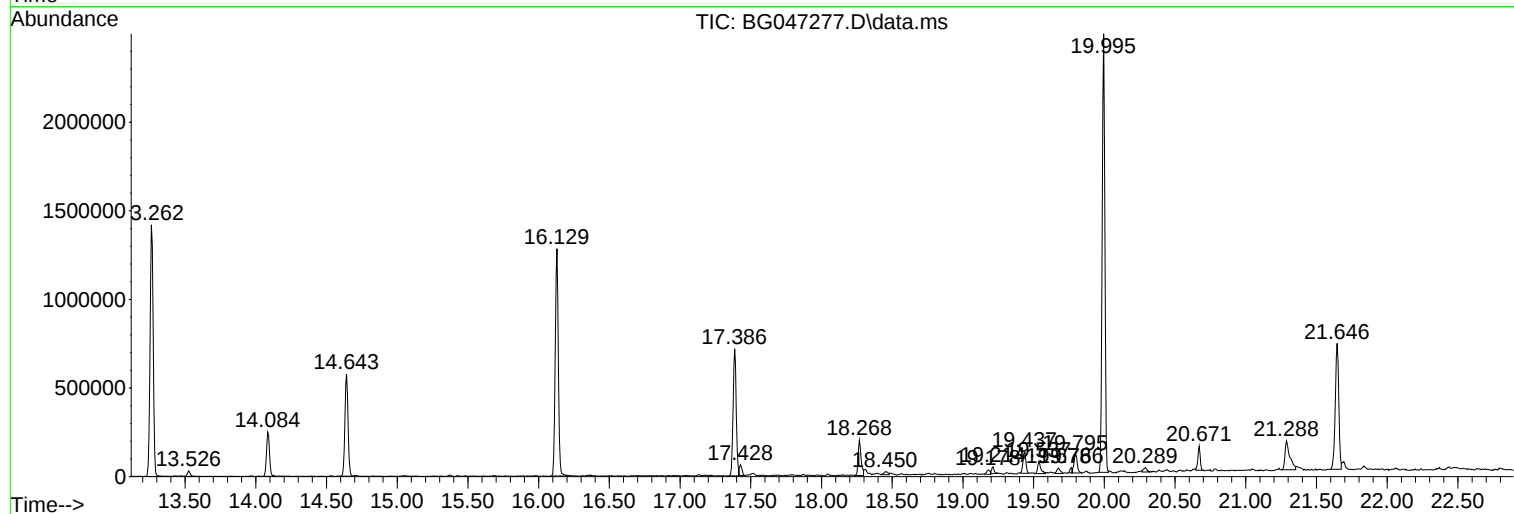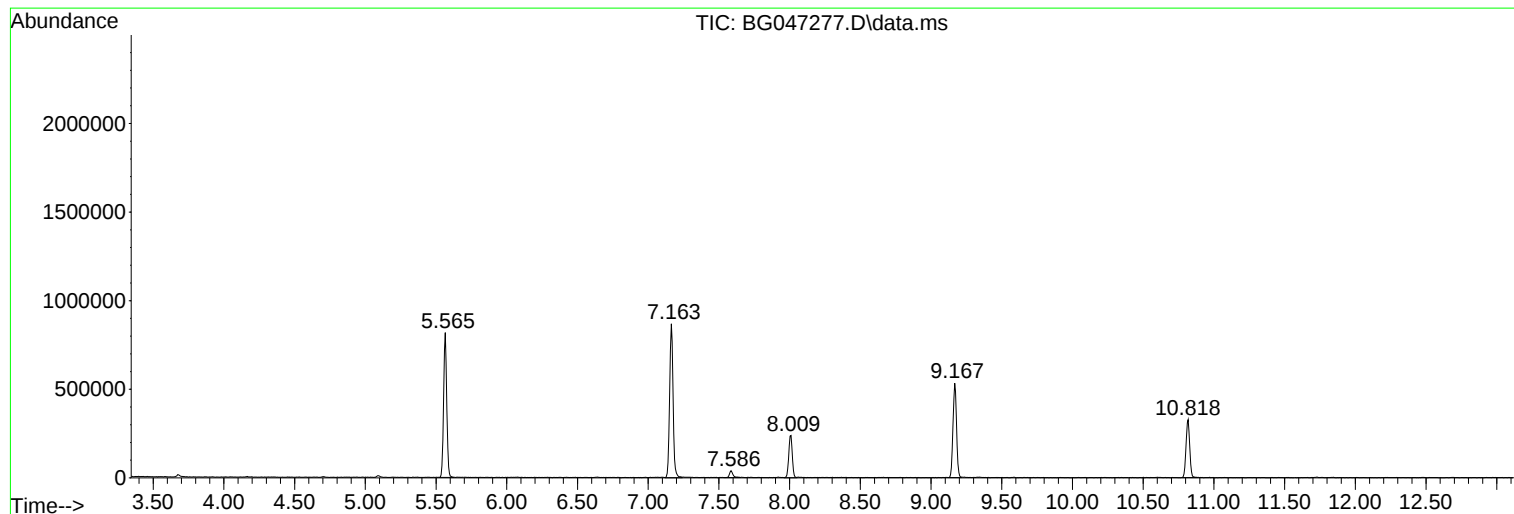

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111120\
Data File : BG047277.D
Acq On : 10 Nov 2020 20:24
Operator : CG/JU
Sample : L4680-05
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PAV-B7-110920-10-20

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG110420.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111120\
Data File : BG047277.D
Acq On : 10 Nov 2020 20:24
Operator : CG/JU
Sample : L4680-05
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PAV-B7-110920-10-20

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG110420.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------