


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111120\
 Data File : BG047270.D
 Acq On : 10 Nov 2020 15:40
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG110420.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Nov 04 16:19:40 2020

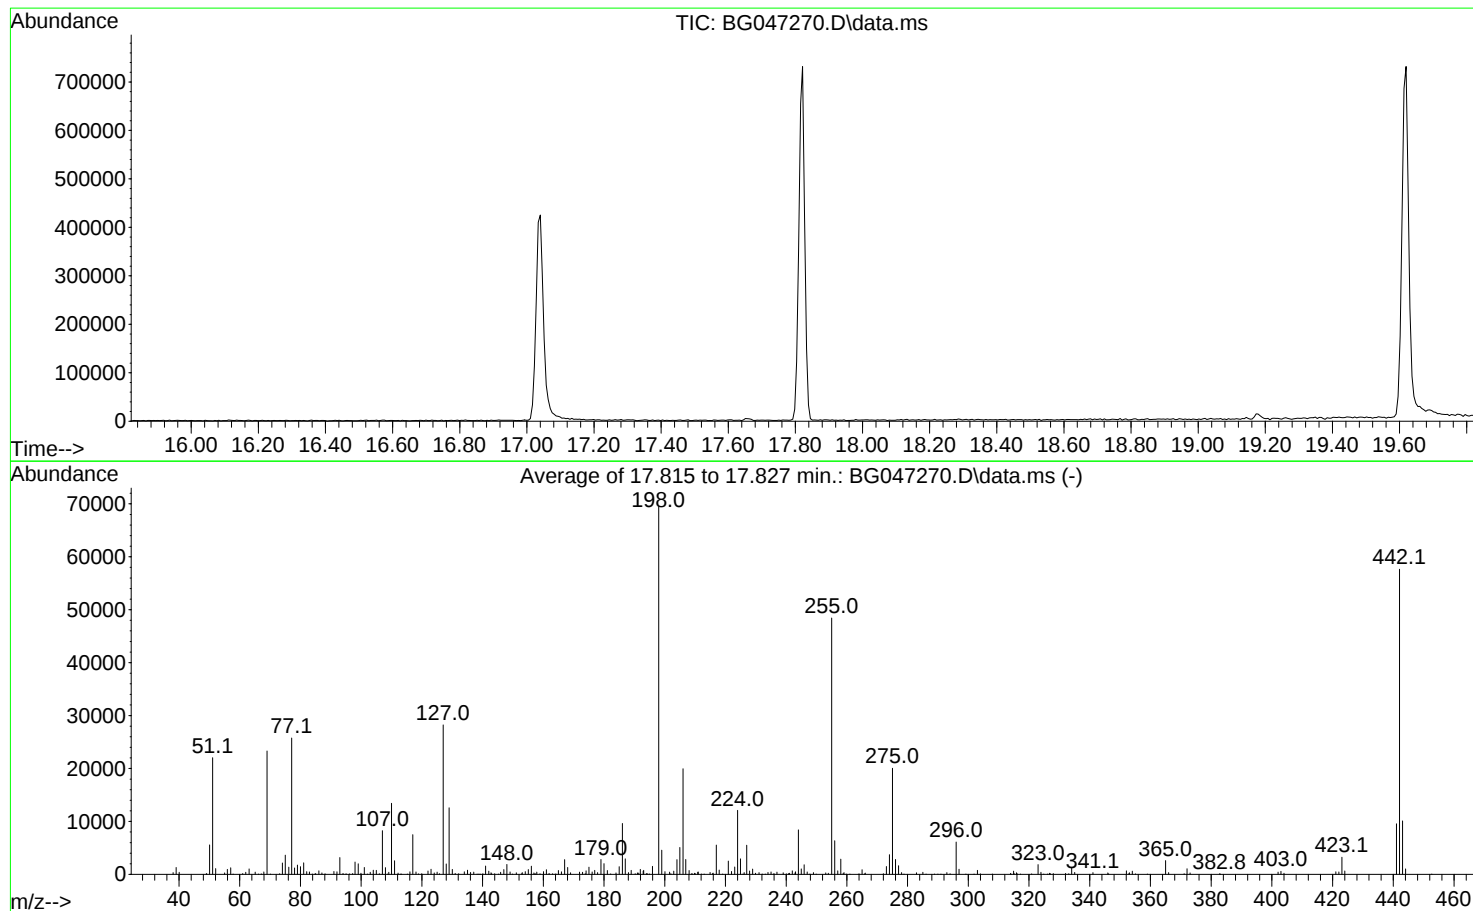

AutoFind: Scans 2464, 2465, 2466; Background Corrected with Scan 2457

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.7	22050	PASS
68	69	0.00	2	1.9	446	PASS
69	198	0.00	100	33.6	23322	PASS
70	69	0.00	2	0.3	77	PASS
127	198	10	80	40.6	28224	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	69501	PASS
199	198	5	9	6.6	4581	PASS
275	198	10	60	28.8	20043	PASS
365	198	1	100	3.8	2614	PASS
441	198	0.01	100	13.8	9567	PASS
442	198	50	100	82.9	57637	PASS
443	442	15	24	17.5	10115	PASS