


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111120\
 Data File : BG047282.D
 Acq On : 11 Nov 2020 13:14
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG110420.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Nov 04 16:19:40 2020

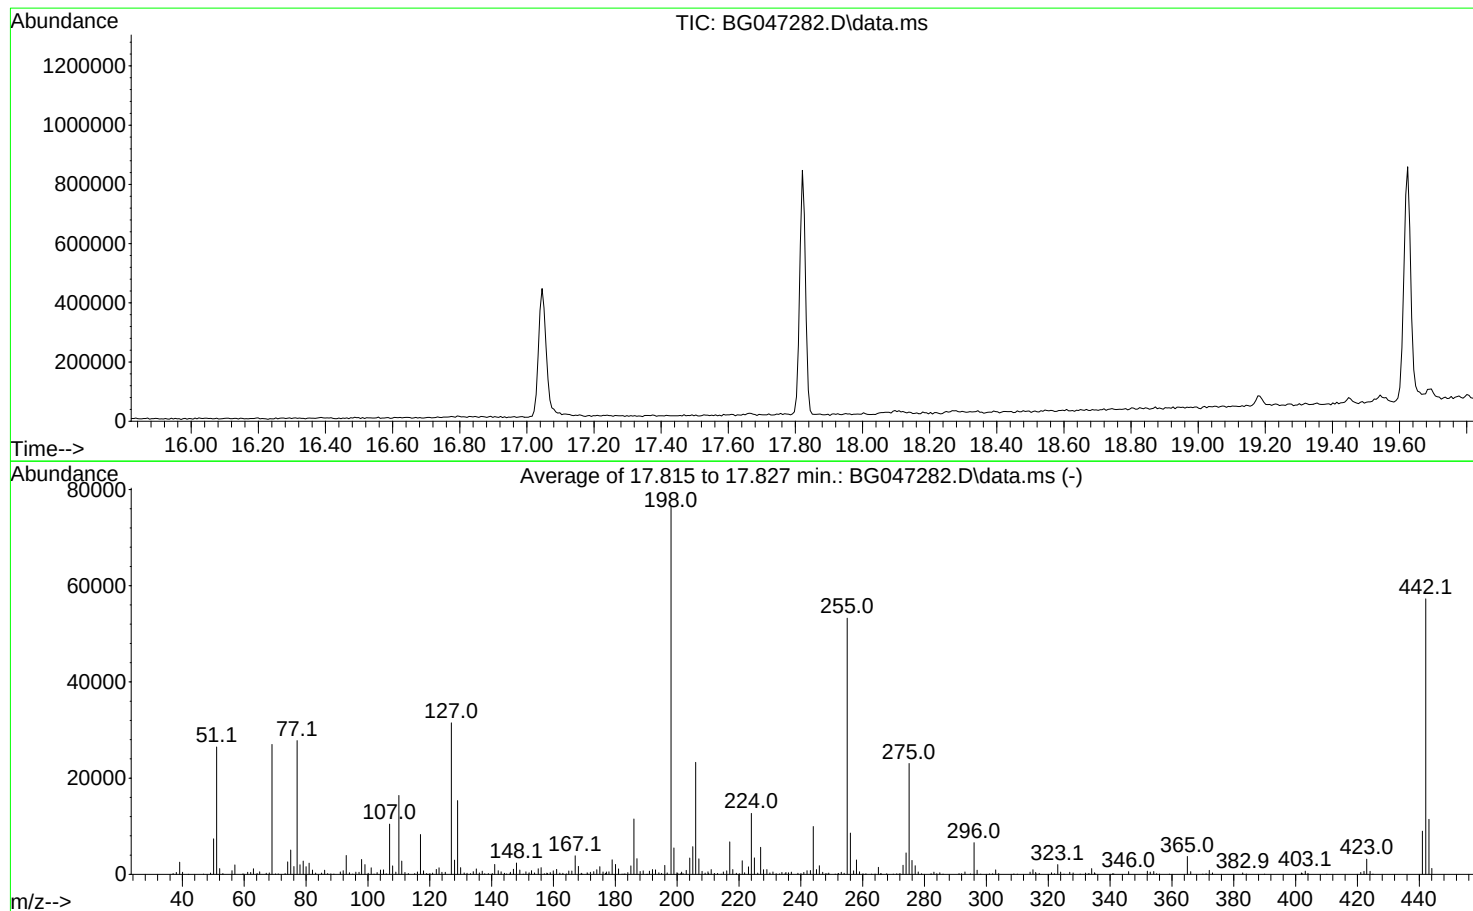

AutoFind: Scans 2464, 2465, 2466; Background Corrected with Scan 2458

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.6	26491	PASS
68	69	0.00	2	1.1	293	PASS
69	198	0.00	100	35.3	27002	PASS
70	69	0.00	2	0.4	116	PASS
127	198	10	80	41.2	31509	PASS
197	198	0.00	2	0.4	300	PASS
198	198	100	100	100.0	76461	PASS
199	198	5	9	7.2	5482	PASS
275	198	10	60	30.1	23036	PASS
365	198	1	100	4.9	3718	PASS
441	198	0.01	100	11.7	8979	PASS
442	198	50	100	74.9	57275	PASS
443	442	15	24	20.0	11436	PASS