


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111120\
 Data File : BG047300.D
 Acq On : 12 Nov 2020 2:51
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG110420.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Nov 04 16:19:40 2020

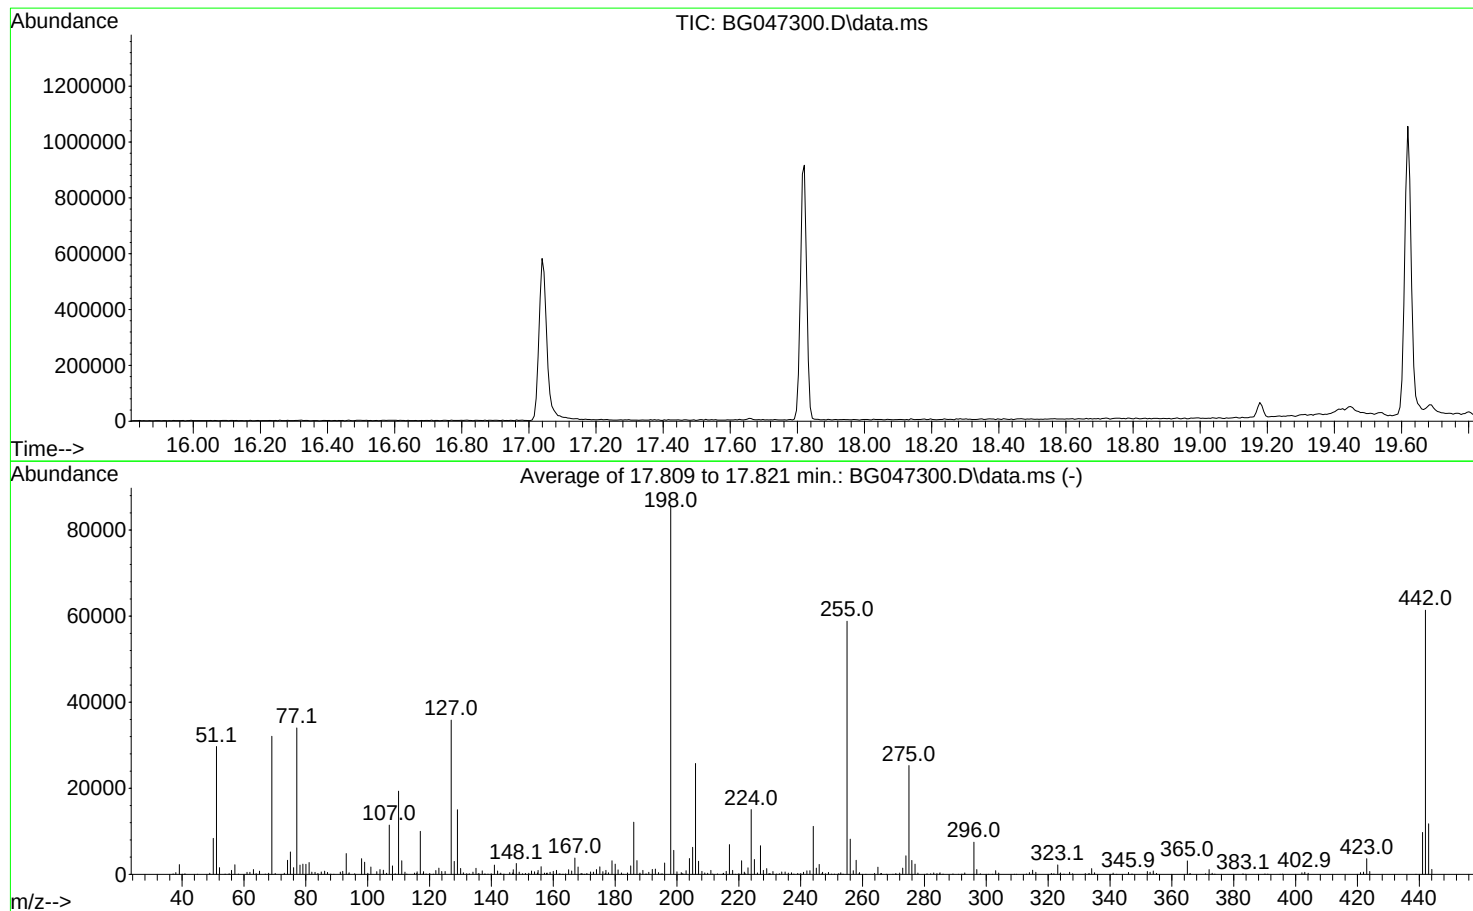

AutoFind: Scans 2463, 2464, 2465; Background Corrected with Scan 2457

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.8	29723	PASS
68	69	0.00	2	0.8	256	PASS
69	198	0.00	100	37.5	32097	PASS
70	69	0.00	2	0.7	240	PASS
127	198	10	80	41.9	35845	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	85480	PASS
199	198	5	9	6.5	5585	PASS
275	198	10	60	29.6	25294	PASS
365	198	1	100	3.6	3116	PASS
441	198	0.01	100	11.4	9734	PASS
442	198	50	100	71.8	61389	PASS
443	442	15	24	19.2	11758	PASS