
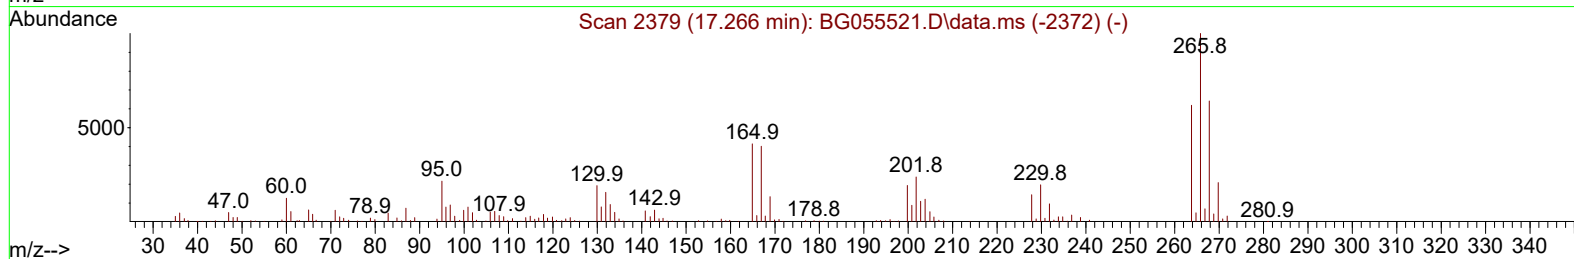
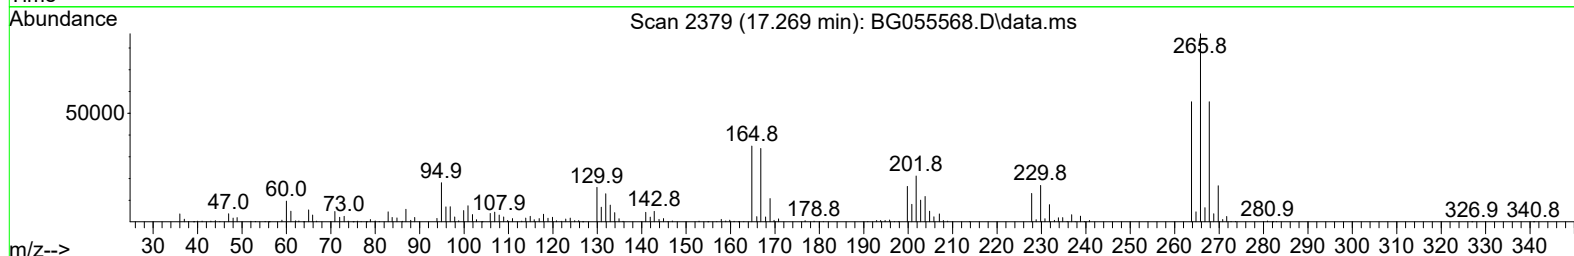


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111122\
Data File : BG055568.D
Acq On : 11 Nov 2022 15:49
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 11 17:28:34 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG110922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 10 03:39:46 2022
Response via : Initial Calibration

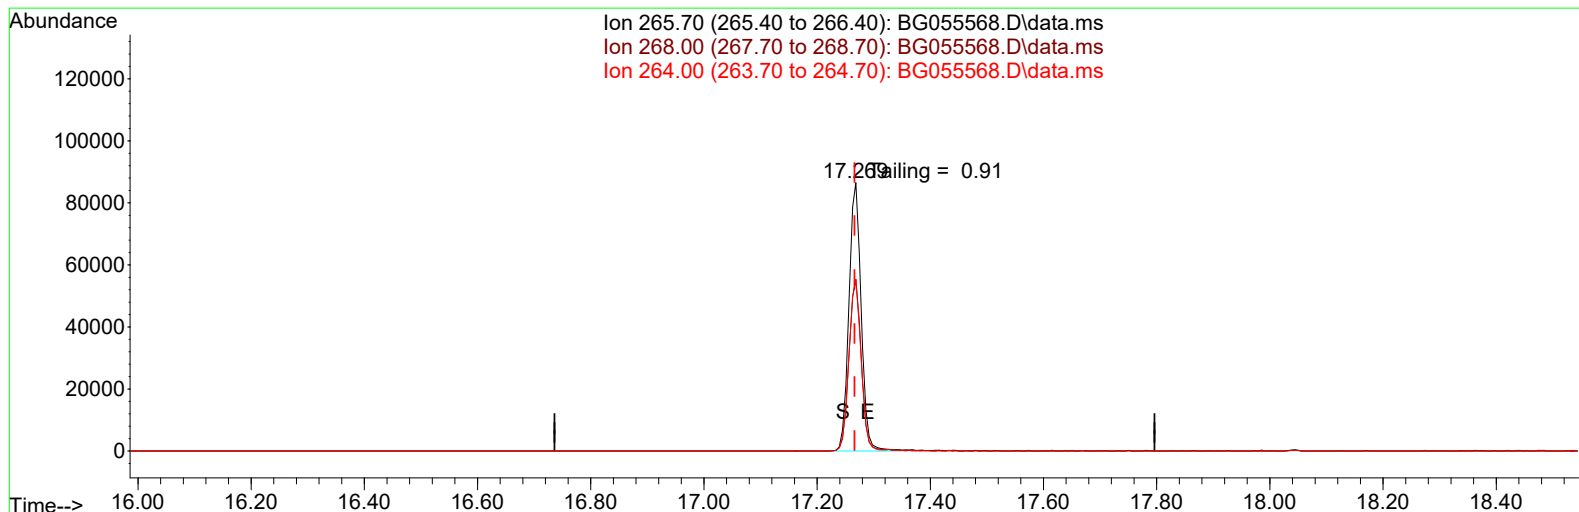

TIC: BG055568.D\data.ms

(70) Pentachlorophenol (C)




17.269min (+ 0.003) 36256.20 ng

response 130090

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.20	63.93
264.00	61.90	63.91
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111122\
Data File : BG055568.D
Acq On : 11 Nov 2022 15:49
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 11 17:28:34 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG110922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 10 03:39:46 2022
Response via : Initial Calibration

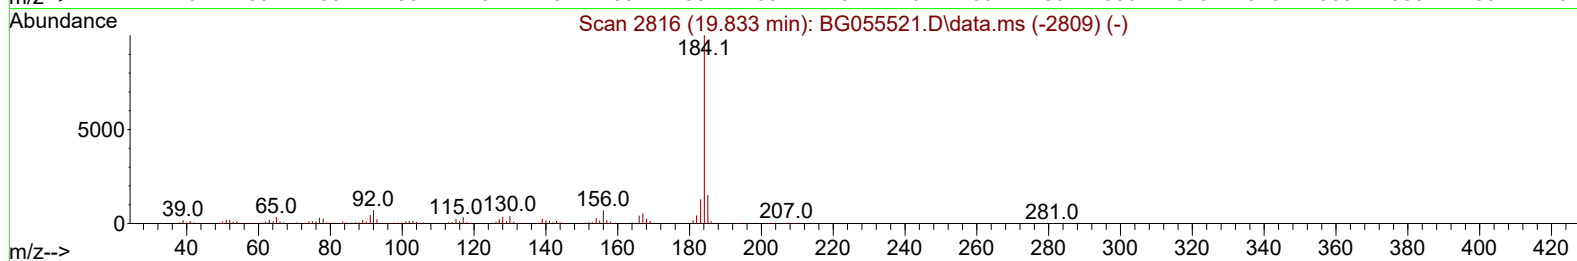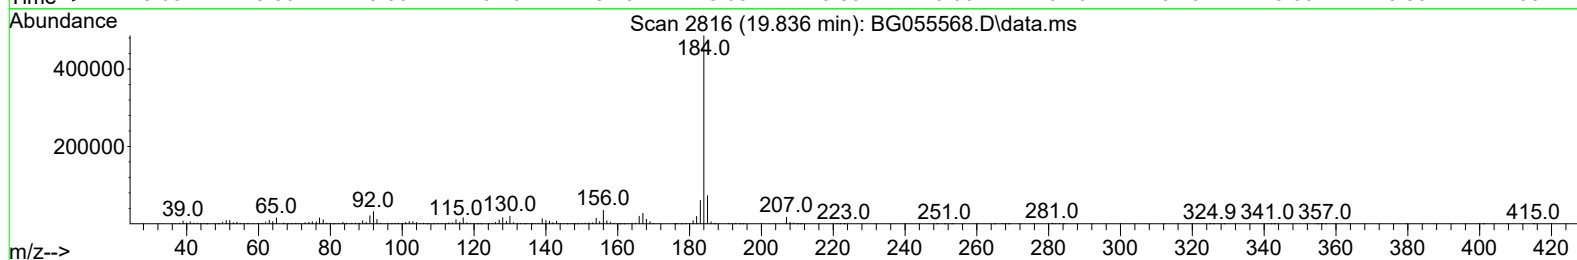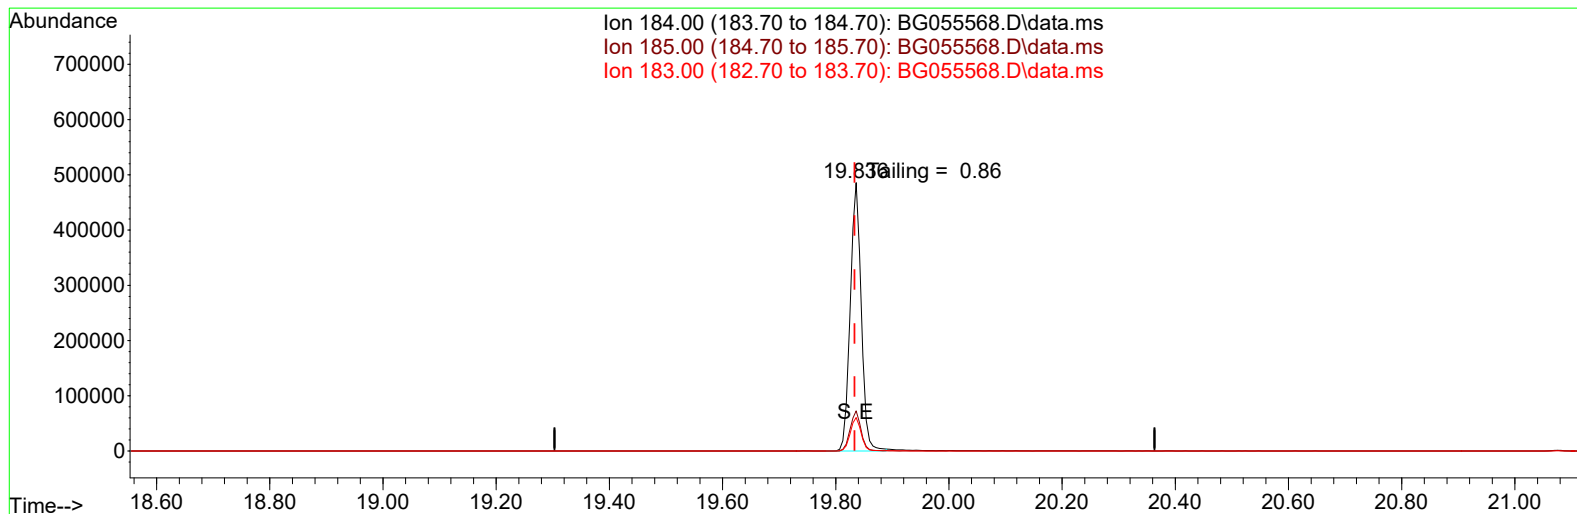

TIC: BG055568.D\data.ms

(77) Benzidine

19.836min (+ 0.003) 48682.03 ng m

response 655889

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.00	15.01
183.00	12.70	12.49
0.00	0.00	0.00