
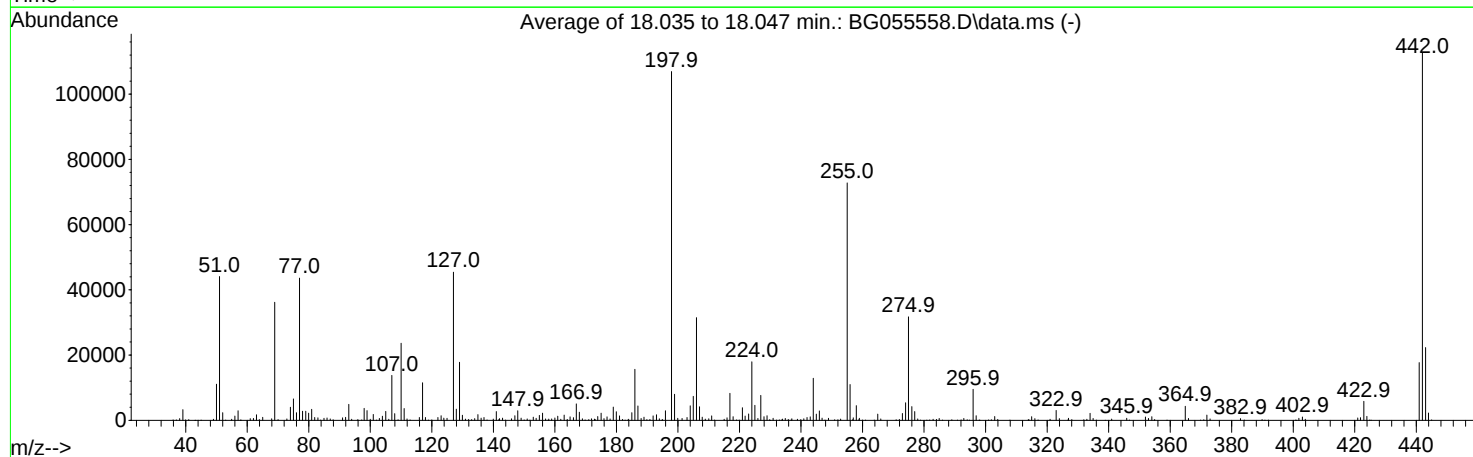


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111122\
 Data File : BG055558.D
 Acq On : 11 Nov 2022 8:42
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG110922.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Nov 10 03:39:46 2022

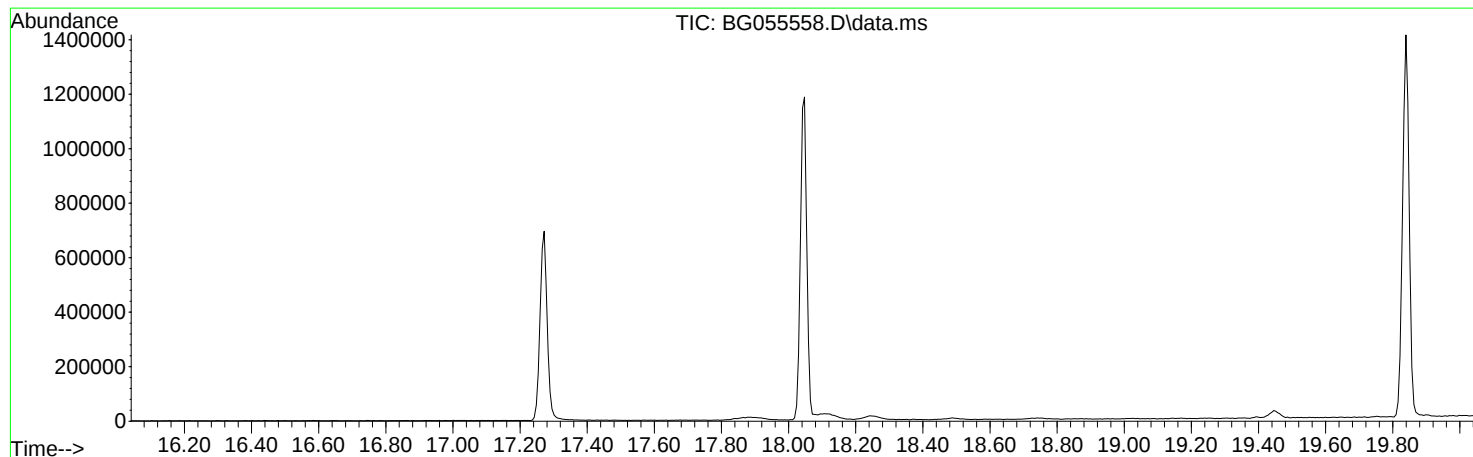




AutoFind: Scans 2510, 2511, 2512; Background Corrected with Scan 2504

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.2	44101	PASS
68	69	0.00	2	1.3	468	PASS
69	198	0.00	100	33.8	36181	PASS
70	69	0.00	2	0.6	206	PASS
127	198	10	80	42.5	45416	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	106915	PASS
199	198	5	9	7.5	7974	PASS
275	198	10	60	29.7	31736	PASS
365	198	1	100	4.0	4291	PASS
441	198	0.01	100	16.6	17705	PASS
442	442	50	100	100.0	112797	PASS
443	442	15	24	19.8	22288	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111122\
Data File : BG055558.D
Acq On : 11 Nov 2022 8:42
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Nov 11 16:40:42 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG110922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 10 03:39:46 2022
Response via : Initial Calibration

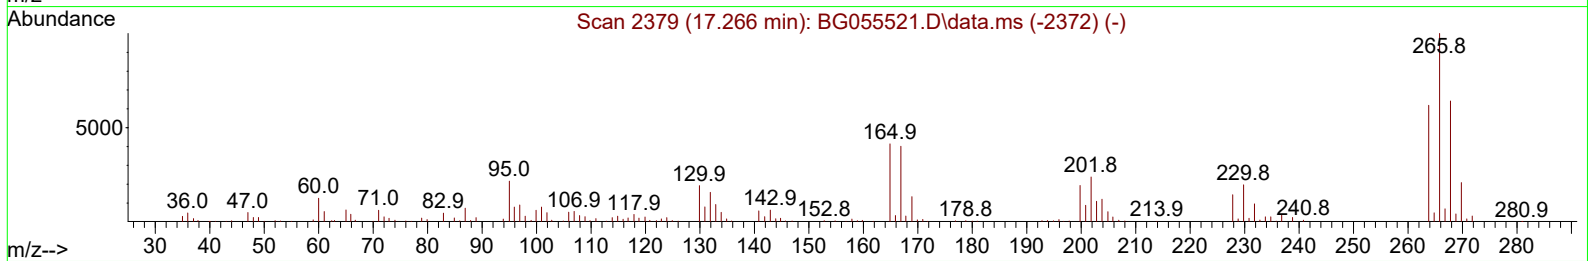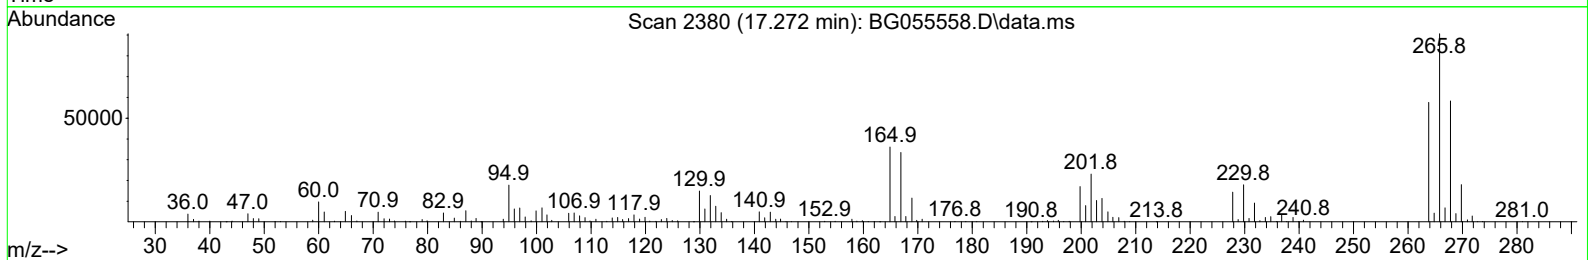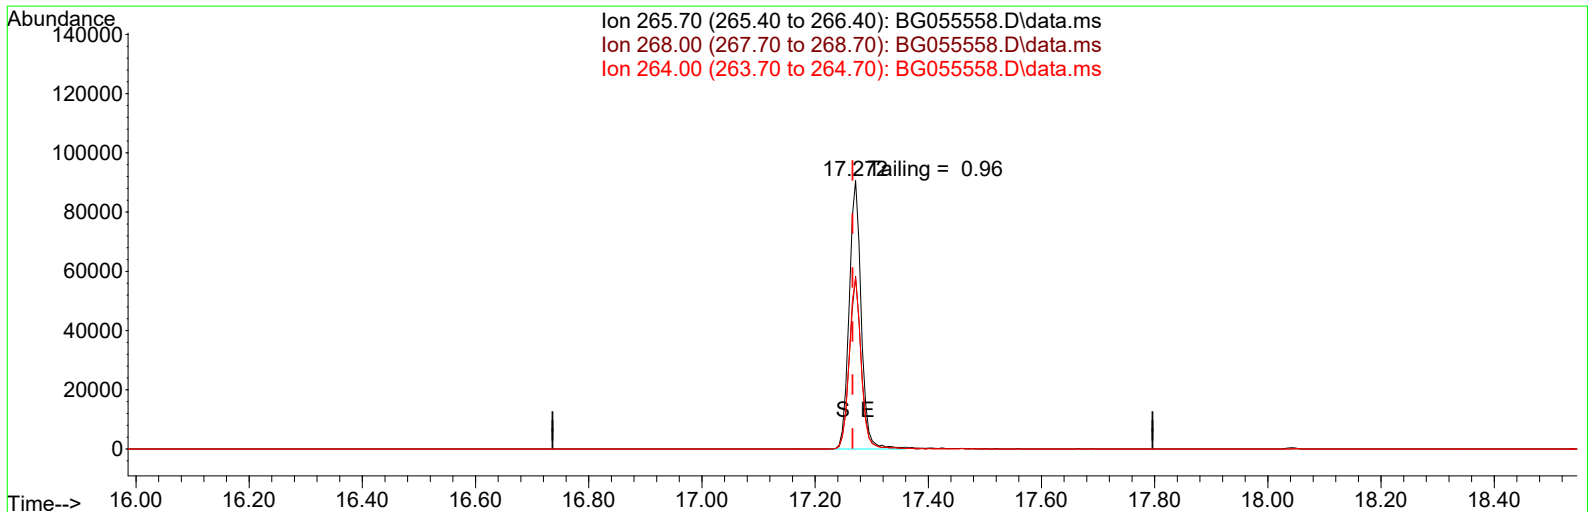

TIC: BG055558.D\data.ms

(70) Pentachlorophenol (C)

17.272min (+ 0.006) 26997.99 ng




response 135081

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.20	64.34
264.00	61.90	63.59
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111122\
Data File : BG055558.D
Acq On : 11 Nov 2022 8:42
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Nov 11 16:40:42 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG110922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 10 03:39:46 2022
Response via : Initial Calibration

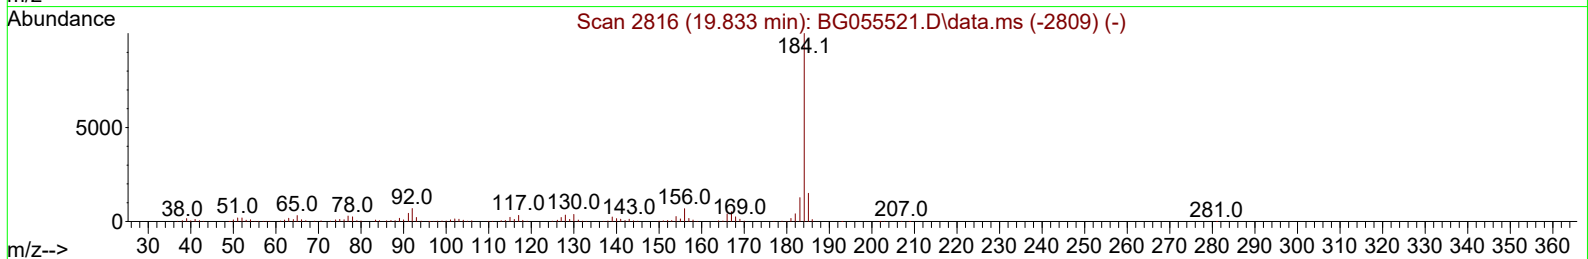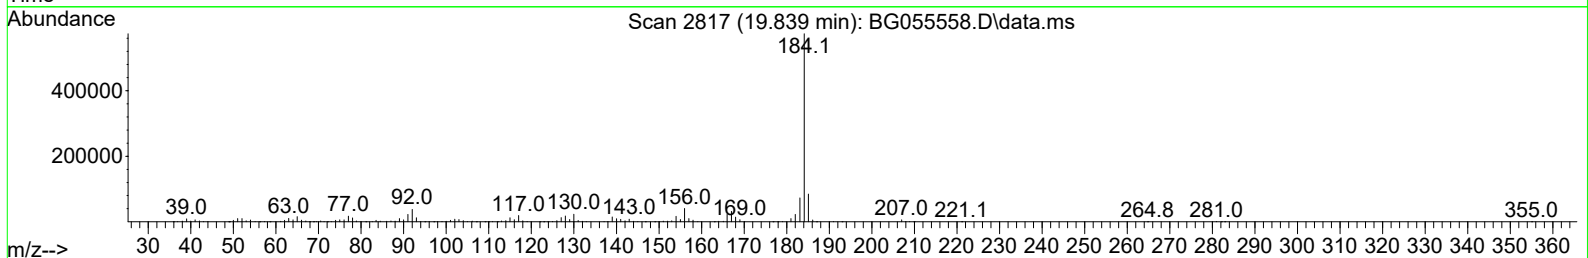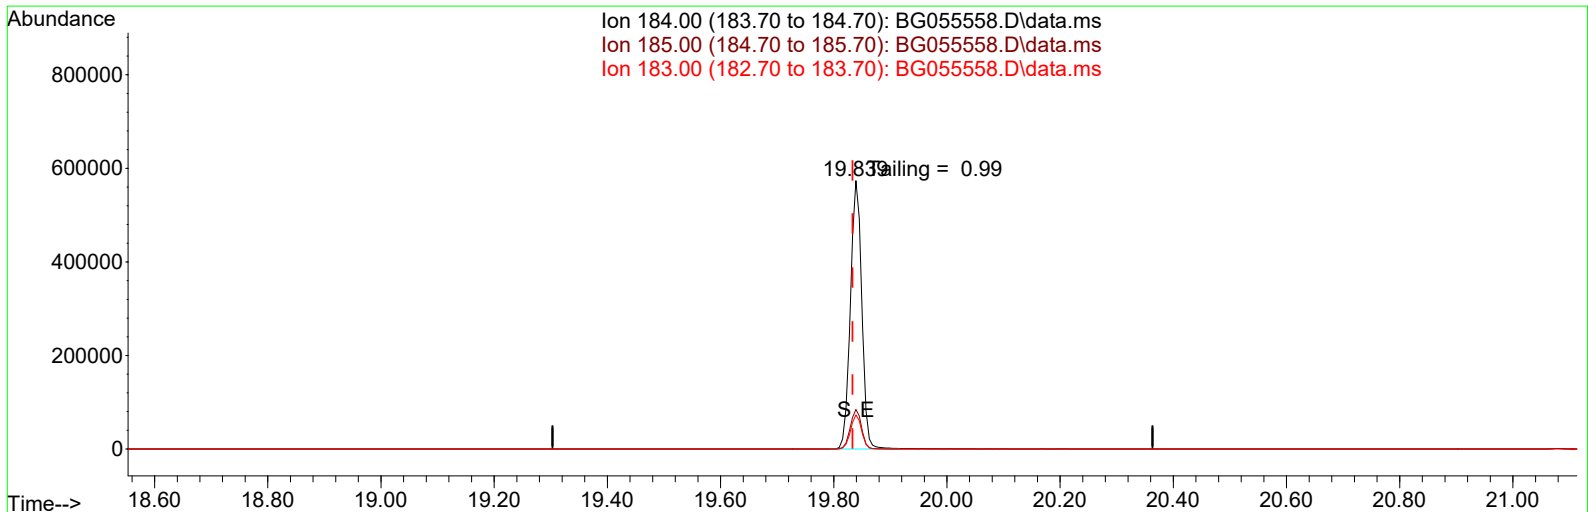

TIC: BG055558.D\data.ms

(77) Benzidine

19.839min (+ 0.006) 0.00 ng

response 800946

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.00	14.75
183.00	12.70	12.72
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/11/2022	BNA_G	<u>BG055558.D</u>
Compound Name	Response	Retention Time
DDT	332755	21.079
DDD	13668	20.627
DDE	261	20.121
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
13929	346684	4.02

Instrument :
BNA_G
ClientSampleId :
DFTPP