
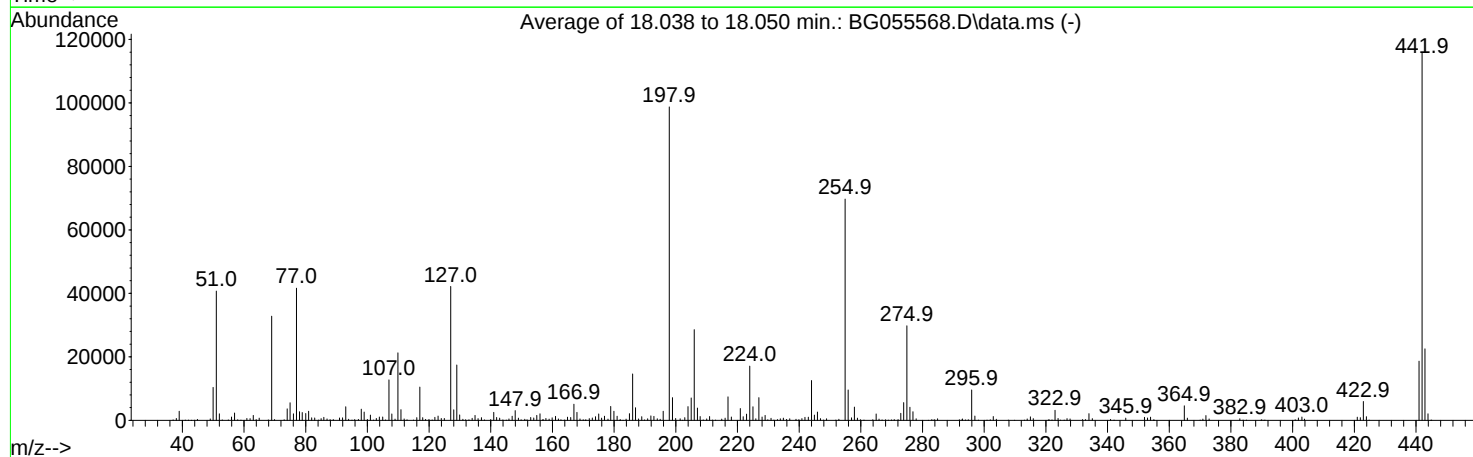


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111122\
 Data File : BG055568.D
 Acq On : 11 Nov 2022 15:49
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG110922.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Nov 10 03:39:46 2022

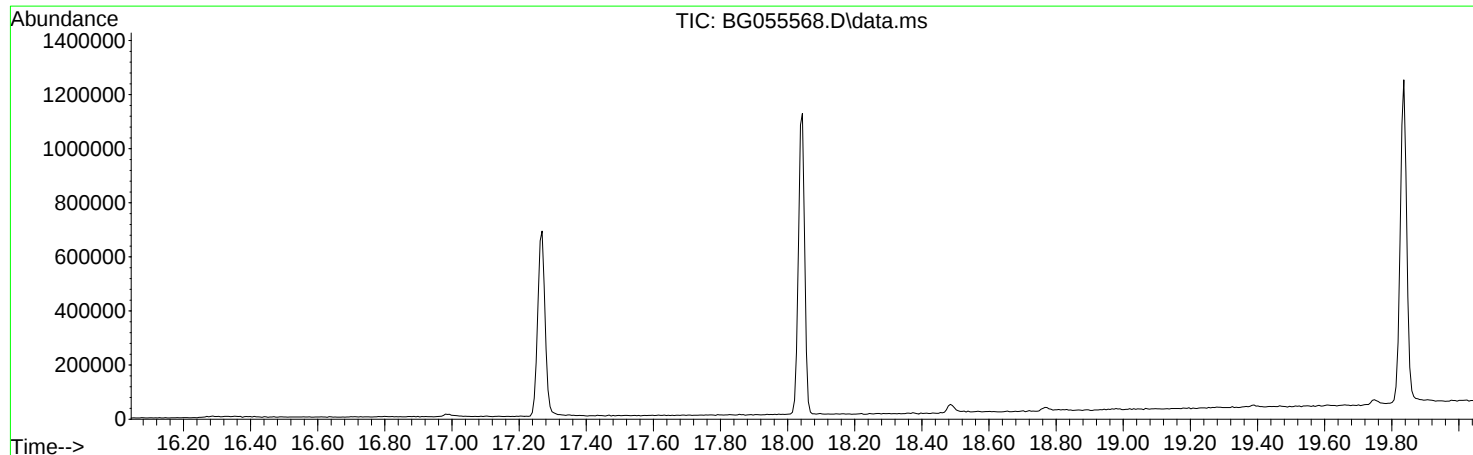




AutoFind: Scans 2510, 2511, 2512; Background Corrected with Scan 2503

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.2	40693	PASS
68	69	0.00	2	0.3	113	PASS
69	198	0.00	100	33.2	32776	PASS
70	69	0.00	2	0.7	223	PASS
127	198	10	80	42.7	42163	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	98741	PASS
199	198	5	9	7.2	7155	PASS
275	198	10	60	30.1	29755	PASS
365	198	1	100	4.6	4541	PASS
441	198	0.01	100	18.9	18648	PASS
442	442	50	100	100.0	115917	PASS
443	442	15	24	19.4	22501	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111122\
Data File : BG055568.D
Acq On : 11 Nov 2022 15:49
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Nov 11 17:28:34 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG110922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 10 03:39:46 2022
Response via : Initial Calibration

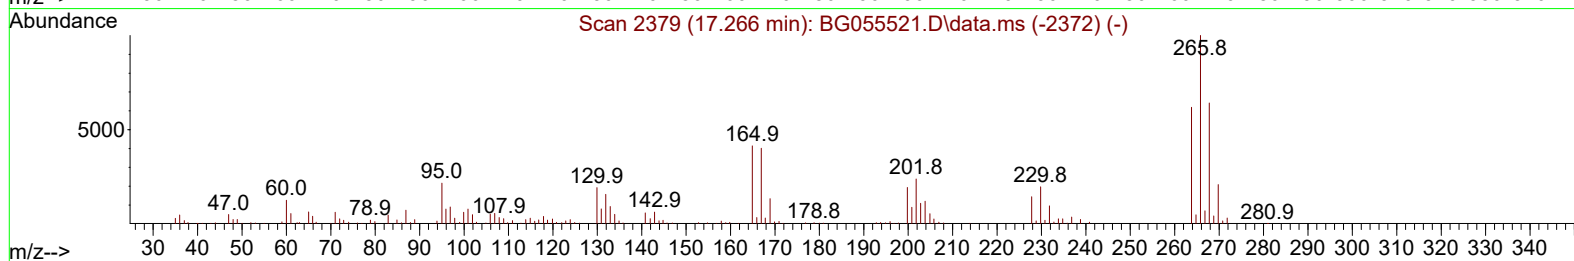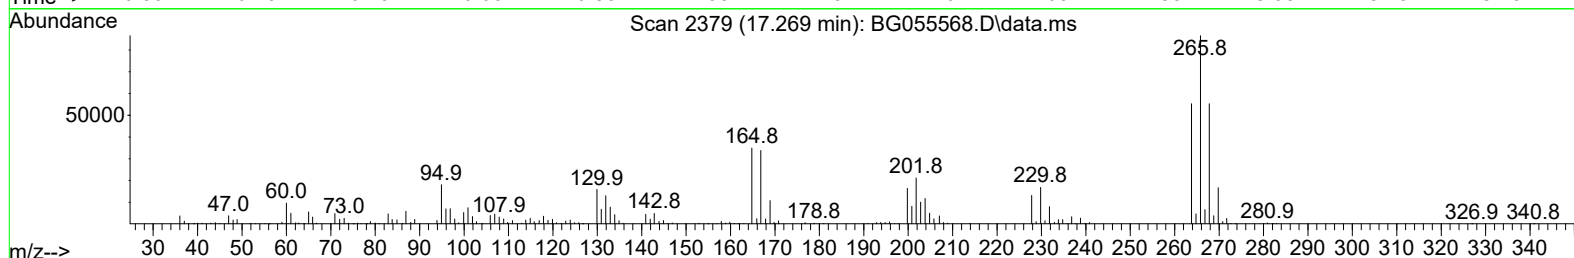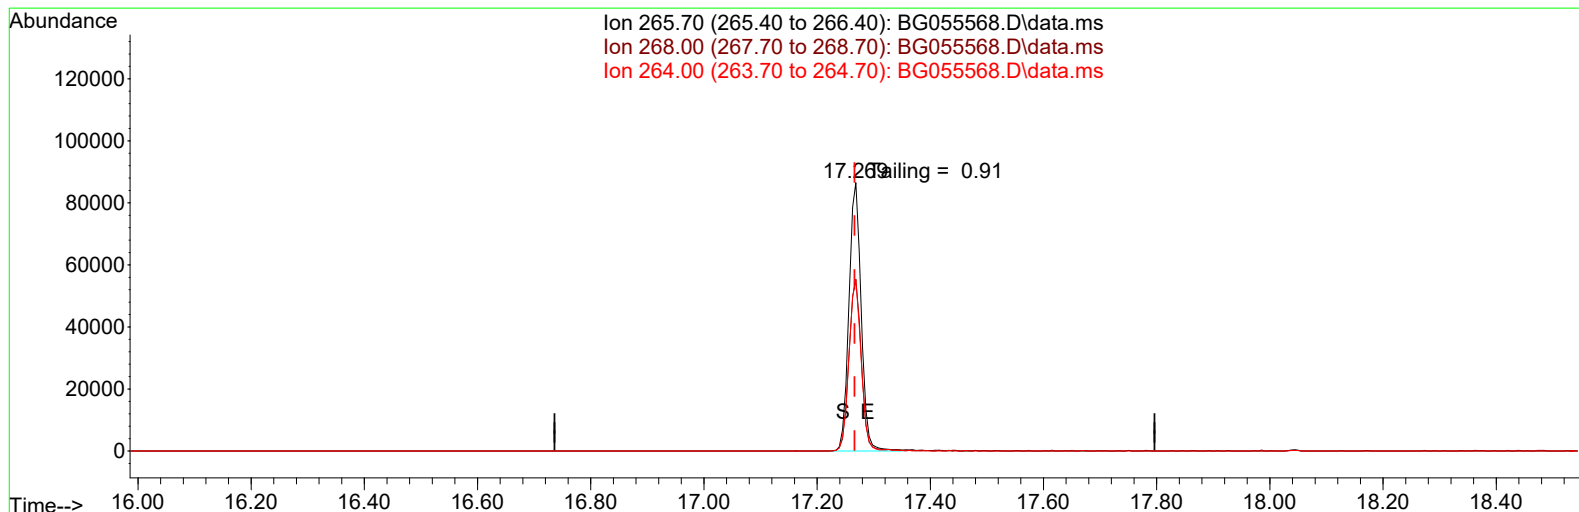

TIC: BG055568.D\data.ms

(70) Pentachlorophenol (C)

17.269min (+ 0.003) 36256.20 ng




response 130090

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.20	63.93
264.00	61.90	63.91
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111122\
Data File : BG055568.D
Acq On : 11 Nov 2022 15:49
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Nov 11 17:28:34 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG110922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 10 03:39:46 2022
Response via : Initial Calibration

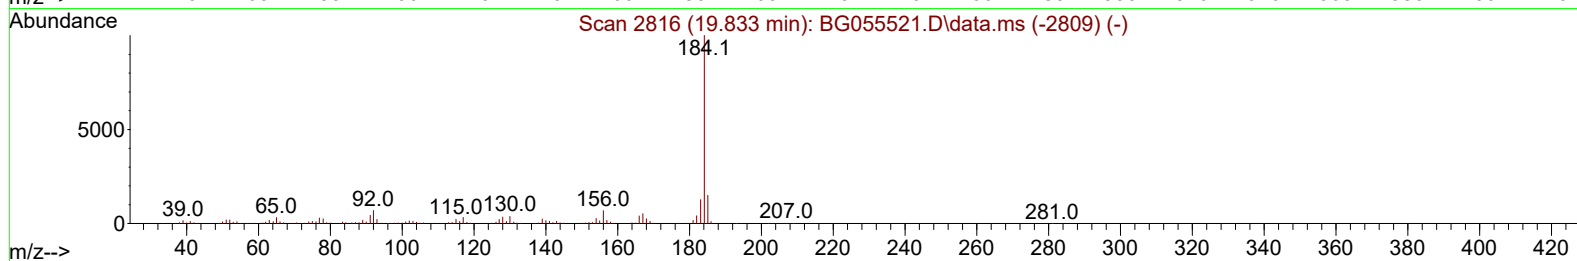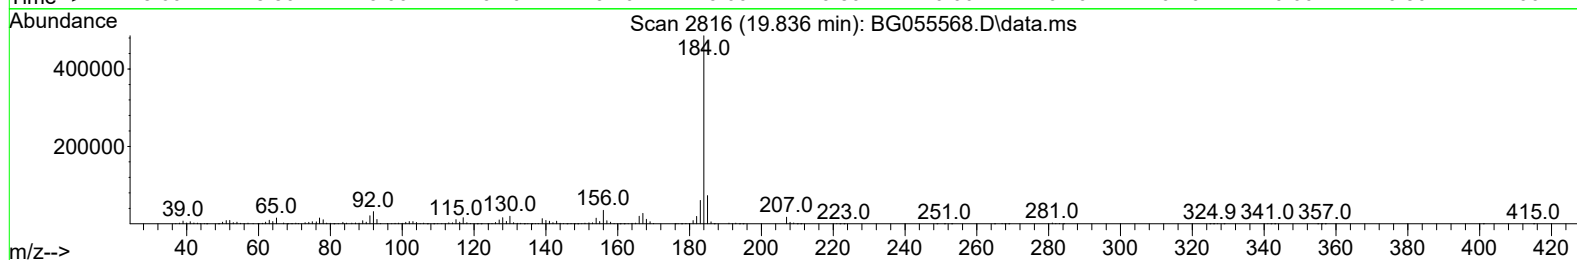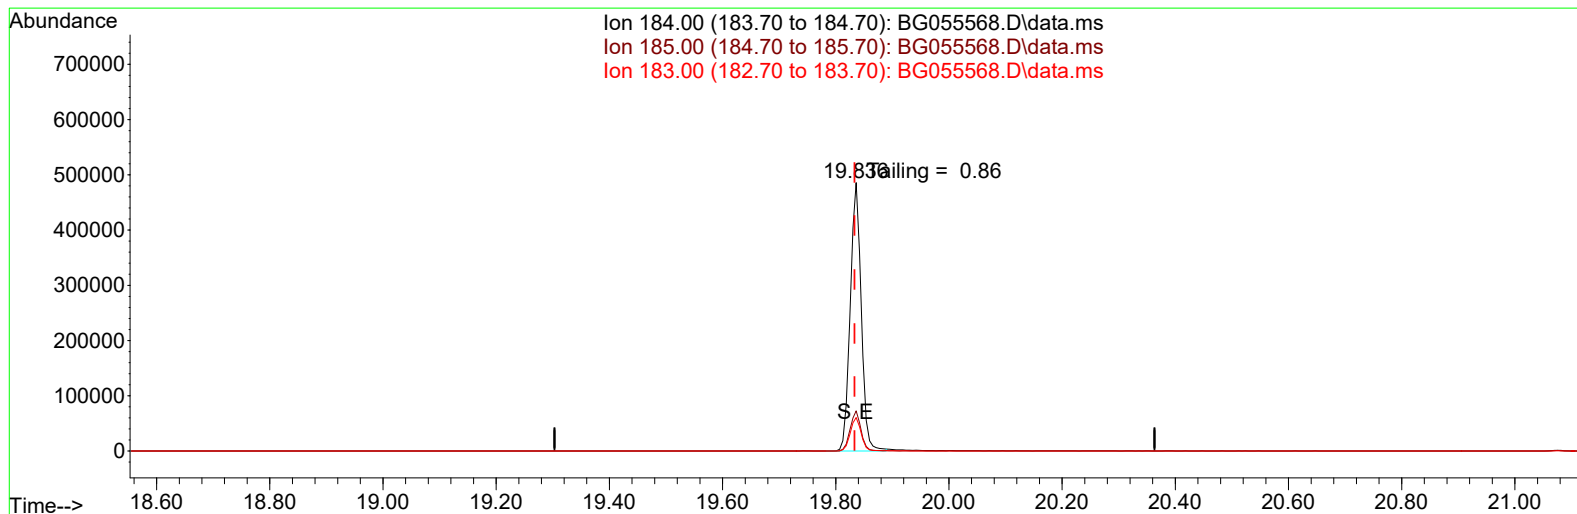

TIC: BG055568.D\data.ms

(77) Benzidine

19.836min (+ 0.003) 48682.03 ng m

response 655889

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.00	15.01
183.00	12.70	12.49
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/11/2022	BNA_G	<u>BG055568.D</u>
Compound Name	Response	Retention Time
DDT	337858	21.076
DDD	8937	20.624
DDE	229	20.124
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
9166	347024	2.64

Instrument :
BNA_G
ClientSampleId :
DFTPP