

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111124\
 Data File : BG063317.D
 Acq On : 12 Nov 2024 9:34
 Operator : RC/JU
 Sample : P4714-17
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0AJ3

Quant Time: Nov 12 10:19:16 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Nov 06 15:45:52 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.835	152	129998	20.000	ng/u1	0.00
20) Naphthalene-d8	10.620	136	636325	20.000	ng/u1	# 0.00
38) Acenaphthene-d10	14.475	164	531828	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.224	188	1213351	20.000	ng/u1	# 0.00
79) Chrysene-d12	21.478	240	1198791	20.000	ng/u1	# 0.00
88) Perylene-d12	24.516	264	1339832	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.300	96	10751	3.740	ng/uL	0.00
4) Pyridine-d5	3.705	84	90913	9.568	ng/u1	0.00
7) Phenol-d5	7.007	99	118642	10.114	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.166	67	190354	27.666	ng/u1	0.00
11) 2-Chlorophenol-d4	7.365	132	215735	28.335	ng/u1	-0.01
15) 4-Methylphenol-d8	8.540	113	230384	23.171	ng/u1	0.00
21) Nitrobenzene-d5	8.987	128	120595	26.957	ng/u1	0.00
24) 2-Nitrophenol-d4	9.710	143	154765	26.767	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.250	165	355740	31.352	ng/u1	0.00
31) 4-Chloroaniline-d4	10.761	131	348381	23.573	ng/u1	0.00
46) Dimethylphthalate-d6	13.875	166	1203525	28.890	ng/u1	0.00
49) Acenaphthylene-d8	14.163	160	1225967	30.067	ng/u1	0.00
54) 4-Nitrophenol-d4	14.692	143	53762	9.426	ng/u1	0.01
60) Fluorene-d10	15.468	176	1065375	30.302	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.597	200	223213	29.271	ng/u1	0.00
73) Anthracene-d10	17.324	188	1831725	35.125	ng/u1	0.00
81) Pyrene-d10	19.622	212	2215149	36.855	ng/u1	0.00
92) Benzo(a)pyrene-d12	24.304	264	2296326	35.498	ng/u1	0.00
Target Compounds						
59) Diethylphthalate	15.291	149	108797	2.657	ng/u1	Qvalue 95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111124\
Data File : BG063317.D
Acq On : 12 Nov 2024 9:34
Operator : RC/JU
Sample : P4714-17
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0AJ3

Quant Time: Nov 12 10:19:16 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 06 15:45:52 2024
Response via : Initial Calibration

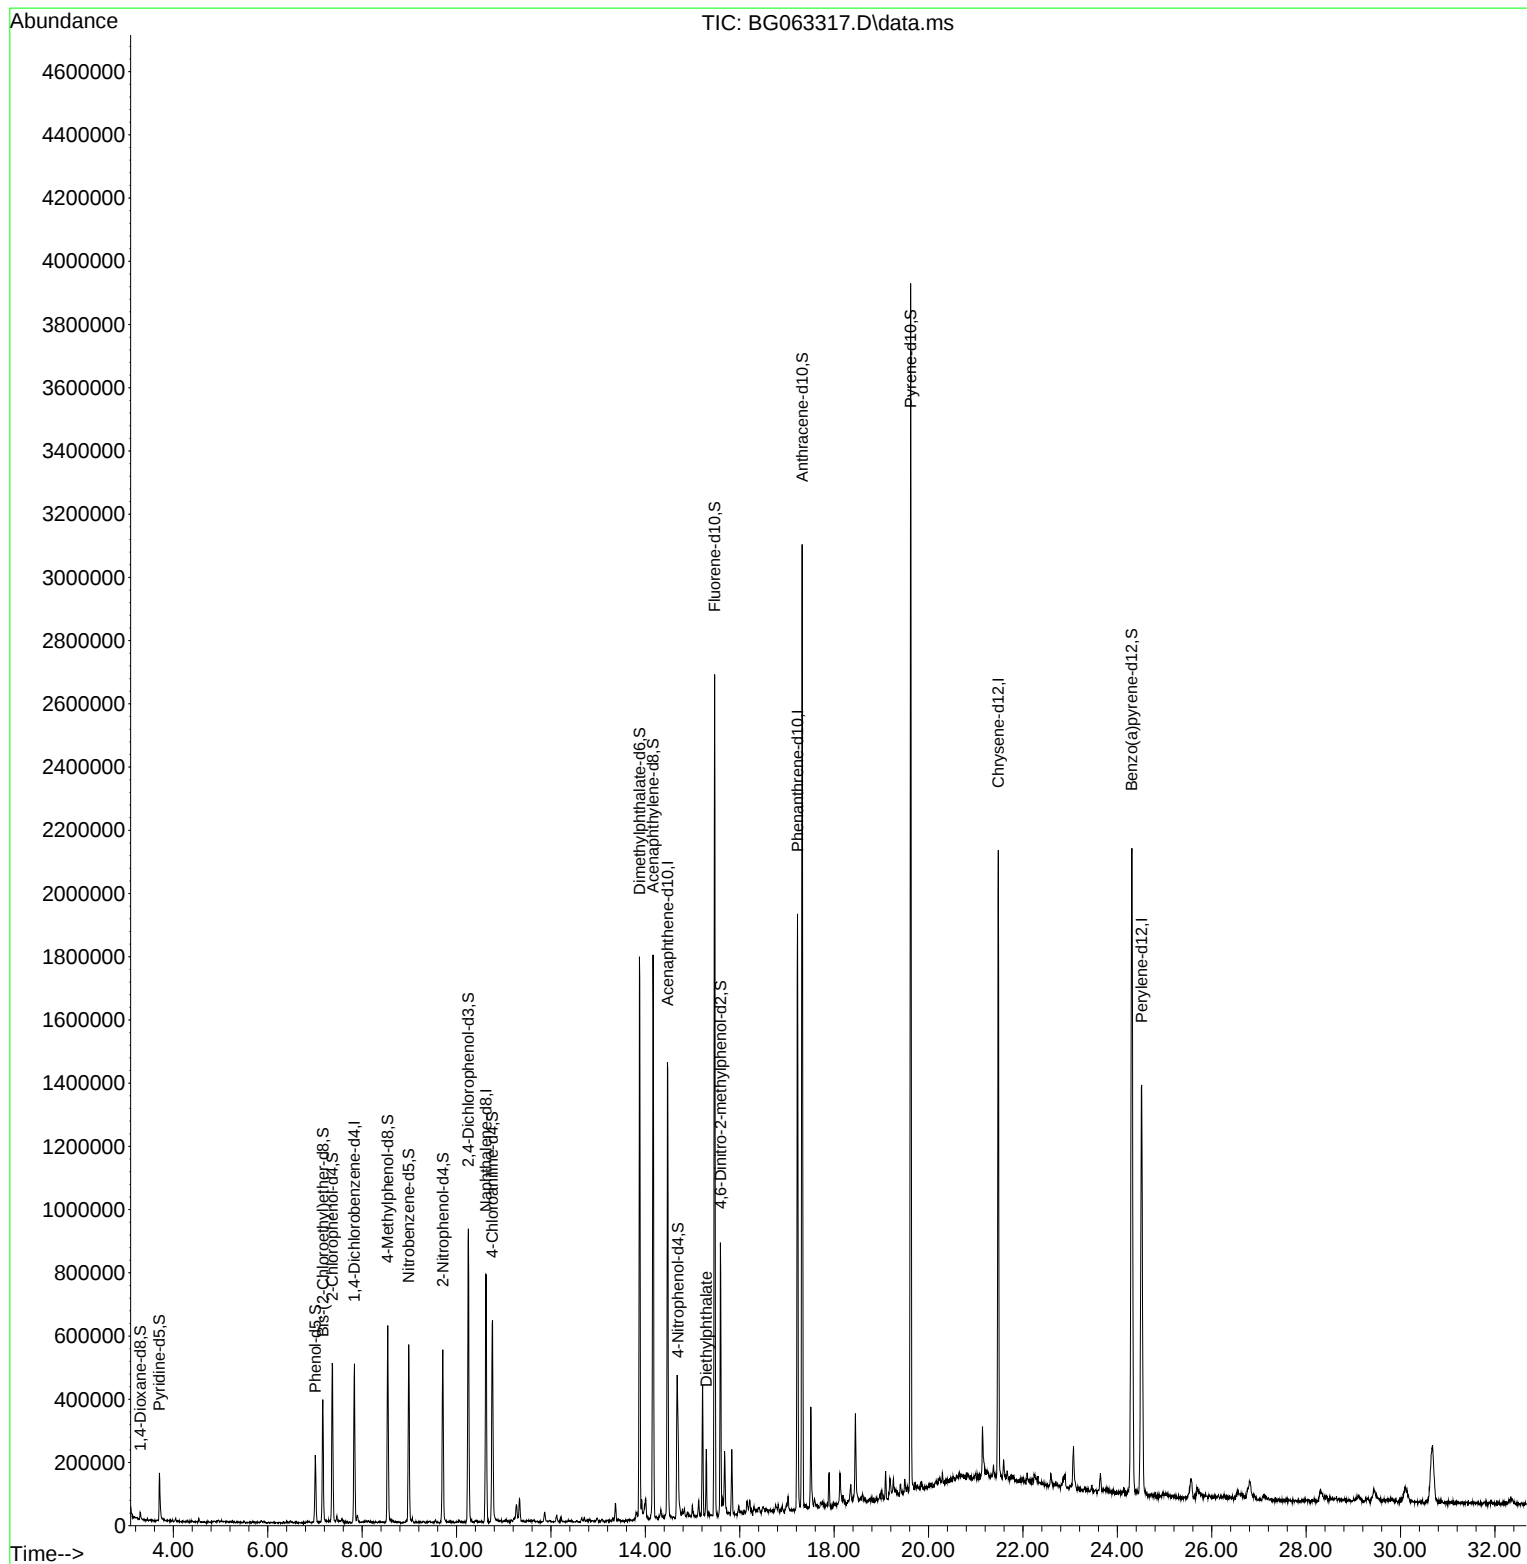

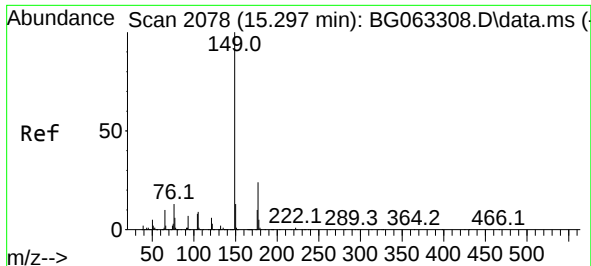

#59
 Diethylphthalate
 Concen: 2.657 ng/ul
 RT: 15.291 min Scan# 2077
 Delta R.T. -0.006 min
 Lab File: BG063317.D
 Acq: 12 Nov 2024 9:34

Instrument :
 BNA_G
 ClientSampleId :
 C0AJ3

Tgt Ion:149 Resp: 108797

Ion	Ratio	Lower	Upper
149	100		
177	21.9	19.6	29.4
150	10.7	10.0	15.0

