

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111124\
 Data File : BG063285.D
 Acq On : 11 Nov 2024 12:24
 Operator : RC/JU
 Sample : PB164576BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK576

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG063285.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.301	32	36	41	rBV3	25338	34450	0.85%	0.094%
2	3.707	100	105	116	rBV	318803	513582	12.67%	1.405%
3	4.036	159	161	162	rBV2	8275	6381	0.16%	0.017%
4	5.522	412	414	416	rBV3	6094	6731	0.17%	0.018%
5	7.009	661	667	676	rBV	425776	705239	17.40%	1.929%
6	7.167	688	694	701	rBV	289166	469176	11.58%	1.284%
7	7.367	722	728	738	rBV	388067	655145	16.16%	1.792%
8	7.696	782	784	786	rBV2	6115	5642	0.14%	0.015%
9	7.837	800	808	818	rVB	299215	508832	12.55%	1.392%
10	8.542	921	928	939	rBV2	566803	955474	23.58%	2.614%
11	8.989	996	1004	1011	rBV	399656	717763	17.71%	1.964%
12	9.711	1119	1127	1138	rVB	385831	694939	17.15%	1.901%
13	10.252	1212	1219	1226	rBV	603699	1065421	26.29%	2.915%
14	10.358	1236	1237	1241	rVB3	6496	6407	0.16%	0.018%
15	10.393	1241	1243	1247	rBV2	5135	6444	0.16%	0.018%
16	10.622	1276	1282	1291	rVB	478581	838420	20.69%	2.294%
17	10.763	1298	1306	1316	rBV	546009	1039146	25.64%	2.843%
18	11.133	1366	1369	1372	rVB4	5148	5955	0.15%	0.016%
19	11.580	1439	1445	1446	rBV4	6108	6866	0.17%	0.019%
20	12.232	1549	1556	1561	rBV4	8581	23016	0.57%	0.063%
21	12.902	1665	1670	1671	rBV2	6616	7614	0.19%	0.021%
22	13.572	1779	1784	1787	rVB	4023	7435	0.18%	0.020%
23	13.877	1829	1836	1847	rBV	1286206	1867327	46.07%	5.108%
24	14.165	1878	1885	1895	rBV	1384133	2155165	53.18%	5.896%
25	14.476	1928	1938	1945	rBV	952855	1526252	37.66%	4.175%
26	14.682	1965	1973	1984	rBV	414196	763739	18.84%	2.089%
27	14.852	2000	2002	2006	rVB5	6944	6833	0.17%	0.019%
28	15.358	2087	2088	2091	rVB	6068	5742	0.14%	0.016%
29	15.469	2100	2107	2116	rBV	1982771	2856011	70.47%	7.813%
30	15.593	2122	2128	2136	rBV	539210	804570	19.85%	2.201%
31	16.251	2237	2240	2244	rVB2	5567	6655	0.16%	0.018%
32	16.368	2257	2260	2262	rBV3	5522	6093	0.15%	0.017%
33	17.226	2398	2406	2413	rBV	1339085	2011330	49.63%	5.502%
34	17.320	2416	2422	2432	rBV	2142973	3299240	81.41%	9.026%
35	17.820	2504	2507	2510	rBV3	5216	6018	0.15%	0.016%
36	18.683	2652	2654	2657	rBV2	5300	5762	0.14%	0.016%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111124\
Data File : BG063285.D
Acq On : 11 Nov 2024 12:24
Operator : RC/JU
Sample : PB164576BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK576

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
Title : SVOA CALIBRATION

37	19.124	2727	2729	2732	rBV3	5485	6786	0.17%	0.019%
38	19.183	2734	2739	2745	rVV2	37918	61226	1.51%	0.167%
39	19.259	2747	2752	2758	rVV2	31099	55123	1.36%	0.151%
40	19.318	2760	2762	2767	rVB5	6552	8183	0.20%	0.022%
41	19.488	2785	2791	2795	rBV6	6917	12484	0.31%	0.034%
42	19.553	2801	2802	2806	rVB4	9721	9081	0.22%	0.025%
43	19.623	2806	2814	2823	rBV	2937155	4052870	100.00%	11.087%
44	20.804	3013	3015	3016	rBV2	9963	7683	0.19%	0.021%
45	21.480	3123	3130	3140	rBV2	1489550	2370050	58.48%	6.484%
46	22.896	3367	3371	3375	rVB7	33250	52147	1.29%	0.143%
47	24.306	3601	3611	3621	rBV	1533395	3877518	95.67%	10.608%
48	24.512	3637	3646	3659	rVB	901612	2439798	60.20%	6.675%




Sum of corrected areas: 36553764

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111124\
Data File : BG063285.D
Acq On : 11 Nov 2024 12:24
Operator : RC/JU
Sample : PB164576BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK576

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

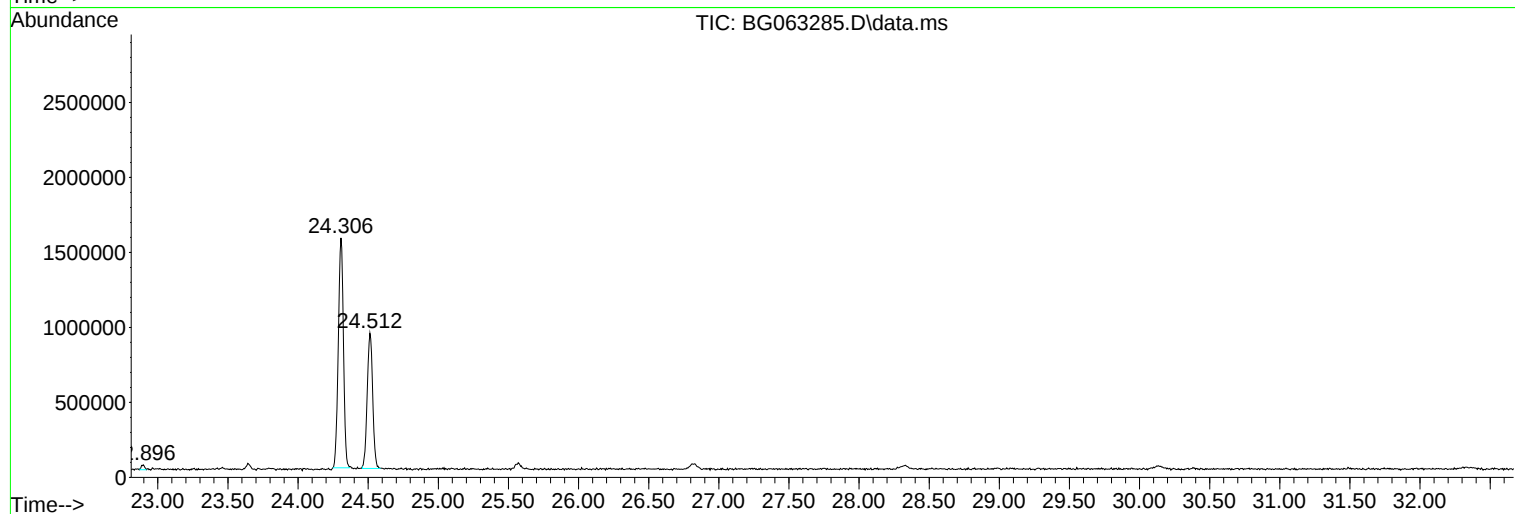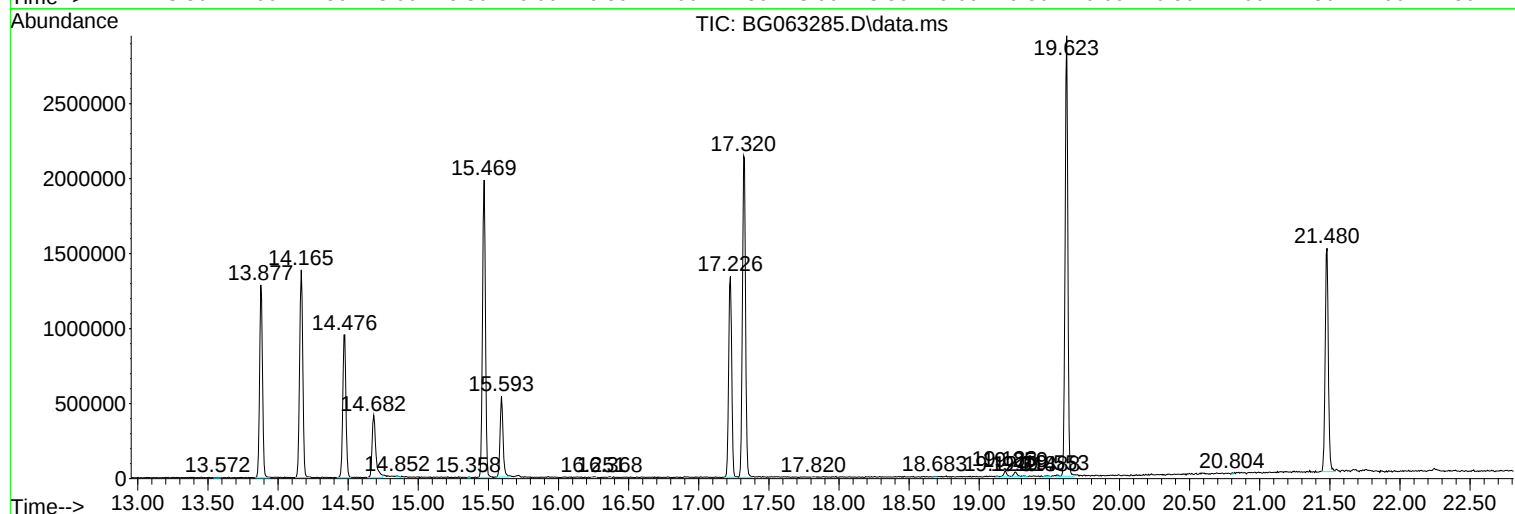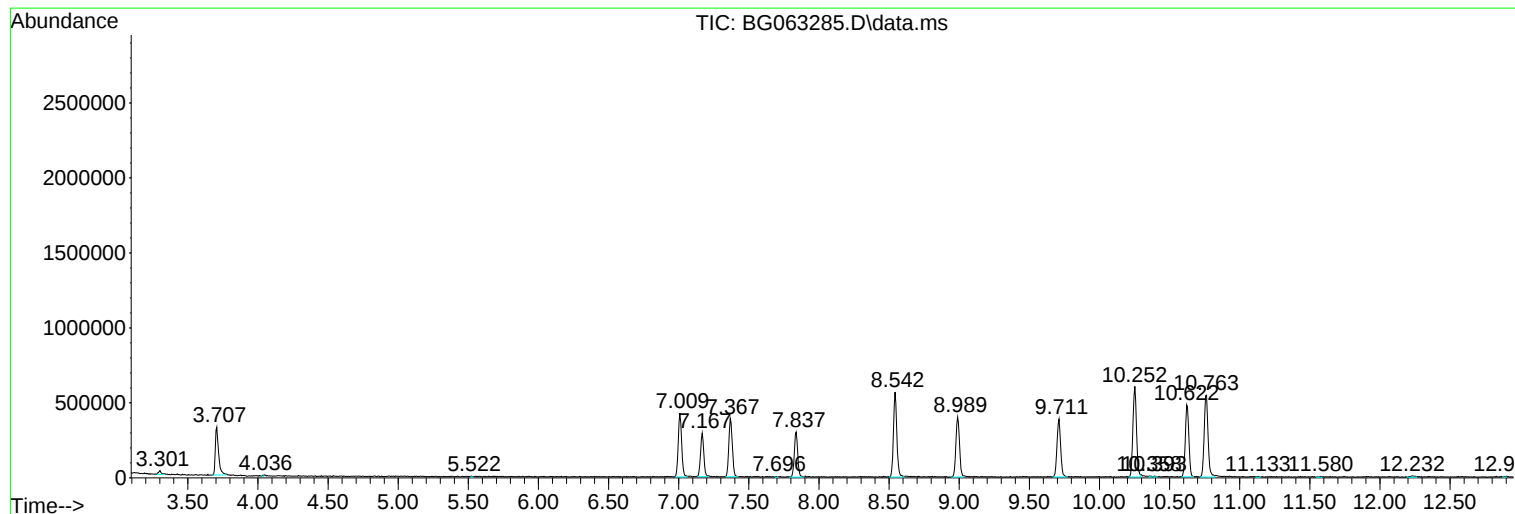

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111124\
Data File : BG063285.D
Acq On : 11 Nov 2024 12:24
Operator : RC/JU
Sample : PB164576BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK576

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111124\
Data File : BG063285.D
Acq On : 11 Nov 2024 12:24
Operator : RC/JU
Sample : PB164576BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK576

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------