

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111124\
 Data File : BG063293.D
 Acq On : 11 Nov 2024 17:45
 Operator : RC/JU
 Sample : PB164614BL
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK614

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG063293.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.301	31	36	38	rBV3	22332	27262	0.72%	0.074%
2	3.506	70	71	74	rVB3	6698	5304	0.14%	0.014%
3	3.700	100	104	116	rBV	267658	436366	11.47%	1.192%
4	4.041	155	162	164	rBV5	8837	14723	0.39%	0.040%
5	4.158	178	182	183	rBV4	5620	5773	0.15%	0.016%
6	4.787	287	289	293	rVB3	5580	6445	0.17%	0.018%
7	4.981	320	322	325	rBV3	5043	5944	0.16%	0.016%
8	5.563	417	421	424	rVB4	6358	7711	0.20%	0.021%
9	7.008	658	667	678	rBV	404945	712179	18.72%	1.945%
10	7.161	687	693	701	rBV	281913	478085	12.57%	1.305%
11	7.366	721	728	738	rBV	394877	659589	17.34%	1.801%
12	7.831	800	807	816	rBV	336542	573485	15.08%	1.566%
13	7.995	834	835	839	rVB3	6703	5920	0.16%	0.016%
14	8.224	872	874	879	rBV2	3263	5276	0.14%	0.014%
15	8.306	884	888	891	rBV4	3637	5493	0.14%	0.015%
16	8.541	921	928	935	rBV2	549808	914444	24.04%	2.497%
17	8.777	965	968	971	rBV3	4729	5464	0.14%	0.015%
18	8.988	997	1004	1016	rBV	407807	711484	18.71%	1.943%
19	9.288	1051	1055	1059	rVB4	4220	5415	0.14%	0.015%
20	9.429	1074	1079	1082	rVB3	4477	6246	0.16%	0.017%
21	9.711	1118	1127	1136	rBV	385965	695867	18.29%	1.900%
22	10.251	1211	1219	1229	rBV2	591304	1075414	28.27%	2.936%
23	10.621	1275	1282	1291	rBV	550361	1000908	26.31%	2.733%
24	10.757	1298	1305	1315	rBV	568423	1057782	27.81%	2.888%
25	12.220	1549	1554	1556	rBV3	10848	16394	0.43%	0.045%
26	12.243	1556	1558	1562	rVB2	5965	6853	0.18%	0.019%
27	12.666	1625	1630	1631	rBV2	4575	6081	0.16%	0.017%
28	13.277	1730	1734	1737	rBV4	4657	5158	0.14%	0.014%
29	13.453	1763	1764	1770	rVB4	5237	5246	0.14%	0.014%
30	13.524	1772	1776	1779	rVB	3590	5318	0.14%	0.015%
31	13.882	1830	1837	1843	rBV	1189753	1802322	47.38%	4.921%
32	14.164	1878	1885	1894	rBV	1313997	2102692	55.28%	5.742%
33	14.476	1930	1938	1948	rBV	1108705	1705534	44.84%	4.657%
34	14.681	1967	1973	1993	rBV	373617	715309	18.81%	1.953%
35	15.469	2099	2107	2118	rBV	1849612	2800810	73.63%	7.648%
36	15.592	2123	2128	2137	rBV	500315	788508	20.73%	2.153%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111124\
 Data File : BG063293.D
 Acq On : 11 Nov 2024 17:45
 Operator : RC/JU
 Sample : PB164614BL
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK614

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
 Title : SVOA CALIBRATION

37	15.715	2145	2149	2152	rVB3	13268	18160	0.48%	0.050%
38	16.050	2204	2206	2208	rVB	5952	5361	0.14%	0.015%
39	16.262	2237	2242	2245	rBV3	5823	8871	0.23%	0.024%
40	16.714	2317	2319	2323	rVB3	5618	9135	0.24%	0.025%
41	16.844	2340	2341	2345	rVB3	5360	5419	0.14%	0.015%
42	16.908	2348	2352	2356	rVB4	5886	10179	0.27%	0.028%
43	16.996	2361	2367	2368	rVV3	5531	9170	0.24%	0.025%
44	17.008	2368	2369	2374	rVB4	10373	12528	0.33%	0.034%
45	17.225	2397	2406	2416	rBV	1508761	2201617	57.88%	6.012%
46	17.325	2416	2423	2434	rVV2	2096994	3131783	82.33%	8.551%
47	17.496	2450	2452	2455	rBV4	5590	6294	0.17%	0.017%
48	17.866	2511	2515	2518	rBV2	6134	9100	0.24%	0.025%
49	18.083	2550	2552	2554	rBV3	6214	5120	0.13%	0.014%
50	18.136	2558	2561	2563	rVB3	5784	6484	0.17%	0.018%
51	18.207	2571	2573	2576	rVB2	7053	6464	0.17%	0.018%
52	18.465	2614	2617	2620	rBV3	7617	10595	0.28%	0.029%
53	18.536	2626	2629	2632	rBV4	5699	7633	0.20%	0.021%
54	18.583	2636	2637	2641	rBV2	4417	5849	0.15%	0.016%
55	18.624	2641	2644	2647	rBV3	7124	11150	0.29%	0.030%
56	18.694	2653	2656	2657	rBV3	5980	5415	0.14%	0.015%
57	19.188	2735	2740	2744	rBV4	38728	51552	1.36%	0.141%
58	19.258	2748	2752	2757	rBV	31359	45761	1.20%	0.125%
59	19.505	2791	2794	2795	rBV3	6570	6756	0.18%	0.018%
60	19.623	2807	2814	2823	rBV	2673818	3803709	100.00%	10.386%
61	19.911	2860	2863	2867	rBV6	6258	10459	0.27%	0.029%
62	19.946	2867	2869	2870	rBV2	7508	5841	0.15%	0.016%
63	20.510	2963	2965	2967	rBV3	8977	6860	0.18%	0.019%
64	21.479	3124	3130	3143	rBV2	1604808	2534401	66.63%	6.920%
65	24.311	3602	3612	3624	rBV	1425757	3694417	97.13%	10.088%
66	24.517	3637	3647	3659	rVB	969345	2593732	68.19%	7.082%




Sum of corrected areas: 36622619

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111124\
Data File : BG063293.D
Acq On : 11 Nov 2024 17:45
Operator : RC/JU
Sample : PB164614BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK614

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

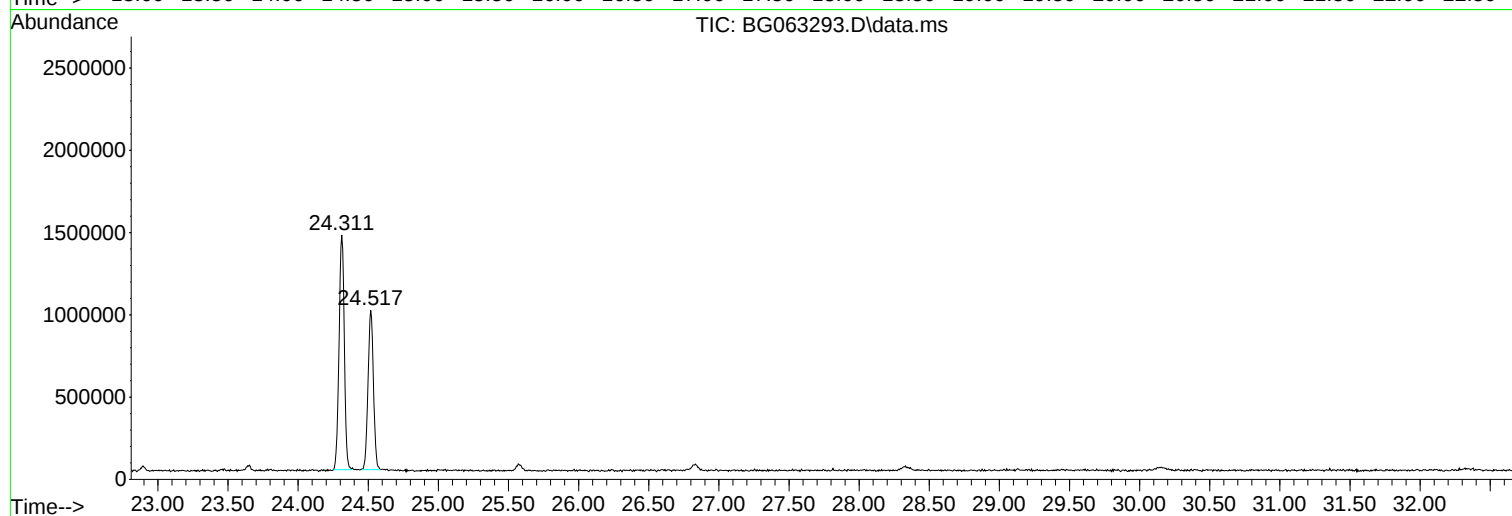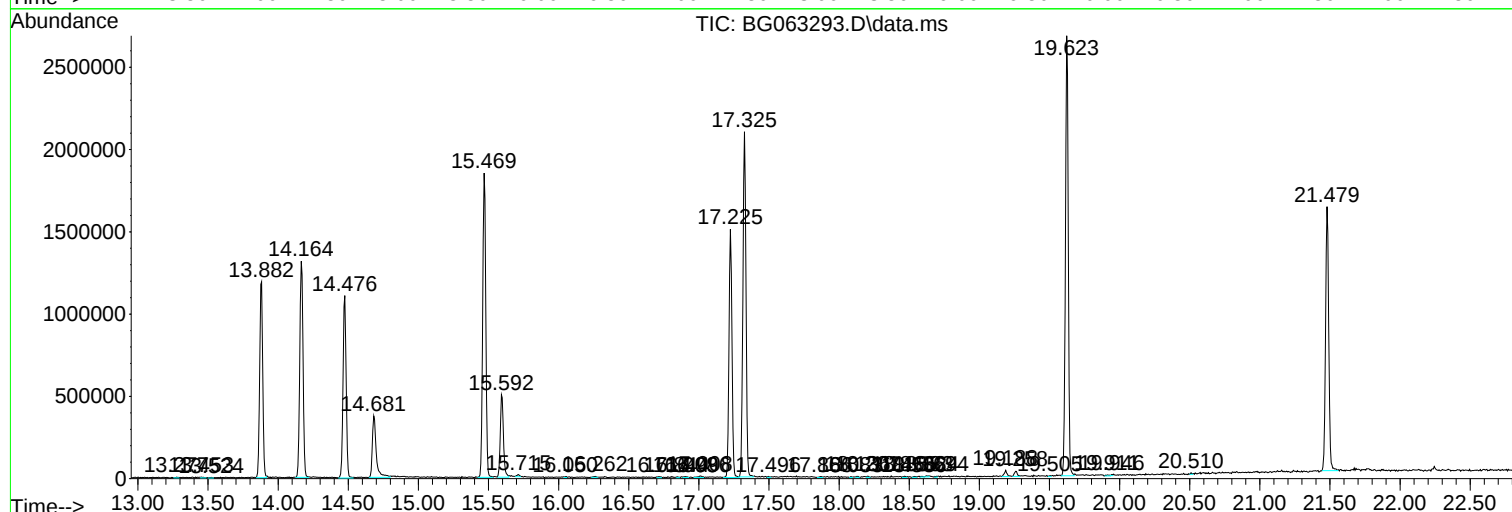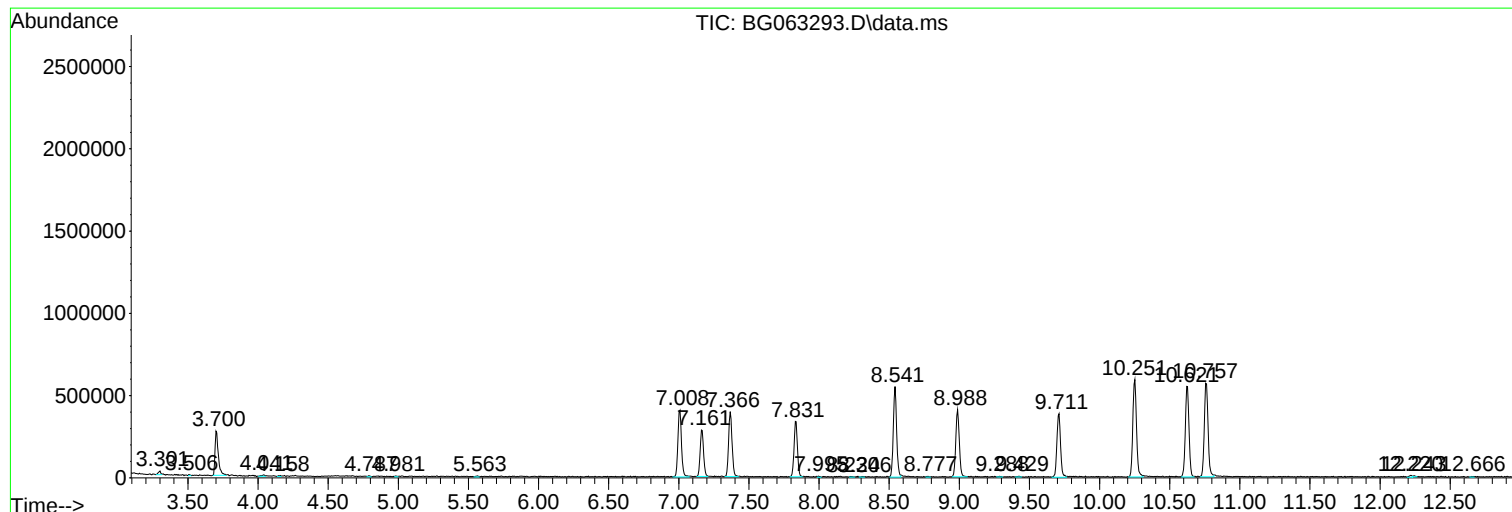

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111124\
Data File : BG063293.D
Acq On : 11 Nov 2024 17:45
Operator : RC/JU
Sample : PB164614BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK614

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111124\
Data File : BG063293.D
Acq On : 11 Nov 2024 17:45
Operator : RC/JU
Sample : PB164614BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK614

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc