

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111124\
Data File : BG063295.D
Acq On : 11 Nov 2024 19:01
Operator : RC/JU
Sample : P4644-08
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0CG1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
Title : SVOA CALIBRATION

Signal : TIC: BG063295.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.299	33	36	39	rBV4	20080	23191	0.50%	0.060%
2	3.710	102	106	113	rBV2	53901	97302	2.10%	0.253%
3	4.568	244	252	257	rBV2	76179	131784	2.84%	0.343%
4	7.006	660	667	675	rBV2	121092	222080	4.78%	0.578%
5	7.165	688	694	702	rVB	320828	518725	11.17%	1.350%
6	7.371	721	729	737	rBV	376241	644801	13.88%	1.678%
7	7.835	800	808	815	rBV	347956	574529	12.37%	1.495%
8	8.540	919	928	938	rBV	369033	667751	14.38%	1.738%
9	8.986	996	1004	1012	rBV	448106	790898	17.03%	2.059%
10	9.198	1034	1040	1045	rBV6	13419	37412	0.81%	0.097%
11	9.427	1074	1079	1082	rVB7	8409	12988	0.28%	0.034%
12	9.492	1085	1090	1093	rBV4	5851	8068	0.17%	0.021%
13	9.709	1119	1127	1136	rBV2	414844	747793	16.10%	1.946%
14	10.250	1212	1219	1233	rBV2	632761	1137317	24.49%	2.960%
15	10.408	1239	1246	1248	rBV5	11418	22079	0.48%	0.057%
16	10.626	1275	1283	1292	rBV	563703	993264	21.39%	2.585%
17	10.761	1297	1306	1317	rBV	392580	755480	16.27%	1.966%
18	11.448	1420	1423	1427	rVB4	10451	13153	0.28%	0.034%
19	11.907	1499	1501	1505	rVB3	6445	8251	0.18%	0.021%
20	12.218	1549	1554	1557	rBV4	11272	16117	0.35%	0.042%
21	13.763	1811	1817	1822	rVB2	4209	7775	0.17%	0.020%
22	13.881	1830	1837	1844	rBV	1394985	1968548	42.39%	5.124%
23	14.163	1876	1885	1893	rBV	1370044	2196414	47.30%	5.717%
24	14.474	1930	1938	1947	rBV	1124644	1694239	36.48%	4.410%
25	14.686	1969	1974	1983	rBV2	92856	204162	4.40%	0.531%
26	15.273	2071	2074	2075	rBV4	7160	7098	0.15%	0.018%
27	15.467	2100	2107	2121	rBV	1948949	3101632	66.79%	8.073%
28	15.590	2122	2128	2139	rBV	662644	1020681	21.98%	2.657%
29	15.831	2164	2169	2177	rVB	107083	157815	3.40%	0.411%
30	16.395	2262	2265	2269	rVB2	33098	47533	1.02%	0.124%
31	16.572	2290	2295	2298	rBV4	5431	8115	0.17%	0.021%
32	16.713	2317	2319	2325	rVB4	7417	10978	0.24%	0.029%
33	16.901	2350	2351	2356	rVB4	7047	8691	0.19%	0.023%
34	17.100	2381	2385	2388	rVB5	6717	8768	0.19%	0.023%
35	17.224	2400	2406	2415	rBV	1474580	2227685	47.97%	5.798%
36	17.324	2416	2423	2431	rVV2	2570359	3727586	80.27%	9.703%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111124\
 Data File : BG063295.D
 Acq On : 11 Nov 2024 19:01
 Operator : RC/JU
 Sample : P4644-08
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0CG1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
 Title : SVOA CALIBRATION

37	17.418	2436	2439	2444	rVB4	7788	8988	0.19%	0.023%
38	17.594	2464	2469	2471	rBV3	8513	14908	0.32%	0.039%
39	17.894	2517	2520	2525	rVB5	17225	26236	0.56%	0.068%
40	18.064	2546	2549	2552	rBV2	4167	7027	0.15%	0.018%
41	18.129	2556	2560	2565	rVV5	20208	34315	0.74%	0.089%
42	18.546	2629	2631	2634	rVB4	9723	9002	0.19%	0.023%
43	18.605	2639	2641	2646	rVV5	14350	25099	0.54%	0.065%
44	18.646	2646	2648	2650	rVB3	9168	7115	0.15%	0.019%
45	18.969	2700	2703	2704	rBV3	11184	12301	0.26%	0.032%
46	19.186	2736	2740	2744	rBV3	39655	56825	1.22%	0.148%
47	19.257	2748	2752	2757	rVB	35223	49701	1.07%	0.129%
48	19.503	2790	2794	2796	rBV5	21282	28407	0.61%	0.074%
49	19.621	2808	2814	2822	rBV	3407525	4643915	100.00%	12.088%
50	19.909	2860	2863	2864	rBV3	9599	11861	0.26%	0.031%
51	21.478	3124	3130	3137	rBV	1592394	2510118	54.05%	6.534%
52	24.310	3602	3612	3624	rBV2	1750223	4515148	97.23%	11.753%
53	24.515	3638	3647	3659	rVB	1005605	2636918	56.78%	6.864%




Sum of corrected areas: 38418587

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111124\
Data File : BG063295.D
Acq On : 11 Nov 2024 19:01
Operator : RC/JU
Sample : P4644-08
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0CG1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

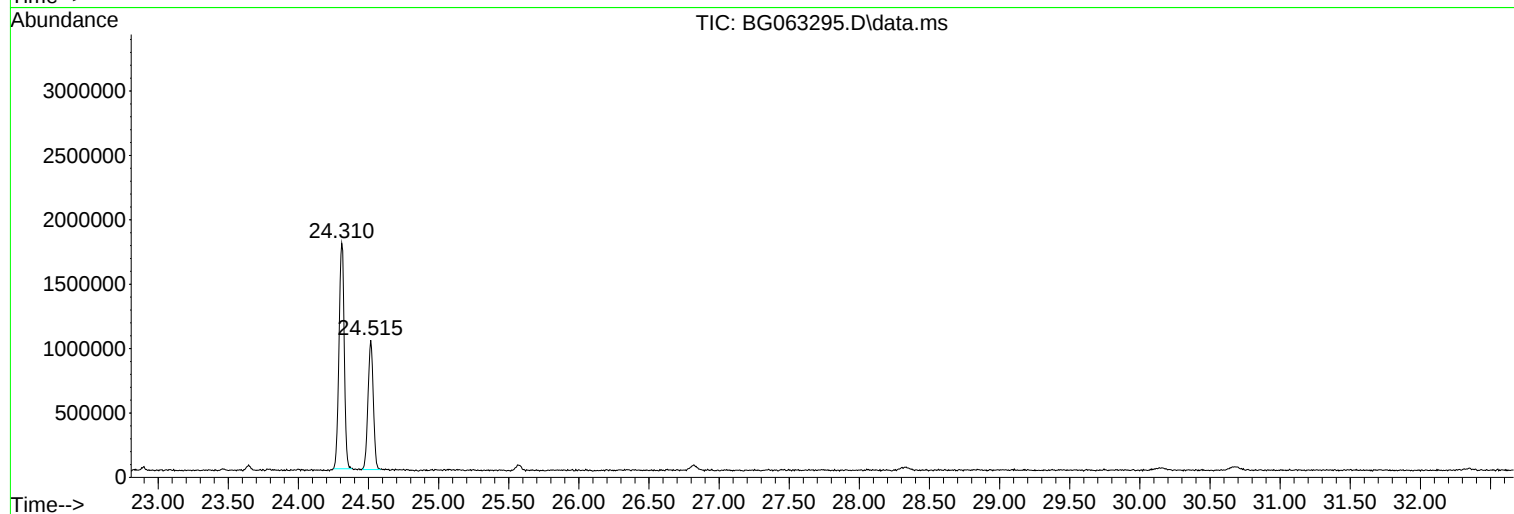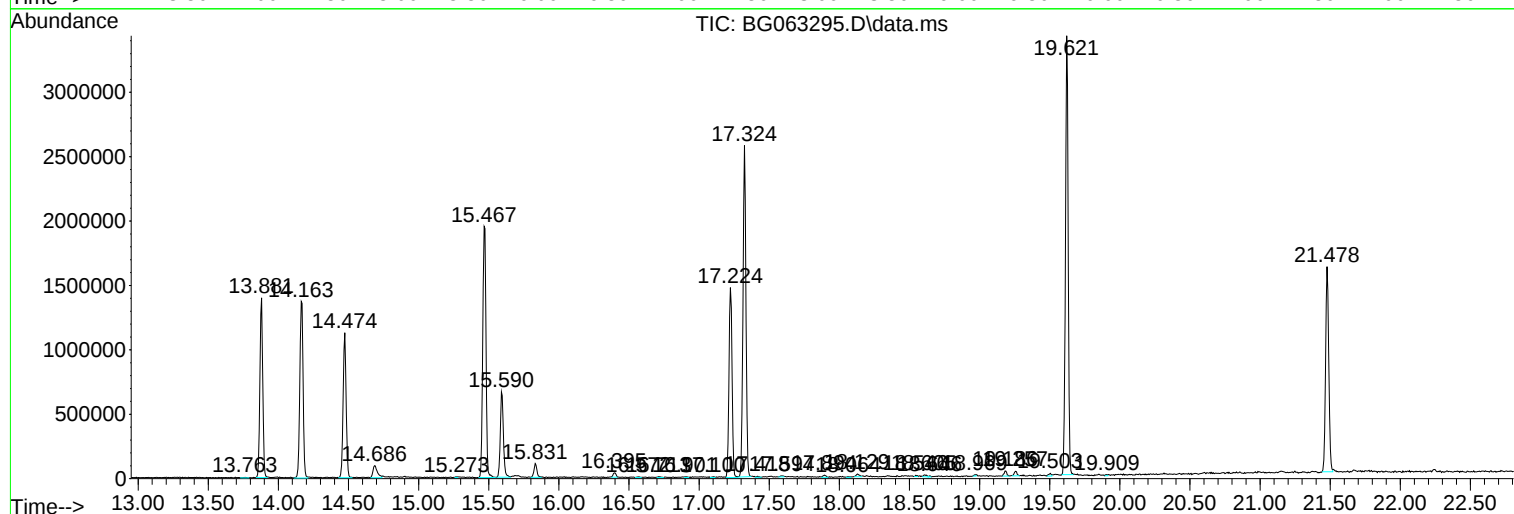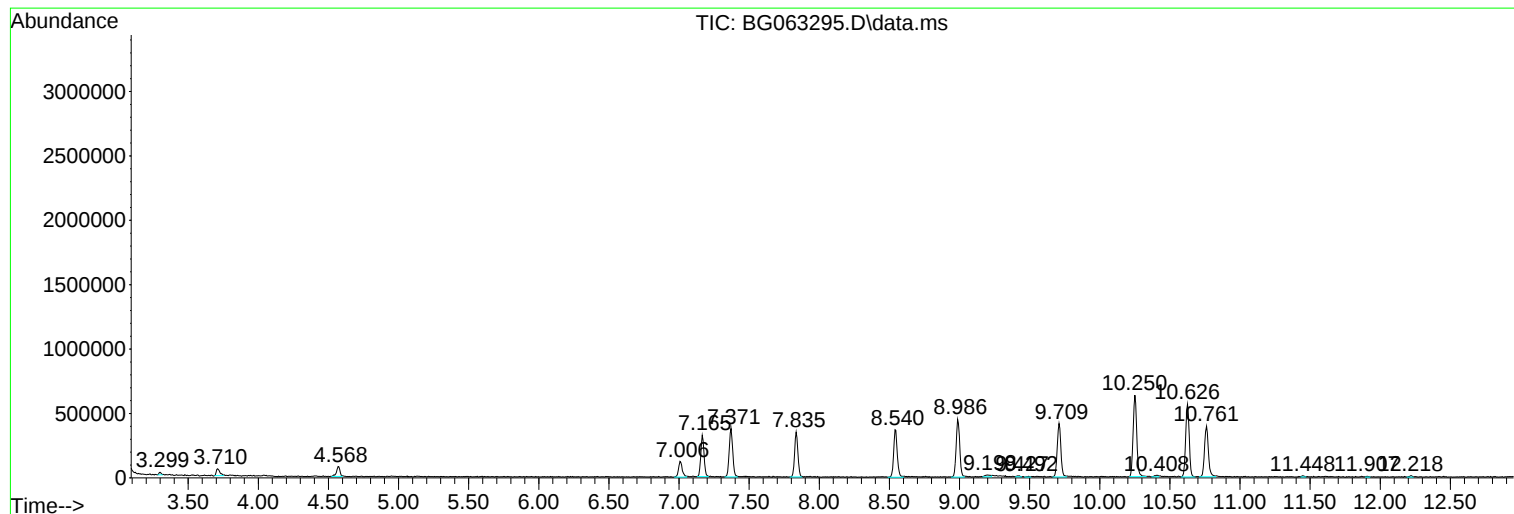

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111124\
Data File : BG063295.D
Acq On : 11 Nov 2024 19:01
Operator : RC/JU
Sample : P4644-08
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0CG1










Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Tetrachloroethylene Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.568	4.59 ng/ul	131784	1,4-Dichlorobenzene-d4	7.835

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Tetrachloroethylene	164	C2Cl4	000127-18-4	96
2			Tetrachloroethylene	164	C2Cl4	000127-18-4	95
3			Tetrachloroethylene	164	C2Cl4	000127-18-4	94
4			Tetrachloroethylene	164	C2Cl4	000127-18-4	90
5			Pyrimidine, 5-fluoro-2,4-dichloro-	166	C4HC12FN2	002927-71-1	27

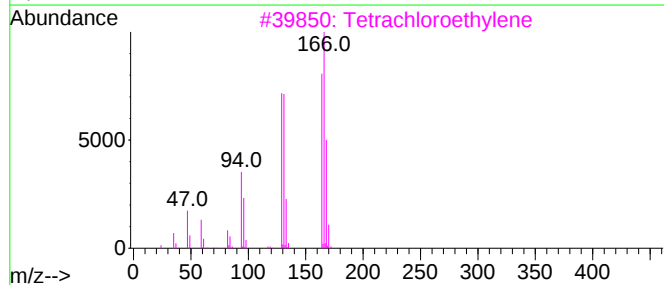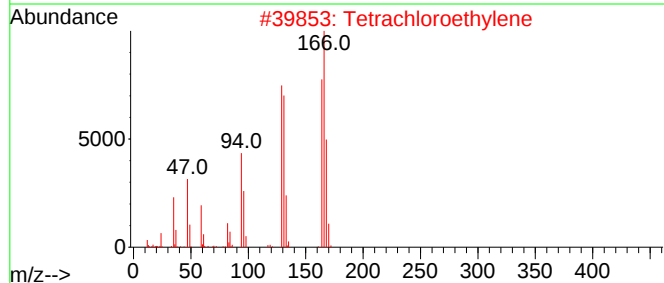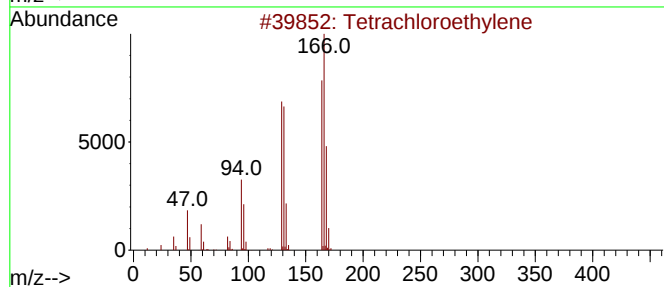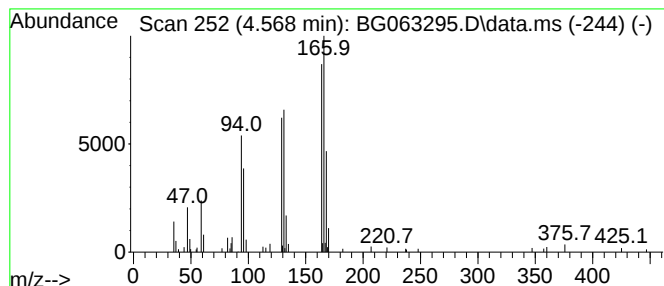

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111124\
Data File : BG063295.D
Acq On : 11 Nov 2024 19:01
Operator : RC/JU
Sample : P4644-08
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0CG1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Tetrachloroethy...	4.568	4.6	ng/u1	131784	1	7.835	574529	20.0