

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111124\
Data File : BG063302.D
Acq On : 11 Nov 2024 23:27
Operator : RC/JU
Sample : P4644-15
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0CF0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
Title : SVOA CALIBRATION

Signal : TIC: BG063302.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.300	33	36	41	rBV5	28149	40150	0.86%	0.097%
2	3.711	103	106	113	rBV	45625	84819	1.81%	0.204%
3	4.093	168	171	174	rBV3	7424	10304	0.22%	0.025%
4	4.569	243	252	261	rBV2	911119	1472673	31.39%	3.542%
5	5.133	346	348	352	rBV4	8008	10043	0.21%	0.024%
6	6.484	572	578	579	rBV2	10606	11402	0.24%	0.027%
7	6.637	599	604	607	rBV3	4752	8649	0.18%	0.021%
8	7.007	659	667	678	rBV	161322	298447	6.36%	0.718%
9	7.166	685	694	703	rBV	352548	563154	12.00%	1.354%
10	7.371	721	729	737	rBV	390203	670451	14.29%	1.613%
11	7.465	740	745	746	rBV4	8058	9091	0.19%	0.022%
12	7.835	800	808	818	rBV2	398701	658426	14.04%	1.584%
13	8.540	922	928	935	rBV2	467366	783947	16.71%	1.886%
14	8.987	997	1004	1016	rBV	485775	846995	18.05%	2.037%
15	9.151	1027	1032	1034	rBV5	6653	8996	0.19%	0.022%
16	9.322	1059	1061	1066	rVB4	4541	6596	0.14%	0.016%
17	9.428	1075	1079	1082	rBV4	6566	6454	0.14%	0.016%
18	9.551	1096	1100	1102	rBV5	6946	9354	0.20%	0.022%
19	9.710	1119	1127	1135	rBV	466046	795352	16.95%	1.913%
20	10.250	1212	1219	1232	rBV	677098	1226265	26.14%	2.949%
21	10.626	1275	1283	1290	rBV	625009	1101666	23.48%	2.650%
22	10.767	1299	1307	1316	rBV2	41600	95912	2.04%	0.231%
23	11.455	1417	1424	1425	rBV3	6797	7636	0.16%	0.018%
24	12.224	1549	1555	1559	rBV4	12318	22650	0.48%	0.054%
25	13.441	1759	1762	1767	rVB2	5425	9338	0.20%	0.022%
26	13.881	1830	1837	1845	rBV	1513578	2152922	45.89%	5.178%
27	14.163	1878	1885	1893	rBV2	1511124	2336492	49.80%	5.620%
28	14.475	1930	1938	1946	rBV	1239965	1919371	40.91%	4.616%
29	14.686	1968	1974	1986	rBV3	101515	217058	4.63%	0.522%
30	15.215	2062	2064	2068	rVB	7449	8859	0.19%	0.021%
31	15.468	2101	2107	2113	rBV	2172059	3303075	70.41%	7.945%
32	15.591	2122	2128	2136	rBV	684419	1043095	22.23%	2.509%
33	15.714	2146	2149	2154	rVB5	16580	19487	0.42%	0.047%
34	15.767	2156	2158	2163	rBV3	4205	6733	0.14%	0.016%
35	15.832	2163	2169	2175	rBV2	117774	180879	3.86%	0.435%
36	16.167	2223	2226	2227	rBV3	6762	6447	0.14%	0.016%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111124\
 Data File : BG063302.D
 Acq On : 11 Nov 2024 23:27
 Operator : RC/JU
 Sample : P4644-15
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0CF0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
 Title : SVOA CALIBRATION

37	16.314	2248	2251	2253	rBV3	5631	7041	0.15%	0.017%
38	16.355	2256	2258	2265	rBV5	5323	12305	0.26%	0.030%
39	16.707	2316	2318	2322	rVB4	6602	8048	0.17%	0.019%
40	17.224	2400	2406	2413	rBV	1627974	2412047	51.42%	5.801%
41	17.324	2416	2423	2434	rBV	2634298	3845062	81.96%	9.248%
42	17.506	2451	2454	2457	rBV2	8437	9312	0.20%	0.022%
43	17.589	2464	2468	2469	rBV2	8159	10714	0.23%	0.026%
44	17.894	2517	2520	2526	rVB6	11783	20165	0.43%	0.049%
45	18.123	2555	2559	2568	rBV2	96459	178516	3.81%	0.429%
46	18.188	2568	2570	2578	rVB6	10970	22392	0.48%	0.054%
47	18.417	2607	2609	2613	rBV4	6473	9310	0.20%	0.022%
48	18.617	2641	2643	2646	rBV4	8282	7822	0.17%	0.019%
49	19.187	2735	2740	2745	rBV3	38722	63674	1.36%	0.153%
50	19.257	2748	2752	2757	rVB	37013	55366	1.18%	0.133%
51	19.410	2775	2778	2783	rBV6	29321	53452	1.14%	0.129%
52	19.622	2808	2814	2821	rBV	3331102	4691288	100.00%	11.283%
53	19.927	2864	2866	2867	rBV2	6803	6444	0.14%	0.015%
54	20.521	2965	2967	2968	rBV2	12539	6986	0.15%	0.017%
55	20.791	3011	3013	3014	rBV2	12220	7182	0.15%	0.017%
56	21.372	3110	3112	3117	rVB2	31673	41375	0.88%	0.100%
57	21.478	3124	3130	3138	rBV2	1791723	2823203	60.18%	6.790%
58	24.310	3602	3612	3622	rBV	1739227	4425215	94.33%	10.644%
59	24.516	3637	3647	3660	rVB	1053919	2887145	61.54%	6.944%
60	24.957	3720	3722	3723	rBV2	16572	10526	0.22%	0.025%
61	28.940	4399	4400	4401	rBV	16434	8783	0.19%	0.021%




Sum of corrected areas: 41576561

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111124\
Data File : BG063302.D
Acq On : 11 Nov 2024 23:27
Operator : RC/JU
Sample : P4644-15
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0CF0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

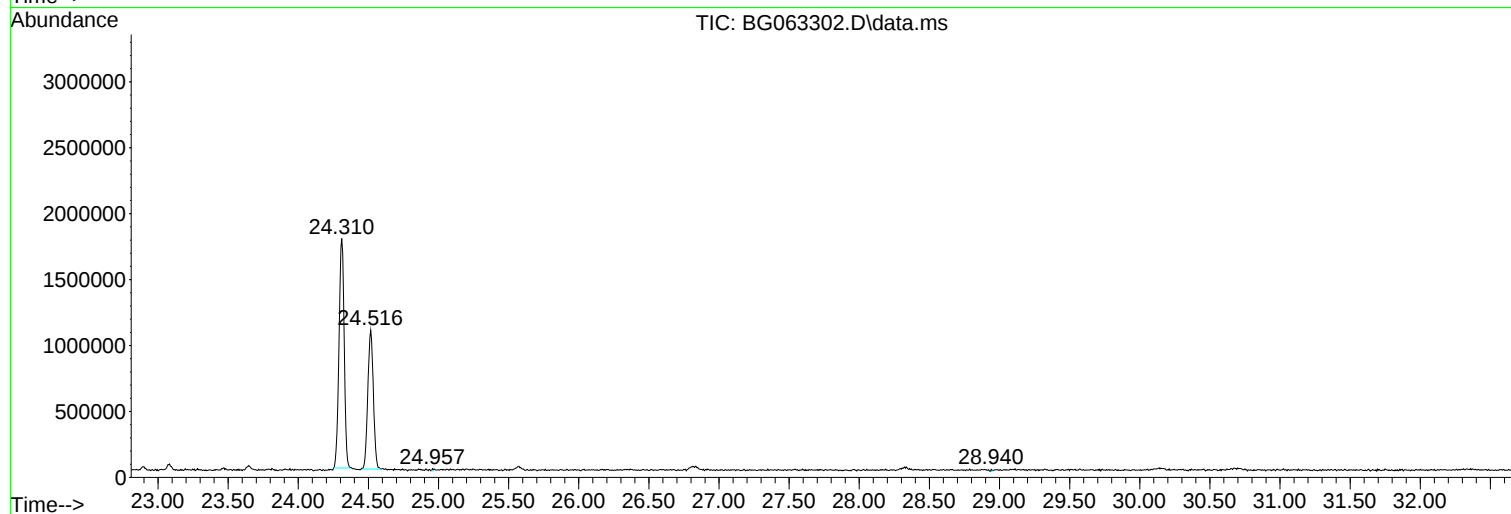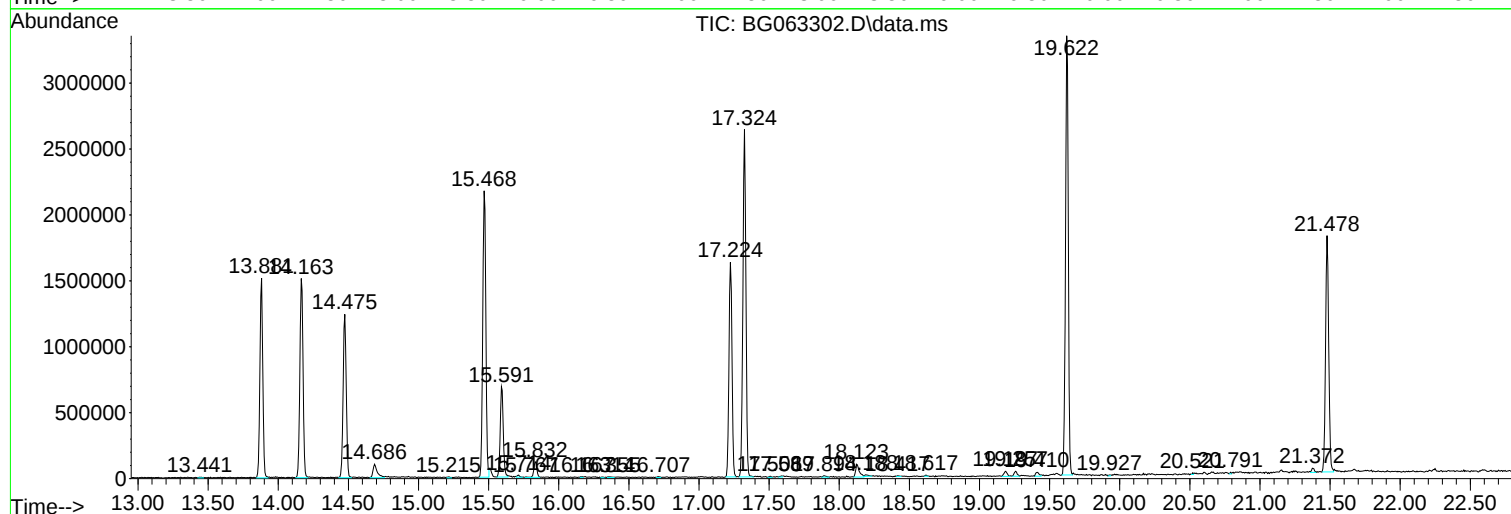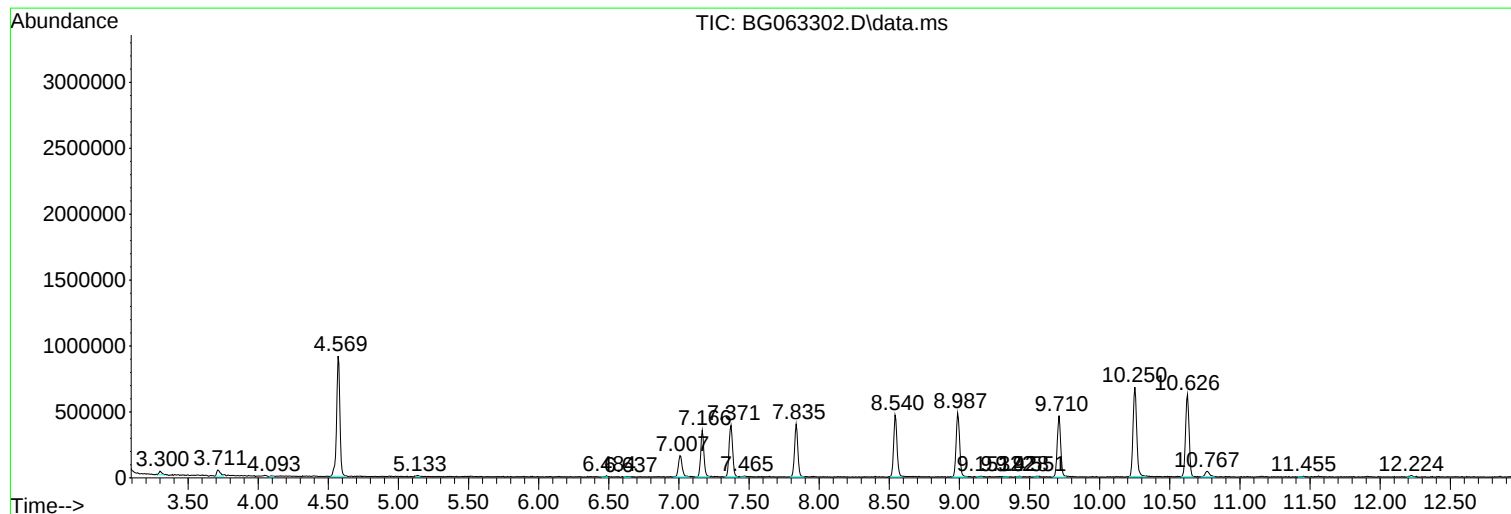

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111124\
Data File : BG063302.D
Acq On : 11 Nov 2024 23:27
Operator : RC/JU
Sample : P4644-15
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0CF0










Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Tetrachloroethylene Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.569	44.73 ng/ul	1472670	1,4-Dichlorobenzene-d4	7.835

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Tetrachloroethylene	164	C2Cl4	000127-18-4	97
2			Tetrachloroethylene	164	C2Cl4	000127-18-4	96
3			Tetrachloroethylene	164	C2Cl4	000127-18-4	94
4			Tetrachloroethylene	164	C2Cl4	000127-18-4	93
5			Pyrimidine, 5-fluoro-2,4-dichloro-	166	C4HC12FN2	002927-71-1	38

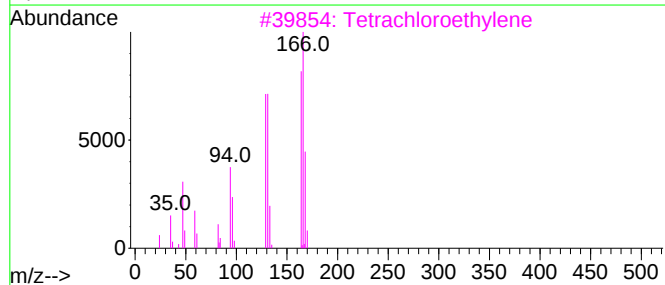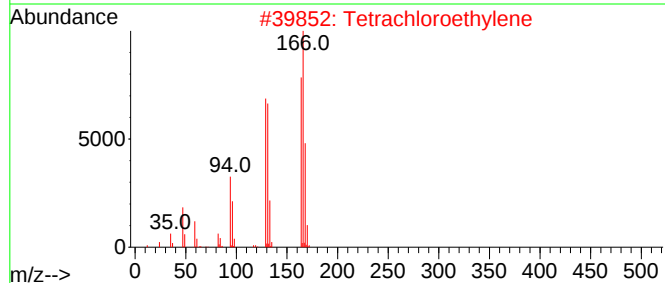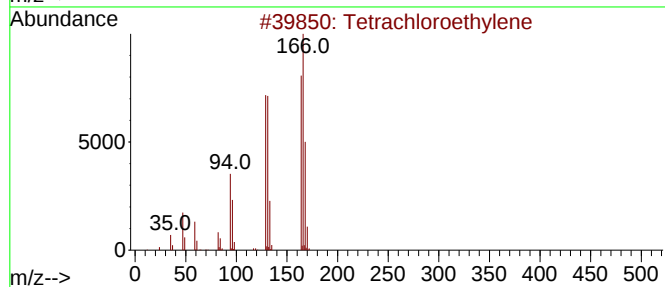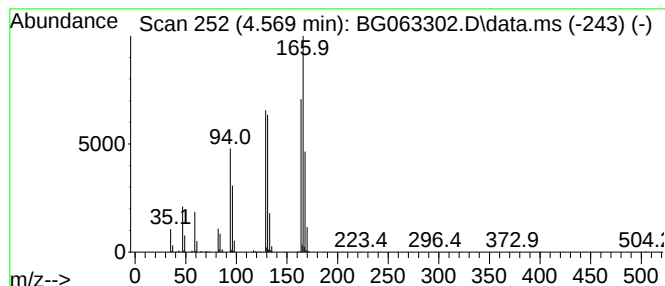

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111124\
Data File : BG063302.D
Acq On : 11 Nov 2024 23:27
Operator : RC/JU
Sample : P4644-15
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0CF0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Tetrachloroethy...	4.569	44.7	ng/ul	1472670	1	7.835	658426	20.0