

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111124\
 Data File : BG063303.D
 Acq On : 12 Nov 2024 00:05
 Operator : RC/JU
 Sample : P4644-16
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0CG3

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG063303.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.299	33	36	43	rVB3	28199	41075	0.86%	0.102%
2	3.710	102	106	111	rBV2	56301	91771	1.92%	0.227%
3	4.545	242	248	254	rBV	61854	90070	1.88%	0.223%
4	6.854	638	641	643	rBV3	6598	7068	0.15%	0.018%
5	7.012	659	668	679	rBV2	140184	287355	6.01%	0.712%
6	7.165	687	694	702	rBV	346875	575403	12.03%	1.425%
7	7.371	722	729	737	rBV	397995	672637	14.07%	1.666%
8	7.629	772	773	778	rBV3	4615	6467	0.14%	0.016%
9	7.835	801	808	816	rBV	365065	612038	12.80%	1.516%
10	8.540	922	928	936	rBV	441952	764004	15.98%	1.893%
11	8.987	995	1004	1013	rBV	509336	889259	18.60%	2.203%
12	9.410	1073	1076	1078	rBV3	5142	7093	0.15%	0.018%
13	9.556	1096	1101	1102	rBV5	6521	9147	0.19%	0.023%
14	9.709	1119	1127	1142	rBV	461163	836119	17.49%	2.071%
15	10.250	1211	1219	1236	rBV	695247	1271082	26.58%	3.149%
16	10.626	1276	1283	1291	rVB	592838	1027142	21.48%	2.544%
17	10.761	1296	1306	1315	rBV3	193069	397225	8.31%	0.984%
18	11.437	1417	1421	1431	rBV6	8994	24403	0.51%	0.060%
19	11.836	1484	1489	1492	rBV2	6055	11534	0.24%	0.029%
20	12.218	1550	1554	1560	rBV6	8620	17344	0.36%	0.043%
21	12.823	1653	1657	1664	rVB4	4354	7891	0.17%	0.020%
22	13.376	1748	1751	1754	rBV	6118	8369	0.18%	0.021%
23	13.440	1758	1762	1765	rVB4	4929	7724	0.16%	0.019%
24	13.881	1830	1837	1847	rBV	1509229	2181279	45.62%	5.404%
25	14.169	1875	1886	1893	rBV	1499216	2431640	50.86%	6.024%
26	14.474	1929	1938	1945	rBV	1147808	1792655	37.49%	4.441%
27	14.598	1955	1959	1960	rBV	5051	7520	0.16%	0.019%
28	14.692	1969	1975	1983	rBV2	94809	193352	4.04%	0.479%
29	14.891	2005	2009	2011	rBV4	7227	10548	0.22%	0.026%
30	15.068	2036	2039	2043	rBV2	6575	8715	0.18%	0.022%
31	15.326	2081	2083	2088	rVB3	5257	6902	0.14%	0.017%
32	15.467	2101	2107	2120	rVB	2224011	3482126	72.83%	8.626%
33	15.591	2122	2128	2141	rVV	711323	1094571	22.89%	2.712%
34	15.708	2144	2148	2154	rVB5	10295	21264	0.44%	0.053%
35	15.832	2165	2169	2177	rVB2	79533	114445	2.39%	0.284%
36	16.255	2237	2241	2245	rVB5	3906	6494	0.14%	0.016%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111124\
 Data File : BG063303.D
 Acq On : 12 Nov 2024 00:05
 Operator : RC/JU
 Sample : P4644-16
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0CG3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
 Title : SVOA CALIBRATION

37	16.760	2324	2327	2329	rBV4	6732	8134	0.17%	0.020%
38	17.001	2365	2368	2372	rBV6	7532	13311	0.28%	0.033%
39	17.089	2379	2383	2388	rVB5	7839	9707	0.20%	0.024%
40	17.224	2400	2406	2415	rBV	1577623	2350644	49.16%	5.823%
41	17.324	2415	2423	2434	rBV2	2631676	3926674	82.13%	9.727%
42	17.582	2463	2467	2468	rBV4	9425	10956	0.23%	0.027%
43	17.894	2517	2520	2524	rBV4	17002	19694	0.41%	0.049%
44	18.064	2546	2549	2552	rBV4	5467	7469	0.16%	0.019%
45	18.129	2556	2560	2569	rVV9	27938	56149	1.17%	0.139%
46	18.193	2569	2571	2575	rBV4	5292	7937	0.17%	0.020%
47	18.599	2638	2640	2641	rBV2	8792	7688	0.16%	0.019%
48	18.611	2641	2642	2646	rVB4	12460	12361	0.26%	0.031%
49	19.181	2736	2739	2744	rVB3	41004	57199	1.20%	0.142%
50	19.257	2747	2752	2757	rBV2	34646	57803	1.21%	0.143%
51	19.504	2790	2794	2799	rBV6	11860	26884	0.56%	0.067%
52	19.621	2808	2814	2821	rBV	3373403	4781308	100.00%	11.844%
53	20.056	2886	2888	2889	rBV2	9967	6908	0.14%	0.017%
54	20.738	3002	3004	3006	rBV3	11804	8248	0.17%	0.020%
55	21.478	3124	3130	3139	rBV2	1702943	2709332	56.67%	6.712%
56	24.310	3602	3612	3625	rVB	1739084	4442150	92.91%	11.004%
57	24.515	3638	3647	3660	rVB2	1075377	2833234	59.26%	7.019%




Sum of corrected areas: 40367521

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111124\
Data File : BG063303.D
Acq On : 12 Nov 2024 00:05
Operator : RC/JU
Sample : P4644-16
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0CG3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

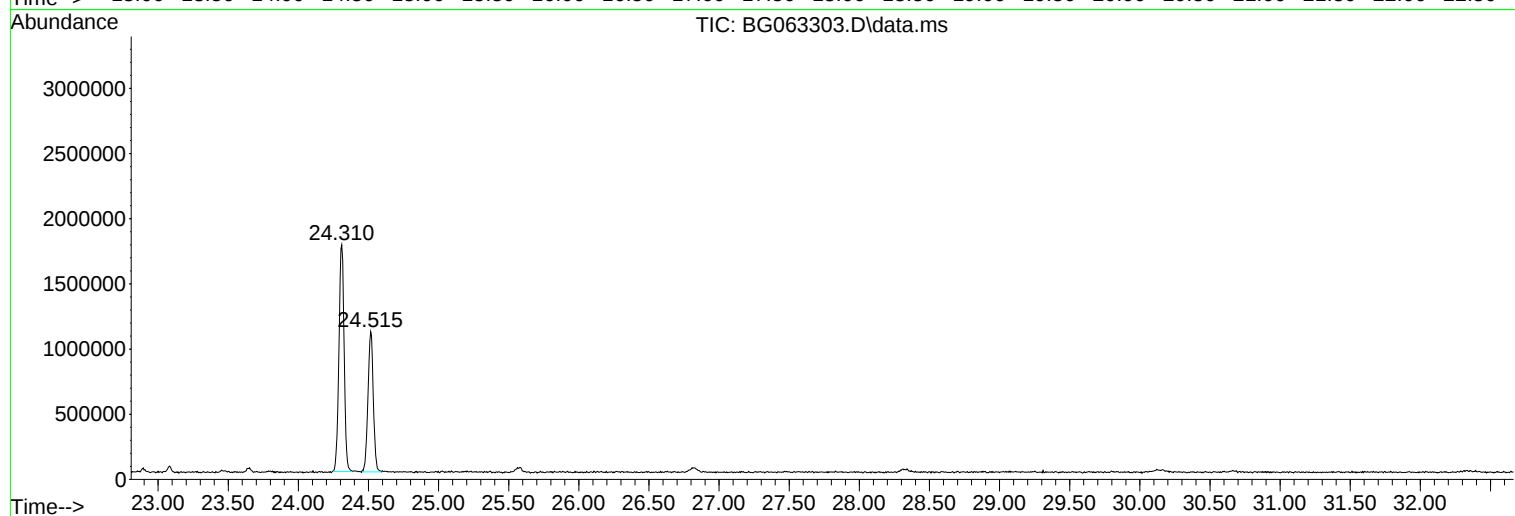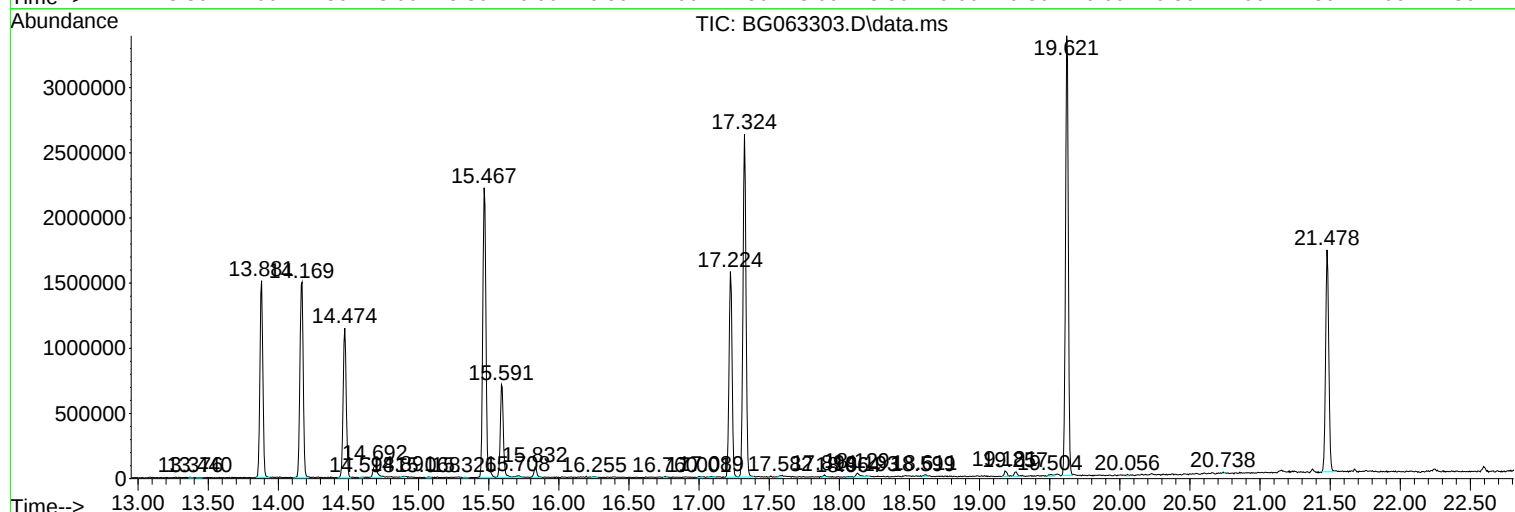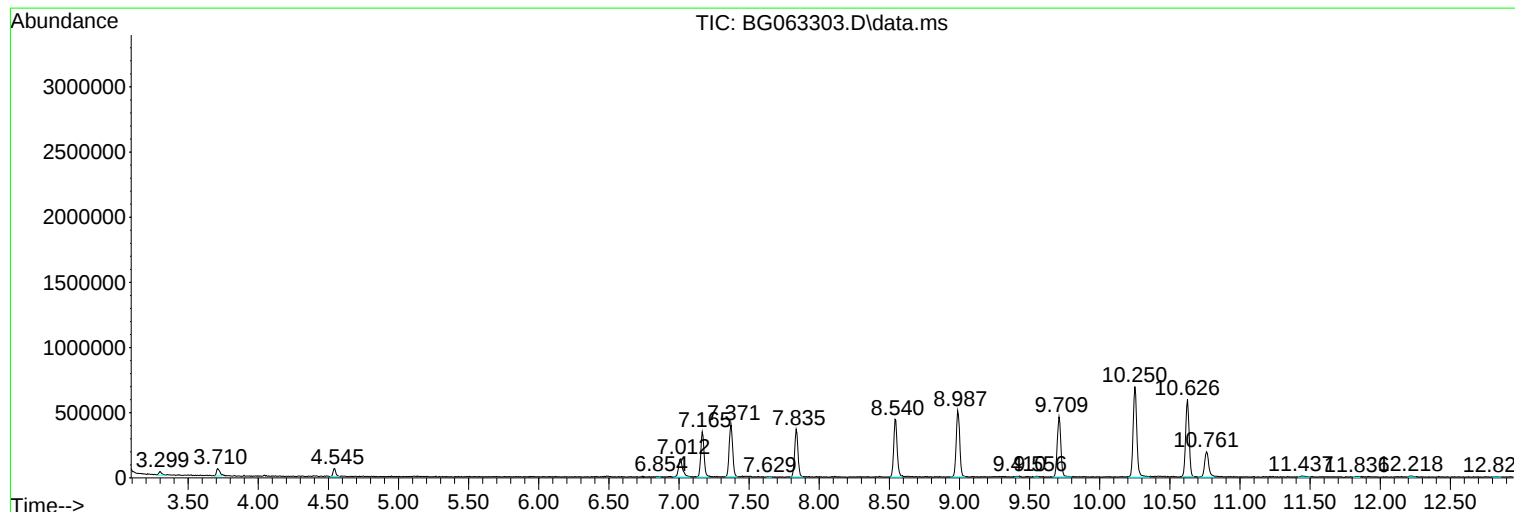

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111124\
Data File : BG063303.D
Acq On : 12 Nov 2024 00:05
Operator : RC/JU
Sample : P4644-16
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0CG3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111124\
Data File : BG063303.D
Acq On : 12 Nov 2024 00:05
Operator : RC/JU
Sample : P4644-16
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0CG3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------