

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111124\
 Data File : BG063306.D
 Acq On : 12 Nov 2024 1:59
 Operator : RC/JU
 Sample : P4644-11
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0CF4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG063306.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.300	33	36	40	rVB4	21185	26065	0.55%	0.064%
2	3.711	102	106	116	rBV	86476	138067	2.91%	0.341%
3	4.040	160	162	167	rVB3	11419	15351	0.32%	0.038%
4	4.393	219	222	223	rBV3	7812	6622	0.14%	0.016%
5	4.481	233	237	240	rBV5	8021	9487	0.20%	0.023%
6	4.546	244	248	250	rVV4	8493	9988	0.21%	0.025%
7	4.951	314	317	319	rBV3	6268	7859	0.17%	0.019%
8	7.007	660	667	674	rBV	165225	294557	6.21%	0.727%
9	7.166	687	694	703	rBV	353149	567377	11.97%	1.400%
10	7.372	722	729	738	rBV	428895	729057	15.38%	1.799%
11	7.460	742	744	748	rBV4	4702	6849	0.14%	0.017%
12	7.836	802	808	815	rBV	375081	630288	13.29%	1.555%
13	8.030	839	841	846	rBV2	6621	7409	0.16%	0.018%
14	8.447	907	912	916	rBV5	9875	20810	0.44%	0.051%
15	8.541	920	928	937	rBV	444545	777016	16.39%	1.917%
16	8.864	980	983	988	rVB3	4334	6899	0.15%	0.017%
17	8.987	996	1004	1013	rBV	501011	869039	18.33%	2.144%
18	9.205	1036	1041	1042	rBV3	8391	12048	0.25%	0.030%
19	9.710	1120	1127	1136	rBV	457393	802381	16.92%	1.979%
20	10.251	1209	1219	1231	rBV	699051	1265644	26.70%	3.122%
21	10.627	1274	1283	1293	rVB	605132	1078472	22.75%	2.660%
22	10.762	1297	1306	1316	rBV	487635	929756	19.61%	2.294%
23	11.602	1447	1449	1453	rVB3	6010	7178	0.15%	0.018%
24	11.902	1496	1500	1502	rBV2	6611	6954	0.15%	0.017%
25	12.225	1549	1555	1557	rBV5	8714	14329	0.30%	0.035%
26	12.660	1626	1629	1632	rBV4	7283	7796	0.16%	0.019%
27	13.088	1698	1702	1705	rBV3	4191	6901	0.15%	0.017%
28	13.876	1829	1836	1848	rBV	1429715	2121571	44.75%	5.234%
29	14.070	1865	1869	1873	rVB3	5893	9437	0.20%	0.023%
30	14.164	1878	1885	1893	rBV	1536234	2342411	49.41%	5.778%
31	14.475	1931	1938	1946	rBV	1148505	1815946	38.30%	4.480%
32	14.687	1968	1974	1988	rBV2	139229	296294	6.25%	0.731%
33	15.327	2081	2083	2088	rBV3	4984	7882	0.17%	0.019%
34	15.468	2099	2107	2120	rBV	2145822	3191514	67.32%	7.873%
35	15.591	2122	2128	2140	rBV	759446	1106165	23.33%	2.729%
36	15.832	2164	2169	2174	rBV2	28637	41222	0.87%	0.102%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111124\
Data File : BG063306.D
Acq On : 12 Nov 2024 1:59
Operator : RC/JU
Sample : P4644-11
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0CF4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
Title : SVOA CALIBRATION

37	16.255	2237	2241	2242	rBV2	5930	6969	0.15%	0.017%
38	16.526	2284	2287	2289	rVB3	8271	6919	0.15%	0.017%
39	16.761	2324	2327	2330	rBV5	8505	10530	0.22%	0.026%
40	17.013	2365	2370	2373	rVB5	5902	10255	0.22%	0.025%
41	17.225	2400	2406	2416	rBV	1603128	2343333	49.43%	5.781%
42	17.325	2416	2423	2434	rVV	2654277	3822170	80.62%	9.429%
43	17.595	2465	2469	2471	rBV3	13088	19741	0.42%	0.049%
44	17.895	2517	2520	2525	rVB6	7924	11613	0.24%	0.029%
45	18.024	2540	2542	2545	rVB2	10844	6839	0.14%	0.017%
46	18.130	2556	2560	2562	rBV3	23666	33820	0.71%	0.083%
47	18.188	2569	2570	2575	rVB5	10024	10093	0.21%	0.025%
48	18.365	2599	2600	2605	rBV3	5492	8595	0.18%	0.021%
49	18.617	2639	2643	2645	rBV5	22110	23261	0.49%	0.057%
50	18.694	2654	2656	2660	rVB5	7295	9594	0.20%	0.024%
51	18.729	2660	2662	2664	rBV3	7604	6671	0.14%	0.016%
52	19.187	2736	2740	2744	rBV2	41863	61111	1.29%	0.151%
53	19.264	2747	2753	2756	rBV2	36620	65576	1.38%	0.162%
54	19.622	2808	2814	2821	rBV	3442538	4741117	100.00%	11.696%
55	20.004	2877	2879	2880	rBV2	10279	8208	0.17%	0.020%
56	20.597	2976	2980	2983	rBV6	17847	30402	0.64%	0.075%
57	21.479	3124	3130	3137	rBV	1772205	2692314	56.79%	6.642%
58	23.647	3495	3499	3509	rVB8	41480	98843	2.08%	0.244%
59	24.311	3602	3612	3623	rVB	1808546	4563470	96.25%	11.258%
60	24.516	3637	3647	3658	rVB	1018579	2758582	58.18%	6.805%




Sum of corrected areas: 40536667

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111124\
Data File : BG063306.D
Acq On : 12 Nov 2024 1:59
Operator : RC/JU
Sample : P4644-11
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0CF4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

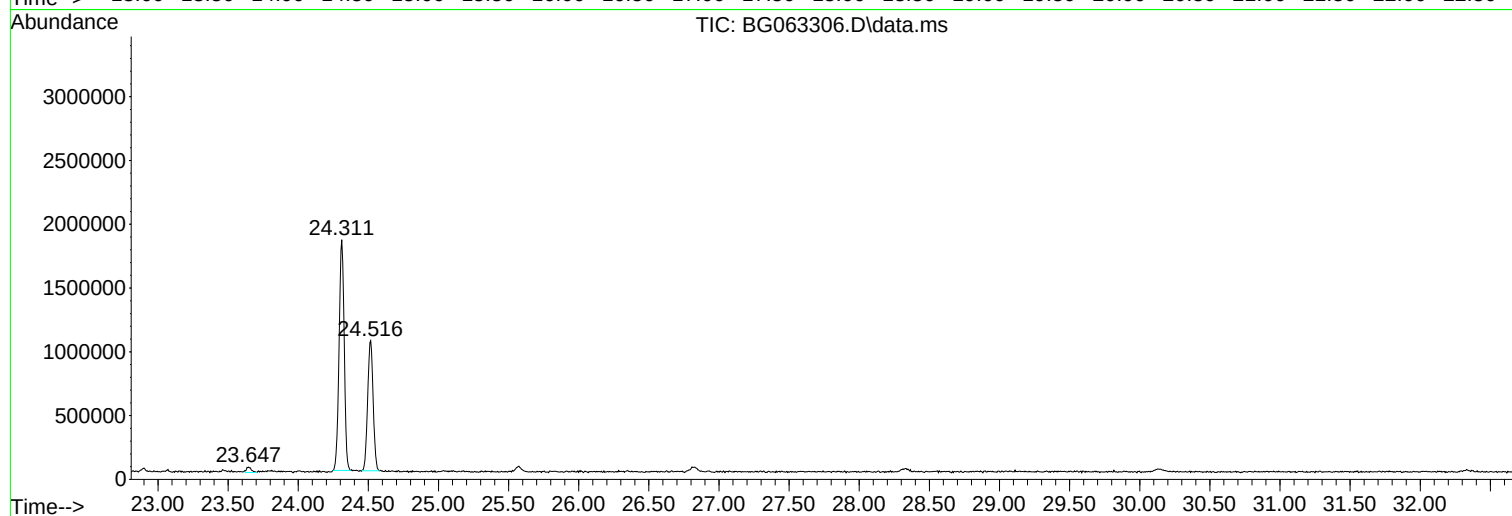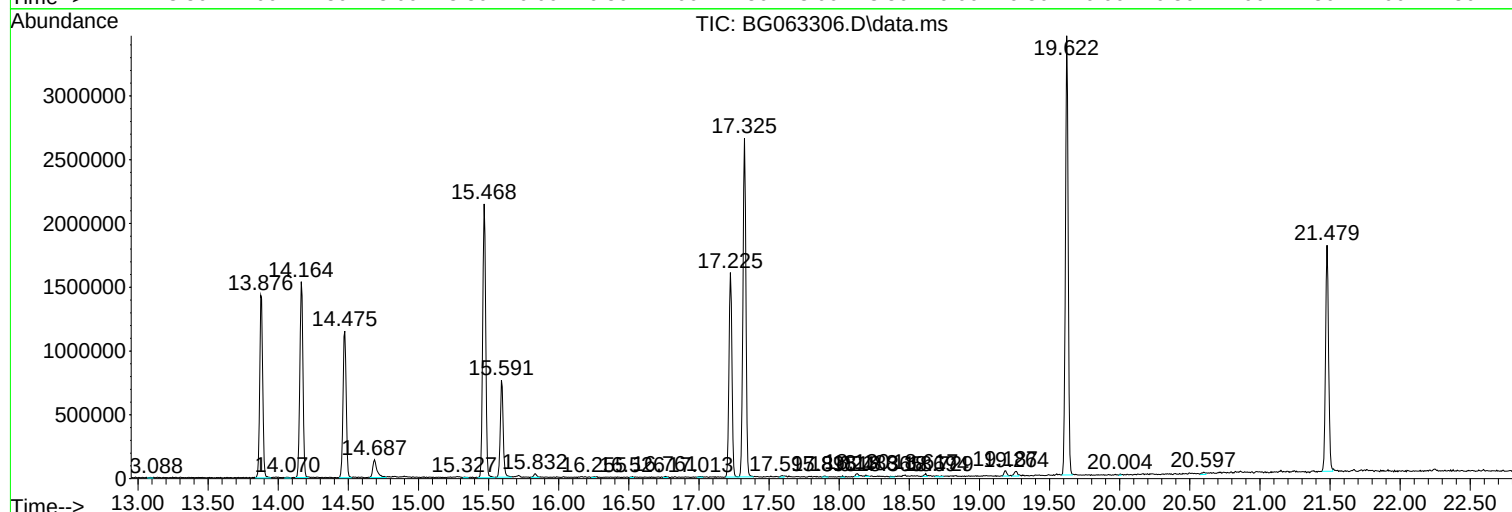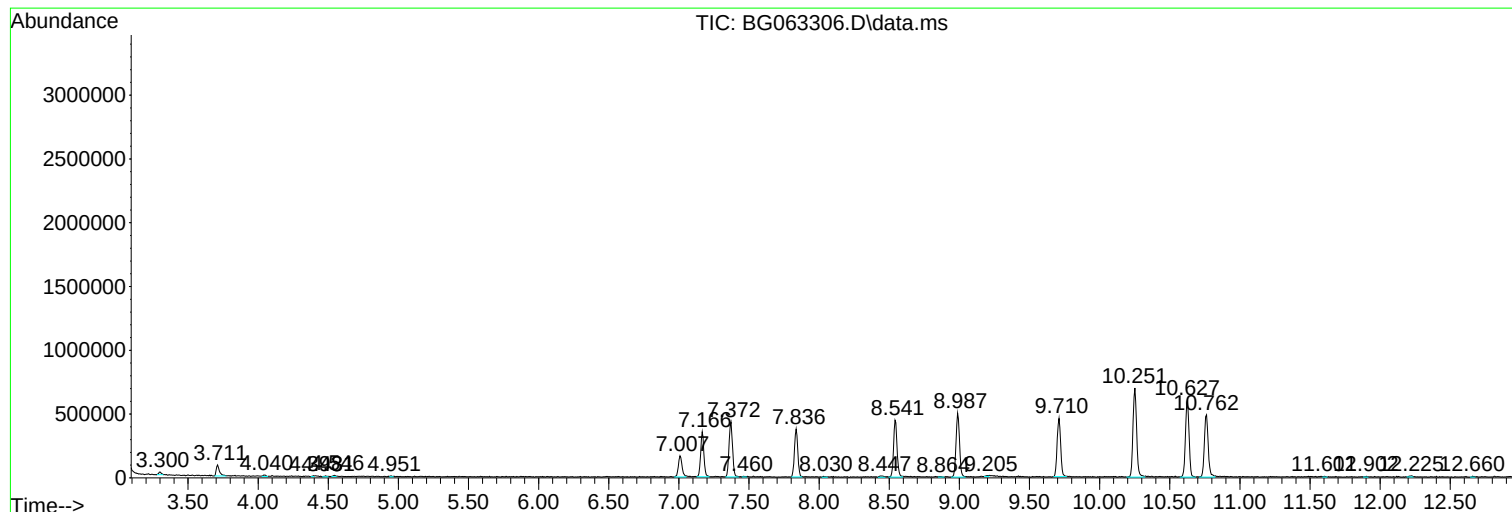

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111124\
Data File : BG063306.D
Acq On : 12 Nov 2024 1:59
Operator : RC/JU
Sample : P4644-11
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0CF4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111124\
Data File : BG063306.D
Acq On : 12 Nov 2024 1:59
Operator : RC/JU
Sample : P4644-11
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0CF4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc