

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111124\
 Data File : BG063309.D
 Acq On : 12 Nov 2024 4:31
 Operator : RC/JU
 Sample : PB164671BL
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK671

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG063309.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.297	32	35	40	rVB2	28839	41317	0.96%	0.098%
2	3.596	84	86	90	rVB4	8146	7093	0.17%	0.017%
3	3.702	100	104	115	rBV	323119	543828	12.69%	1.286%
4	4.043	160	162	167	rVB5	10086	13826	0.32%	0.033%
5	4.583	251	254	257	rBV4	5457	6532	0.15%	0.015%
6	5.001	323	325	327	rBV3	5333	6273	0.15%	0.015%
7	6.170	522	524	528	rVB2	4997	6174	0.14%	0.015%
8	7.010	657	667	675	rBV	481142	841940	19.64%	1.991%
9	7.169	688	694	701	rBV	347400	573101	13.37%	1.355%
10	7.368	720	728	739	rBV	481042	798080	18.62%	1.887%
11	7.621	768	771	775	rBV4	3595	6388	0.15%	0.015%
12	7.833	801	807	819	rVB2	416464	700500	16.34%	1.656%
13	8.543	920	928	939	rBV	673664	1142457	26.65%	2.701%
14	8.990	996	1004	1012	rBV	494984	869186	20.27%	2.055%
15	9.419	1075	1077	1082	rVB3	4721	6183	0.14%	0.015%
16	9.707	1119	1126	1133	rBV	474976	830865	19.38%	1.965%
17	10.253	1211	1219	1232	rBV	685224	1276538	29.78%	3.018%
18	10.623	1275	1282	1290	rBV	688003	1183687	27.61%	2.799%
19	10.759	1296	1305	1316	rBV	662489	1209365	28.21%	2.860%
20	12.221	1551	1554	1562	rVB4	9432	17796	0.42%	0.042%
21	13.138	1705	1710	1711	rBV	5368	6847	0.16%	0.016%
22	13.878	1829	1836	1846	rBV	1450423	2019006	47.10%	4.774%
23	13.990	1853	1855	1859	rVB4	5967	6903	0.16%	0.016%
24	14.166	1877	1885	1893	rBV2	1563845	2448266	57.11%	5.789%
25	14.413	1921	1927	1930	rBV3	5586	8592	0.20%	0.020%
26	14.472	1930	1937	1944	rBV	1307552	2001551	46.69%	4.733%
27	14.683	1967	1973	1984	rBV	469988	834166	19.46%	1.972%
28	14.924	2011	2014	2017	rBV4	3890	6065	0.14%	0.014%
29	15.100	2041	2044	2048	rBV3	4912	7914	0.18%	0.019%
30	15.465	2099	2106	2114	rBV	2006116	3132154	73.06%	7.406%
31	15.553	2119	2121	2122	rBV2	6720	5878	0.14%	0.014%
32	15.594	2122	2128	2137	rBV	604160	909397	21.21%	2.150%
33	15.700	2144	2146	2147	rBV2	8879	8277	0.19%	0.020%
34	16.082	2207	2211	2213	rVB2	5510	5947	0.14%	0.014%
35	16.182	2226	2228	2231	rBV3	5148	6409	0.15%	0.015%
36	16.716	2316	2319	2321	rBV3	5715	7196	0.17%	0.017%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111124\
 Data File : BG063309.D
 Acq On : 12 Nov 2024 4:31
 Operator : RC/JU
 Sample : PB164671BL
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK671

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
 Title : SVOA CALIBRATION

37	16.834	2338	2339	2343	rBV2	4850	5842	0.14%	0.014%
38	17.169	2392	2396	2398	rBV3	4867	7558	0.18%	0.018%
39	17.222	2398	2405	2415	rVB	1739237	2561400	59.75%	6.057%
40	17.321	2415	2422	2433	rBV2	2309733	3489263	81.39%	8.250%
41	17.592	2466	2468	2471	rBV2	4271	5863	0.14%	0.014%
42	18.191	2566	2570	2573	rVB3	6199	8030	0.19%	0.019%
43	18.402	2604	2606	2611	rBV3	6274	9749	0.23%	0.023%
44	19.184	2734	2739	2744	rBV3	34948	52808	1.23%	0.125%
45	19.254	2746	2751	2759	rBV2	34713	66026	1.54%	0.156%
46	19.507	2792	2794	2797	rVB4	7698	6525	0.15%	0.015%
47	19.542	2797	2800	2801	rBV3	9979	10406	0.24%	0.025%
48	19.619	2807	2813	2820	rBV	3015749	4287089	100.00%	10.137%
49	20.012	2878	2880	2883	rBV4	7364	6343	0.15%	0.015%
50	20.482	2958	2960	2963	rBV4	8341	8715	0.20%	0.021%
51	20.547	2969	2971	2973	rBV3	11572	12908	0.30%	0.031%
52	21.475	3123	3129	3140	rBV	1966859	2997317	69.91%	7.087%
53	23.638	3494	3497	3498	rBV2	33680	41299	0.96%	0.098%
54	24.307	3602	3611	3624	rVB	1640361	4147833	96.75%	9.808%
55	24.513	3636	3646	3659	rBV	1157563	3070915	71.63%	7.261%




Sum of corrected areas: 42291586

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111124\
Data File : BG063309.D
Acq On : 12 Nov 2024 4:31
Operator : RC/JU
Sample : PB164671BL
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK671

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

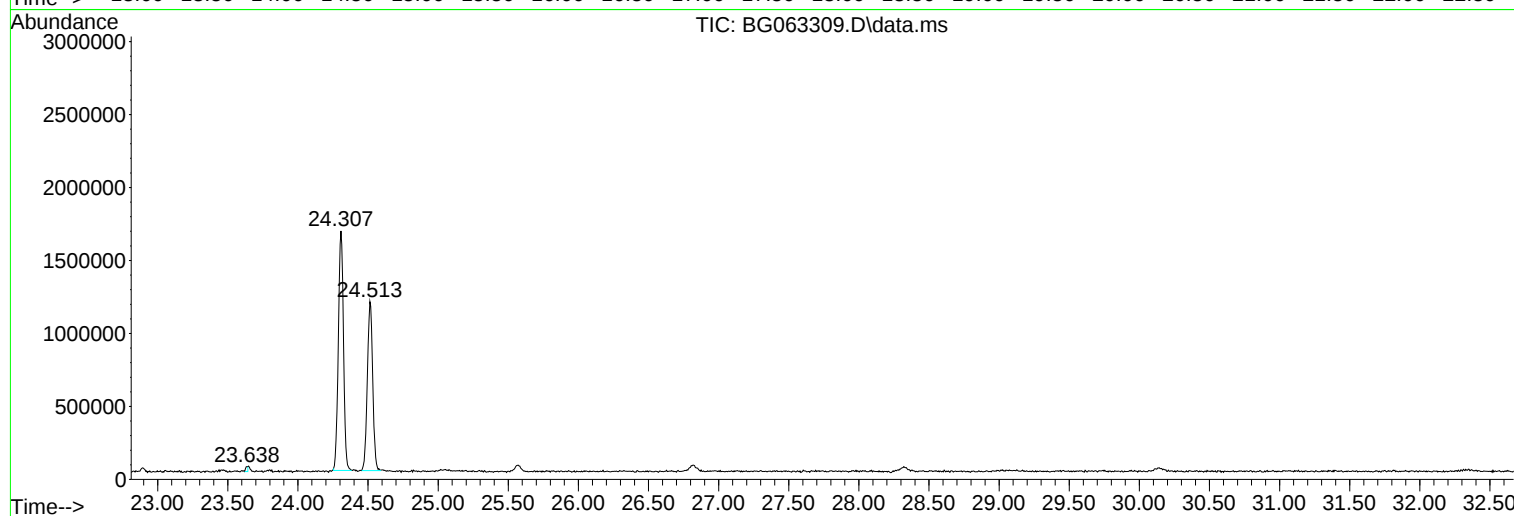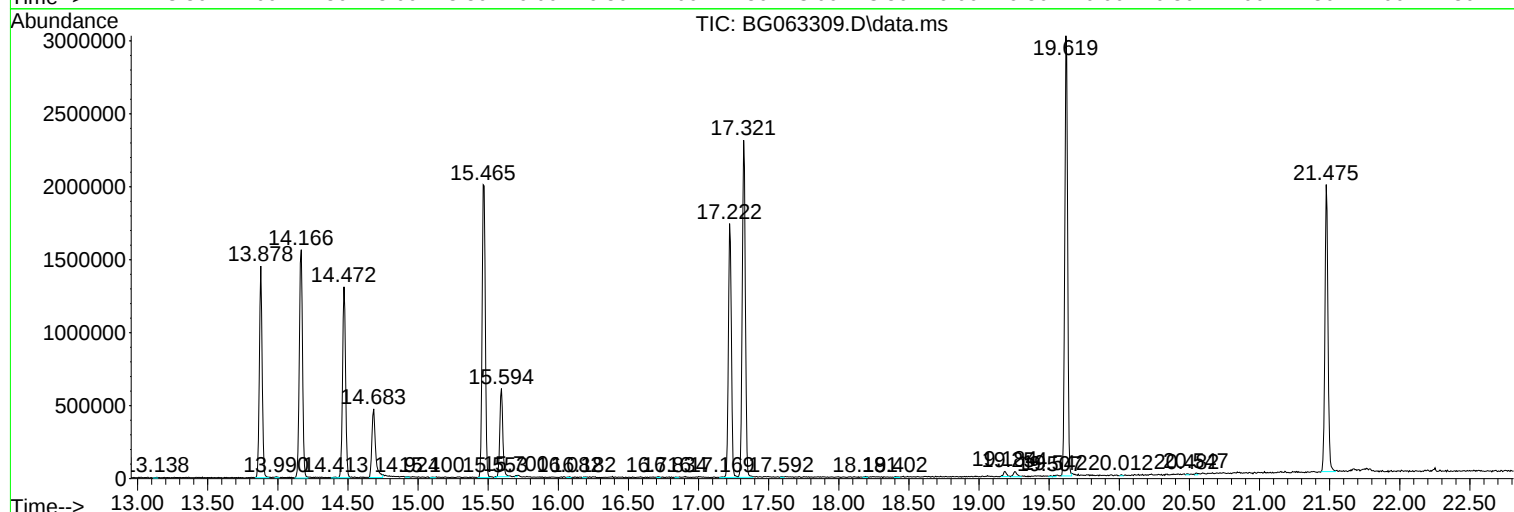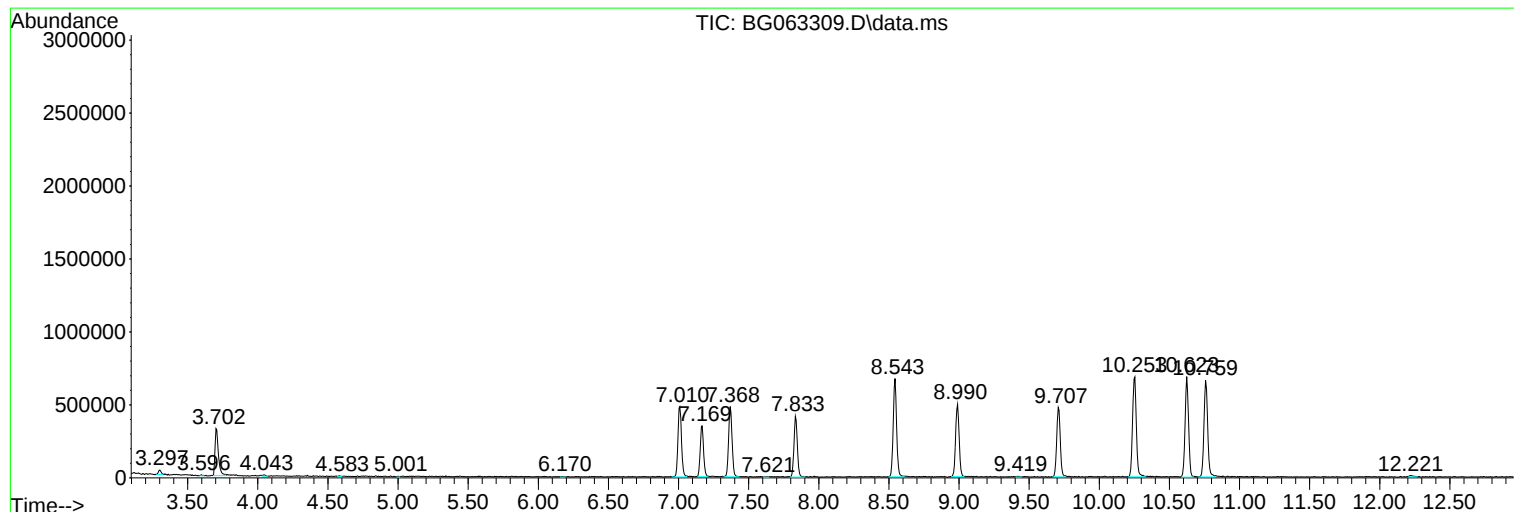

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111124\
Data File : BG063309.D
Acq On : 12 Nov 2024 4:31
Operator : RC/JU
Sample : PB164671BL
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK671

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111124\
Data File : BG063309.D
Acq On : 12 Nov 2024 4:31
Operator : RC/JU
Sample : PB164671BL
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK671

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------