

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111124\
 Data File : BG063310.D
 Acq On : 12 Nov 2024 5:09
 Operator : RC/JU
 Sample : PB164568BL
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK568

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG063310.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.301	32	36	41	rVB2	30241	39519	0.90%	0.090%
2	3.707	100	105	116	rBV	397796	665987	15.19%	1.521%
3	4.218	191	192	197	rVB4	6652	7447	0.17%	0.017%
4	5.135	347	348	353	rBV5	4279	6444	0.15%	0.015%
5	6.245	535	537	542	rBV3	4791	8648	0.20%	0.020%
6	7.009	658	667	678	rBV	523044	899437	20.52%	2.055%
7	7.167	688	694	702	rVB	382403	605719	13.82%	1.384%
8	7.367	722	728	737	rBV	513715	844260	19.26%	1.929%
9	7.831	800	807	816	rBV	421171	727582	16.60%	1.662%
10	8.542	921	928	937	rBV	721799	1210558	27.62%	2.766%
11	8.989	996	1004	1012	rBV	528465	926398	21.13%	2.116%
12	9.712	1120	1127	1136	rBV2	467058	859419	19.61%	1.963%
13	10.252	1211	1219	1232	rBV	731298	1331889	30.39%	3.043%
14	10.428	1246	1249	1251	rBV3	5356	6923	0.16%	0.016%
15	10.622	1273	1282	1293	rVB	694262	1217888	27.79%	2.782%
16	10.757	1296	1305	1322	rBV	674905	1292757	29.49%	2.953%
17	11.433	1418	1420	1423	rBV	4120	6231	0.14%	0.014%
18	12.220	1550	1554	1561	rBV4	10597	21591	0.49%	0.049%
19	12.843	1654	1660	1662	rBV4	4834	9398	0.21%	0.021%
20	13.877	1827	1836	1845	rBV	1439478	2108851	48.11%	4.818%
21	14.165	1877	1885	1894	rBV	1598937	2518974	57.47%	5.755%
22	14.471	1930	1937	1946	rVB	1315873	2039153	46.52%	4.658%
23	14.682	1967	1973	1988	rBV	499510	864259	19.72%	1.974%
24	14.900	2008	2010	2014	rVB2	6488	7906	0.18%	0.018%
25	15.469	2100	2107	2116	rBV	2212326	3255522	74.27%	7.437%
26	15.593	2122	2128	2139	rBV	582579	924875	21.10%	2.113%
27	15.710	2144	2148	2155	rVB5	12710	23812	0.54%	0.054%
28	16.897	2347	2350	2351	rBV2	6303	7804	0.18%	0.018%
29	17.021	2366	2371	2373	rBV3	5854	8267	0.19%	0.019%
30	17.220	2398	2405	2413	rBV	1689645	2586093	59.00%	5.908%
31	17.320	2416	2422	2429	rVV	2408825	3629745	82.81%	8.292%
32	17.972	2531	2533	2539	rBV3	4807	6619	0.15%	0.015%
33	18.425	2606	2610	2612	rVB3	5035	7164	0.16%	0.016%
34	18.460	2612	2616	2618	rBV5	7267	10607	0.24%	0.024%
35	18.566	2630	2634	2639	rBV3	4969	11592	0.26%	0.026%
36	18.724	2656	2661	2663	rBV5	4541	6120	0.14%	0.014%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111124\
Data File : BG063310.D
Acq On : 12 Nov 2024 5:09
Operator : RC/JU
Sample : PB164568BL
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK568

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
Title : SVOA CALIBRATION

37	18.901	2688	2691	2692	rBV3	7076	8489	0.19%	0.019%
38	19.130	2728	2730	2733	rVB3	7994	6521	0.15%	0.015%
39	19.183	2733	2739	2744	rBV3	42788	66604	1.52%	0.152%
40	19.259	2744	2752	2759	rBV2	38764	77302	1.76%	0.177%
41	19.623	2807	2814	2821	rBV	3184724	4383251	100.00%	10.014%
42	20.593	2977	2979	2982	rBV4	13360	12236	0.28%	0.028%
43	21.480	3123	3130	3138	rBV	1890984	3004232	68.54%	6.863%
44	22.890	3365	3370	3376	rBV6	36527	59603	1.36%	0.136%
45	24.306	3600	3611	3621	rBV2	1652279	4332060	98.83%	9.897%
46	24.518	3637	3647	3659	rVB	1163621	3117411	71.12%	7.122%




Sum of corrected areas: 43773167

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111124\
Data File : BG063310.D
Acq On : 12 Nov 2024 5:09
Operator : RC/JU
Sample : PB164568BL
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK568

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

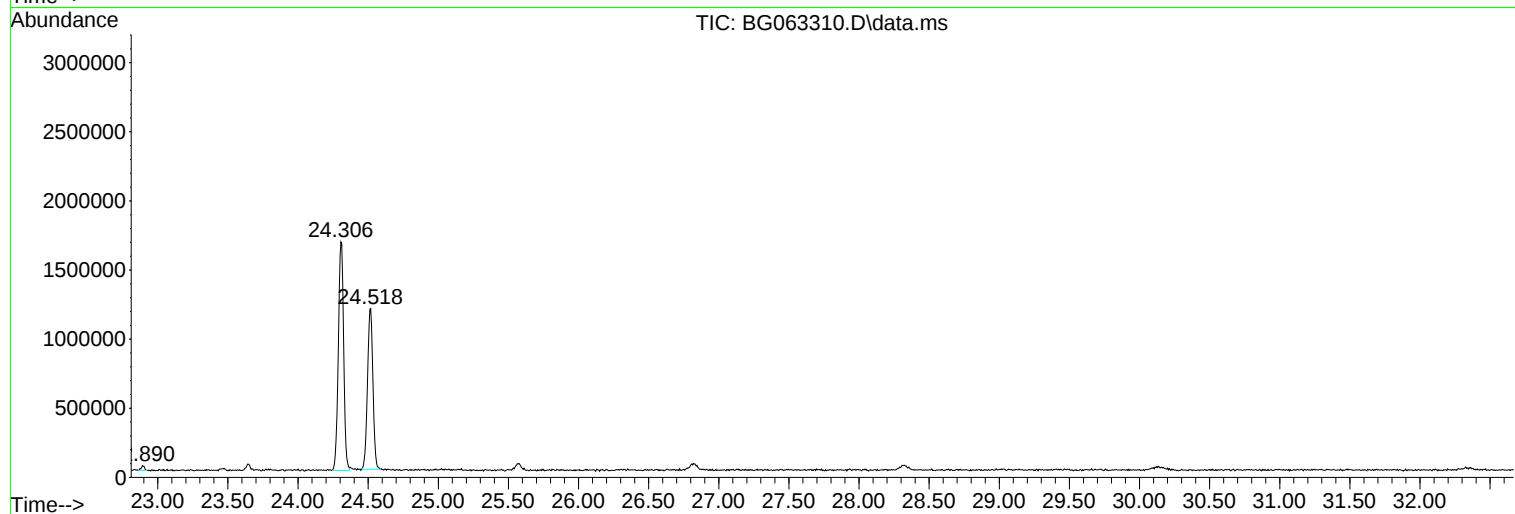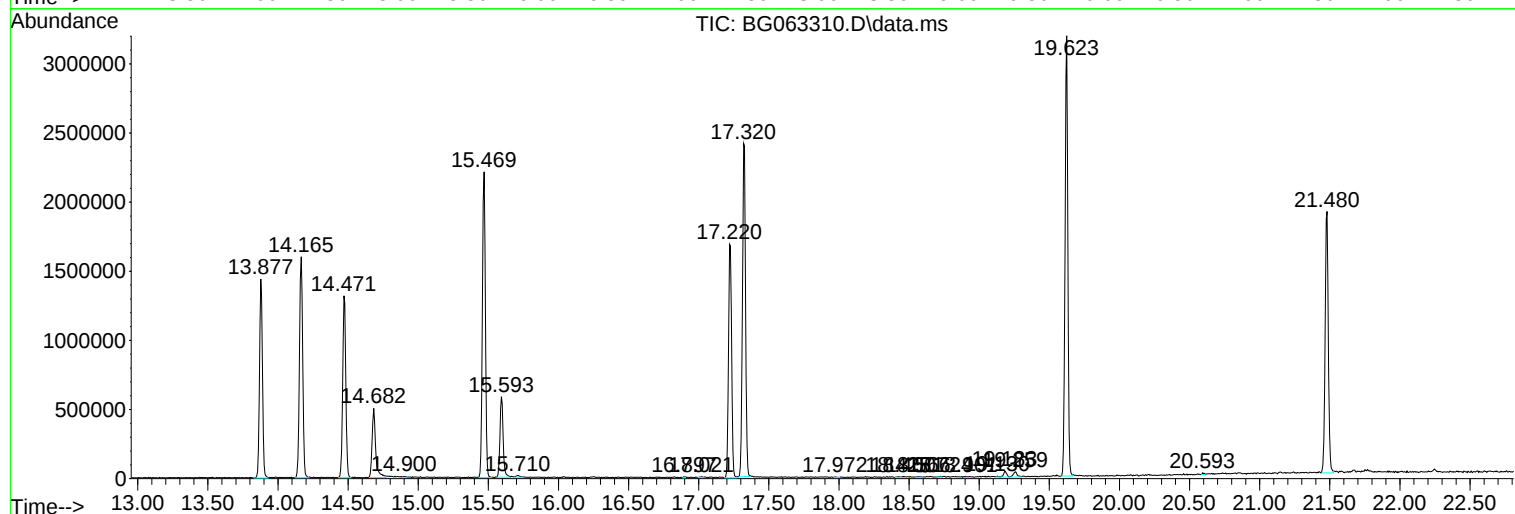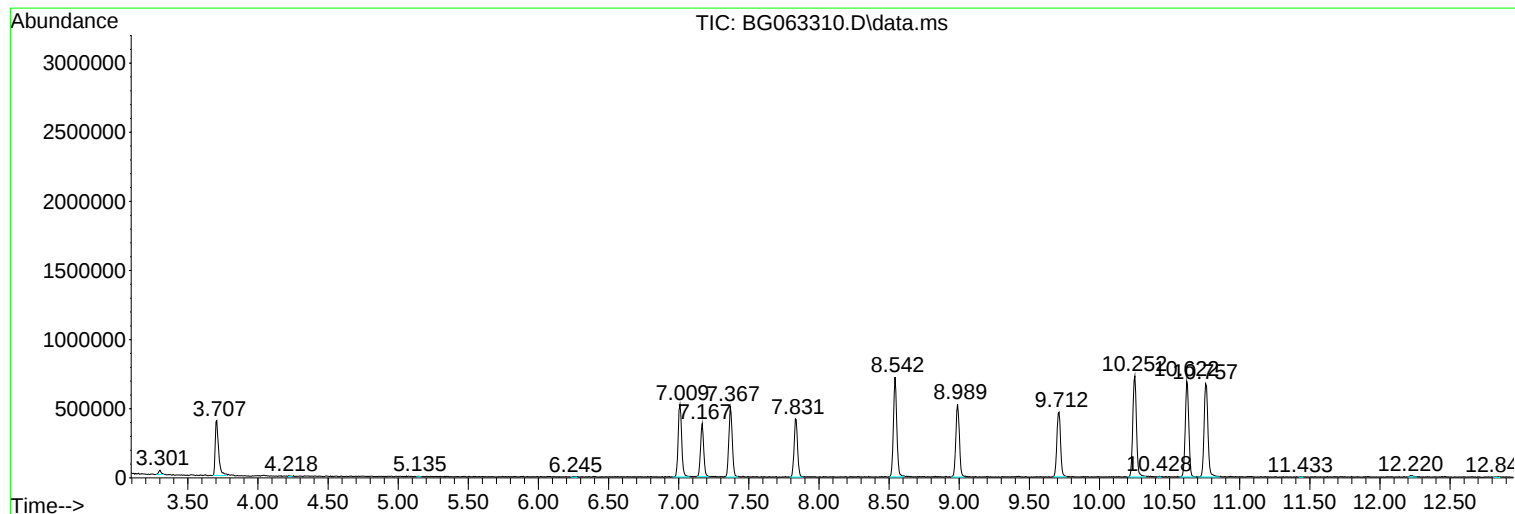

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111124\
Data File : BG063310.D
Acq On : 12 Nov 2024 5:09
Operator : RC/JU
Sample : PB164568BL
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK568

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111124\
Data File : BG063310.D
Acq On : 12 Nov 2024 5:09
Operator : RC/JU
Sample : PB164568BL
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK568

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc