

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111124\
 Data File : BG063311.D
 Acq On : 12 Nov 2024 5:47
 Operator : RC/JU
 Sample : P4625-02
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0AA2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG063311.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.299	33	36	41	rVB4	29030	31291	0.61%	0.070%
2	3.546	74	78	81	rBV6	6036	8416	0.16%	0.019%
3	3.711	101	106	117	rVB	92472	170670	3.32%	0.381%
4	3.899	136	138	142	rBV3	6236	7791	0.15%	0.017%
5	4.046	160	163	168	rVB4	8007	12177	0.24%	0.027%
6	4.539	241	247	253	rBV	45236	69404	1.35%	0.155%
7	5.491	403	409	410	rBV4	7122	12177	0.24%	0.027%
8	5.691	439	443	446	rBV4	10280	15637	0.30%	0.035%
9	6.490	575	579	582	rBV4	6762	9688	0.19%	0.022%
10	6.825	632	636	638	rBV4	4833	7236	0.14%	0.016%
11	7.007	661	667	681	rVB2	187306	340740	6.63%	0.760%
12	7.165	685	694	704	rBV	426390	693710	13.50%	1.547%
13	7.371	722	729	737	rBV	494781	839175	16.33%	1.871%
14	7.835	801	808	815	rBV	408773	659086	12.83%	1.470%
15	8.540	922	928	939	rVB	573112	932466	18.15%	2.079%
16	8.910	988	991	997	rBV4	5021	8256	0.16%	0.018%
17	8.987	997	1004	1012	rBV	602171	1040572	20.25%	2.321%
18	9.709	1118	1127	1138	rBV	568469	993181	19.33%	2.215%
19	9.986	1172	1174	1177	rBV2	6598	7298	0.14%	0.016%
20	10.250	1212	1219	1232	rBV	848175	1526687	29.72%	3.405%
21	10.626	1275	1283	1290	rVB	626307	1111642	21.64%	2.479%
22	10.761	1299	1306	1316	rBV	569338	1086267	21.14%	2.422%
23	11.637	1452	1455	1457	rBV4	9566	9510	0.19%	0.021%
24	12.224	1548	1555	1556	rBV3	12283	20523	0.40%	0.046%
25	13.252	1728	1730	1736	rVB	6412	8490	0.17%	0.019%
26	13.881	1830	1837	1844	rBV	1678340	2464289	47.97%	5.495%
27	14.163	1878	1885	1896	rBV	1763504	2792436	54.35%	6.227%
28	14.474	1929	1938	1946	rBV	1194622	1896603	36.92%	4.229%
29	14.604	1955	1960	1963	rBV2	7300	9311	0.18%	0.021%
30	14.686	1968	1974	1983	rBV2	136445	278410	5.42%	0.621%
31	15.467	2100	2107	2118	rBV	2513176	3724168	72.49%	8.305%
32	15.591	2123	2128	2136	rBV	809125	1184834	23.06%	2.642%
33	15.708	2145	2148	2152	rVB4	10906	12055	0.23%	0.027%
34	15.832	2164	2169	2175	rVB	43062	63431	1.23%	0.141%
35	16.167	2222	2226	2227	rBV3	7508	8920	0.17%	0.020%
36	17.007	2366	2369	2372	rBV2	6184	8492	0.17%	0.019%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111124\
 Data File : BG063311.D
 Acq On : 12 Nov 2024 5:47
 Operator : RC/JU
 Sample : P4625-02
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0AA2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
 Title : SVOA CALIBRATION

37	17.224	2398	2406	2411	rBV	1688025	2394369	46.60%	5.340%
38	17.324	2416	2423	2433	rVB	2867187	4255122	82.82%	9.489%
39	17.512	2451	2455	2459	rBV3	23865	34914	0.68%	0.078%
40	18.129	2556	2560	2562	rBV4	8256	11759	0.23%	0.026%
41	18.188	2567	2570	2572	rBV2	15937	15588	0.30%	0.035%
42	19.187	2735	2740	2744	rVB3	45553	68406	1.33%	0.153%
43	19.257	2748	2752	2755	rVV3	39815	57726	1.12%	0.129%
44	19.286	2755	2757	2765	rVB4	35262	56766	1.10%	0.127%
45	19.621	2808	2814	2823	rBV	3683956	5137650	100.00%	11.457%
46	20.373	2940	2942	2945	rVB4	14679	10768	0.21%	0.024%
47	20.661	2989	2991	2993	rBV3	11486	9273	0.18%	0.021%
48	20.708	2995	2999	3003	rVB2	18935	28705	0.56%	0.064%
49	20.996	3046	3048	3051	rBV4	14736	10733	0.21%	0.024%
50	21.478	3124	3130	3141	rVB2	1731457	2739874	53.33%	6.110%
51	21.666	3160	3162	3167	rBV6	19665	23508	0.46%	0.052%
52	24.310	3602	3612	3626	rVB	1990255	5058716	98.46%	11.281%
53	24.516	3637	3647	3658	rVB	1068199	2863462	55.73%	6.386%




Sum of corrected areas: 44842378

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111124\
Data File : BG063311.D
Acq On : 12 Nov 2024 5:47
Operator : RC/JU
Sample : P4625-02
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0AA2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

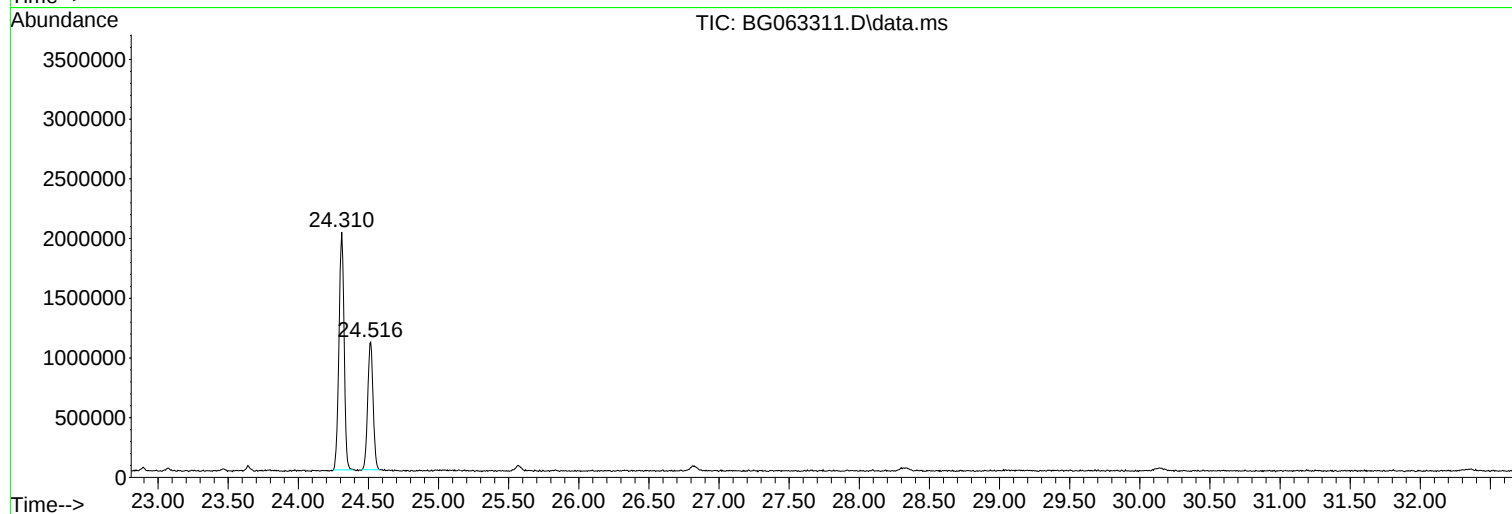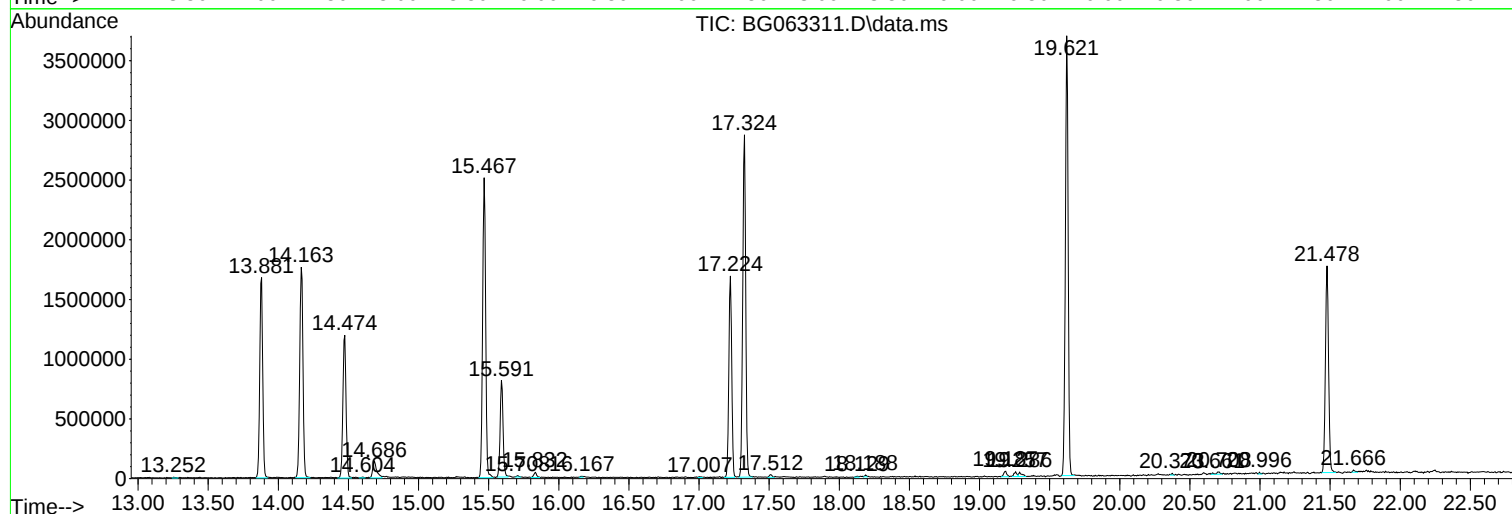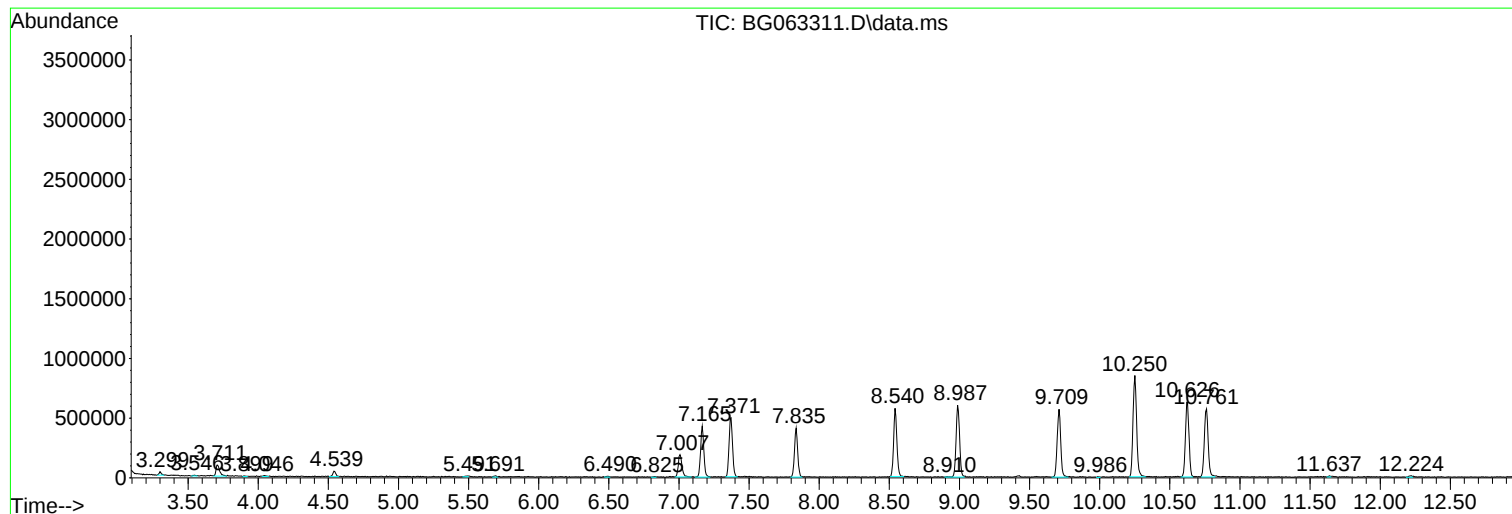

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111124\
Data File : BG063311.D
Acq On : 12 Nov 2024 5:47
Operator : RC/JU
Sample : P4625-02
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0AA2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111124\
Data File : BG063311.D
Acq On : 12 Nov 2024 5:47
Operator : RC/JU
Sample : P4625-02
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0AA2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
