

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111124\
 Data File : BG063314.D
 Acq On : 12 Nov 2024 7:41
 Operator : RC/JU
 Sample : P4625-06
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0AA9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG063314.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.299	31	36	42	rBV6	28252	40184	0.82%	0.095%
2	3.711	102	106	114	rBV	69475	102147	2.08%	0.242%
3	4.040	157	162	168	rBV2	37874	62824	1.28%	0.149%
4	4.404	222	224	228	rVB5	5984	7034	0.14%	0.017%
5	4.539	244	247	254	rVB3	18080	31755	0.65%	0.075%
6	5.356	382	386	389	rBV4	5336	8338	0.17%	0.020%
7	5.479	405	407	409	rBV3	7723	6907	0.14%	0.016%
8	5.679	438	441	448	rBV2	10225	17117	0.35%	0.041%
9	7.007	660	667	675	rBV	148455	261420	5.33%	0.619%
10	7.165	686	694	702	rBV	345921	570656	11.63%	1.350%
11	7.371	721	729	738	rBV	419059	718083	14.63%	1.699%
12	7.471	743	746	750	rVB4	5857	7219	0.15%	0.017%
13	7.835	801	808	816	rVB	428006	709503	14.46%	1.679%
14	8.458	909	914	917	rBV3	4627	8512	0.17%	0.020%
15	8.540	921	928	941	rVV	474802	797884	16.26%	1.888%
16	8.987	996	1004	1012	rBV2	506311	869247	17.71%	2.057%
17	9.363	1066	1068	1072	rVB4	5531	7155	0.15%	0.017%
18	9.410	1072	1076	1078	rVV3	7099	10268	0.21%	0.024%
19	9.457	1082	1084	1089	rVB3	6463	7784	0.16%	0.018%
20	9.592	1102	1107	1111	rBV4	3273	7380	0.15%	0.017%
21	9.710	1120	1127	1137	rBV	482319	828704	16.89%	1.961%
22	10.250	1212	1219	1231	rBV	691256	1252353	25.52%	2.964%
23	10.626	1275	1283	1291	rBV	701413	1226464	24.99%	2.902%
24	10.761	1299	1306	1316	rBV	455124	877735	17.89%	2.077%
25	11.678	1459	1462	1465	rVB2	6161	6690	0.14%	0.016%
26	12.218	1550	1554	1557	rBV4	10936	16254	0.33%	0.038%
27	12.577	1613	1615	1618	rVB	6734	7056	0.14%	0.017%
28	12.759	1641	1646	1647	rBV3	5634	6667	0.14%	0.016%
29	12.824	1654	1657	1660	rBV4	6787	7731	0.16%	0.018%
30	13.805	1820	1824	1828	rVB	5941	10078	0.21%	0.024%
31	13.881	1828	1837	1846	rBV	1459016	2158286	43.98%	5.107%
32	14.163	1876	1885	1895	rBV2	1501899	2379950	48.50%	5.632%
33	14.475	1929	1938	1946	rBV	1268385	1970582	40.16%	4.663%
34	14.610	1958	1961	1964	rVB2	5582	7714	0.16%	0.018%
35	14.686	1967	1974	1983	rBV	111344	226678	4.62%	0.536%
36	14.892	2004	2009	2010	rBV5	7376	9673	0.20%	0.023%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111124\
 Data File : BG063314.D
 Acq On : 12 Nov 2024 7:41
 Operator : RC/JU
 Sample : P4625-06
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0AA9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
 Title : SVOA CALIBRATION

37	14.974	2018	2023	2030	rBV	70326	100499	2.05%	0.238%
38	15.203	2060	2062	2068	rBV4	5464	8152	0.17%	0.019%
39	15.291	2074	2077	2080	rVB5	8269	11710	0.24%	0.028%
40	15.468	2100	2107	2114	rBV	2172744	3216876	65.55%	7.612%
41	15.591	2122	2128	2141	rBV	742984	1116340	22.75%	2.642%
42	15.703	2145	2147	2152	rVB4	10095	13561	0.28%	0.032%
43	16.167	2222	2226	2228	rBV4	12544	16229	0.33%	0.038%
44	16.366	2257	2260	2265	rBV3	4839	8075	0.16%	0.019%
45	16.637	2301	2306	2307	rBV3	5928	7657	0.16%	0.018%
46	16.907	2347	2352	2353	rBV5	9129	10507	0.21%	0.025%
47	17.224	2396	2406	2415	rBV	1685208	2556484	52.10%	6.050%
48	17.324	2415	2423	2431	rBV	2670108	4056753	82.67%	9.600%
49	17.512	2449	2455	2459	rVB3	8756	13198	0.27%	0.031%
50	17.888	2517	2519	2522	rVB4	8363	9449	0.19%	0.022%
51	17.941	2527	2528	2531	rVB3	9274	6812	0.14%	0.016%
52	18.123	2556	2559	2563	rBV4	7697	12895	0.26%	0.031%
53	18.194	2568	2571	2574	rVB2	10304	15342	0.31%	0.036%
54	19.181	2735	2739	2744	rBV2	40363	55761	1.14%	0.132%
55	19.257	2746	2752	2756	rBV2	37351	60329	1.23%	0.143%
56	19.621	2807	2814	2826	rBV	3461694	4907245	100.00%	11.612%
57	19.909	2861	2863	2866	rVB4	7845	7420	0.15%	0.018%
58	19.945	2866	2869	2871	rBV4	8724	9193	0.19%	0.022%
59	21.478	3123	3130	3139	rBV	1859126	2945671	60.03%	6.971%
60	24.304	3601	3611	3625	rBV	1892192	4869629	99.23%	11.523%
61	24.510	3638	3646	3657	rVB	1125769	2979022	60.71%	7.049%




Sum of corrected areas: 42258841

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111124\
Data File : BG063314.D
Acq On : 12 Nov 2024 7:41
Operator : RC/JU
Sample : P4625-06
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0AA9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

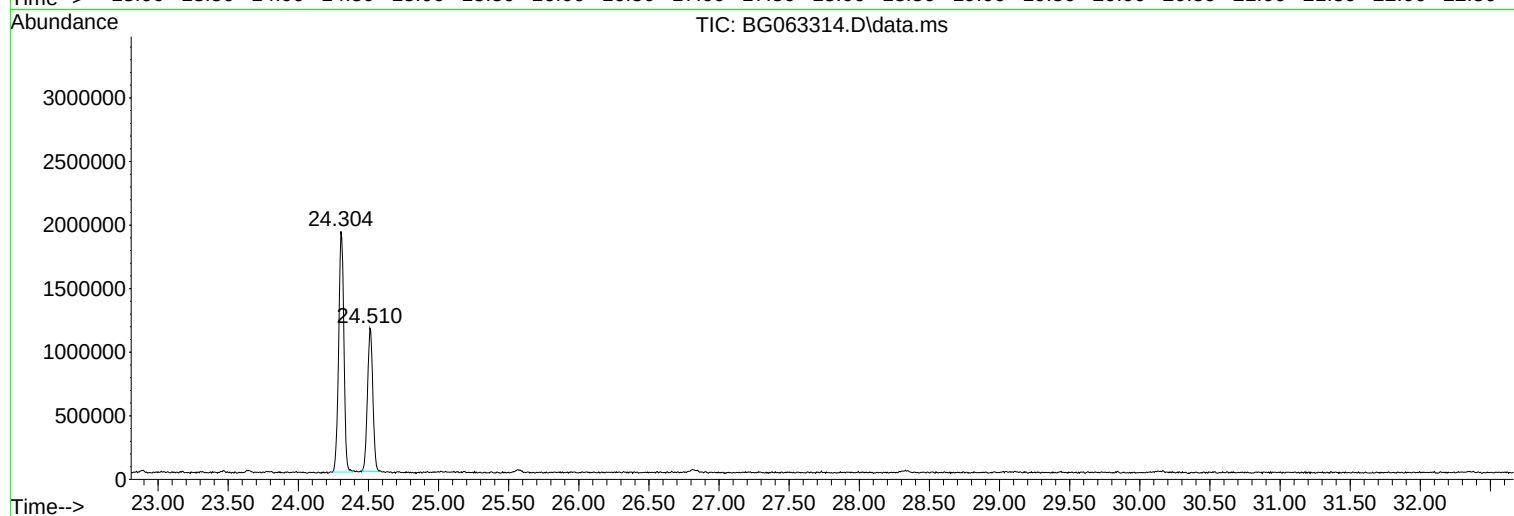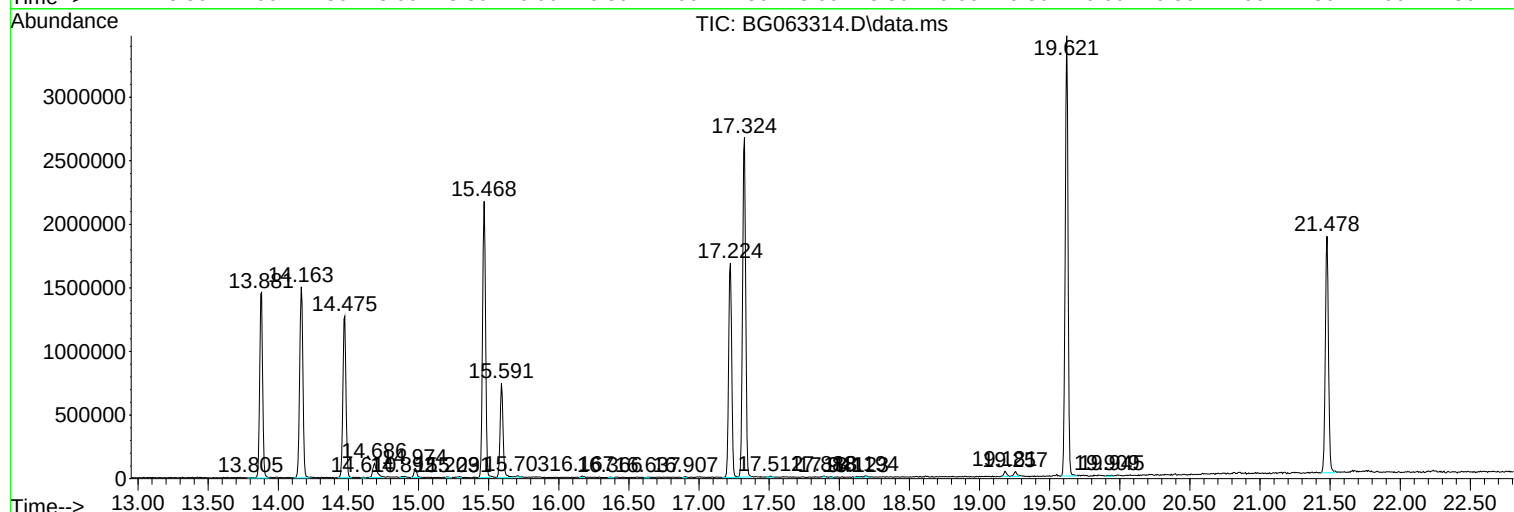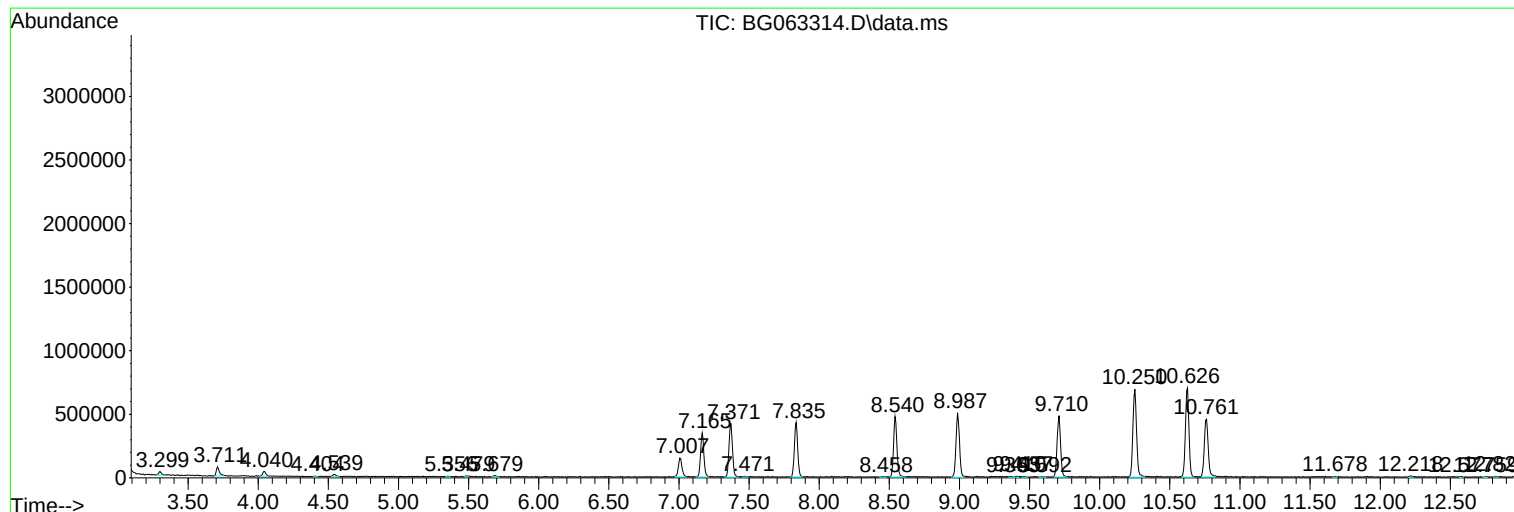

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111124\
Data File : BG063314.D
Acq On : 12 Nov 2024 7:41
Operator : RC/JU
Sample : P4625-06
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0AA9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111124\
Data File : BG063314.D
Acq On : 12 Nov 2024 7:41
Operator : RC/JU
Sample : P4625-06
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0AA9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc