

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111124\
 Data File : BG063324.D
 Acq On : 12 Nov 2024 14:01
 Operator : RC/JU
 Sample : PB164734BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK734

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG063324.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.299	32	36	40	rBV4	27279	36142	0.86%	0.086%
2	3.704	100	105	115	rBV	367197	608401	14.44%	1.447%
3	4.168	183	184	188	rBV3	5738	7345	0.17%	0.017%
4	4.597	255	257	262	rVB4	5621	7262	0.17%	0.017%
5	5.296	373	376	381	rBV5	5110	8831	0.21%	0.021%
6	7.006	660	667	676	rBV	501896	844325	20.04%	2.009%
7	7.165	688	694	703	rVB	347468	552555	13.12%	1.315%
8	7.318	717	720	722	rBV3	5431	6043	0.14%	0.014%
9	7.365	722	728	739	rVB	470571	793466	18.83%	1.888%
10	7.835	801	808	816	rBV	436165	716216	17.00%	1.704%
11	8.540	921	928	937	rBV	681667	1156167	27.44%	2.751%
12	8.986	997	1004	1021	rBV	494037	874418	20.76%	2.080%
13	9.709	1118	1127	1137	rBV	474150	828013	19.65%	1.970%
14	10.249	1211	1219	1232	rBV	730974	1287970	30.57%	3.064%
15	10.625	1276	1283	1291	rVB	656696	1176359	27.92%	2.799%
16	10.755	1298	1305	1316	rBV	642923	1209336	28.71%	2.877%
17	11.912	1498	1502	1506	rVB5	5152	7340	0.17%	0.017%
18	12.224	1552	1555	1557	rBV3	7144	9335	0.22%	0.022%
19	12.858	1656	1663	1666	rBV4	2841	6120	0.15%	0.015%
20	13.645	1794	1797	1802	rBV3	3319	7355	0.17%	0.017%
21	13.880	1829	1837	1843	rBV	1361144	2002105	47.52%	4.763%
22	14.163	1878	1885	1894	rBV	1571203	2401881	57.01%	5.714%
23	14.474	1930	1938	1947	rBV	1276034	2020979	47.97%	4.808%
24	14.680	1967	1973	1987	rBV	443102	821469	19.50%	1.954%
25	15.467	2099	2107	2114	rBV	2141169	3096001	73.49%	7.366%
26	15.590	2120	2128	2137	rBV	517343	822663	19.53%	1.957%
27	15.708	2145	2148	2152	rVB6	9759	16809	0.40%	0.040%
28	17.224	2399	2406	2414	rBV	1798799	2583161	61.32%	6.146%
29	17.323	2416	2423	2435	rVV	2282484	3489914	82.84%	8.303%
30	17.423	2439	2440	2445	rVB4	7737	7347	0.17%	0.017%
31	17.670	2479	2482	2484	rBV3	5787	6099	0.14%	0.015%
32	17.794	2498	2503	2505	rVB4	5057	7422	0.18%	0.018%
33	17.899	2517	2521	2526	rVB2	8017	14423	0.34%	0.034%
34	18.199	2566	2572	2575	rVB5	5172	9480	0.23%	0.023%
35	18.334	2590	2595	2596	rBV4	7073	9123	0.22%	0.022%
36	18.781	2669	2671	2674	rBV3	5887	5965	0.14%	0.014%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111124\
 Data File : BG063324.D
 Acq On : 12 Nov 2024 14:01
 Operator : RC/JU
 Sample : PB164734BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK734

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
 Title : SVOA CALIBRATION

37	18.928	2693	2696	2699	rBV2	5664	6773	0.16%	0.016%
38	19.074	2719	2721	2724	rVB4	7248	6870	0.16%	0.016%
39	19.104	2724	2726	2730	rBV5	7538	12131	0.29%	0.029%
40	19.186	2735	2740	2744	rVV2	37957	58587	1.39%	0.139%
41	19.257	2747	2752	2759	rVB3	32934	62406	1.48%	0.148%
42	19.380	2769	2773	2775	rBV4	7511	11217	0.27%	0.027%
43	19.533	2795	2799	2800	rBV3	7720	6533	0.16%	0.016%
44	19.621	2807	2814	2821	rBV	3091046	4212907	100.00%	10.023%
45	20.596	2978	2980	2983	rVB4	12041	10952	0.26%	0.026%
46	20.808	3015	3016	3018	rBV2	15544	13261	0.31%	0.032%
47	21.477	3123	3130	3139	rBV	1885746	3035785	72.06%	7.223%
48	24.304	3601	3611	3624	rVB	1584943	4074964	96.73%	9.695%
49	24.509	3636	3646	3658	rBV3	1131733	3061870	72.68%	7.285%




Sum of corrected areas: 42032096

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111124\
Data File : BG063324.D
Acq On : 12 Nov 2024 14:01
Operator : RC/JU
Sample : PB164734BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK734

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

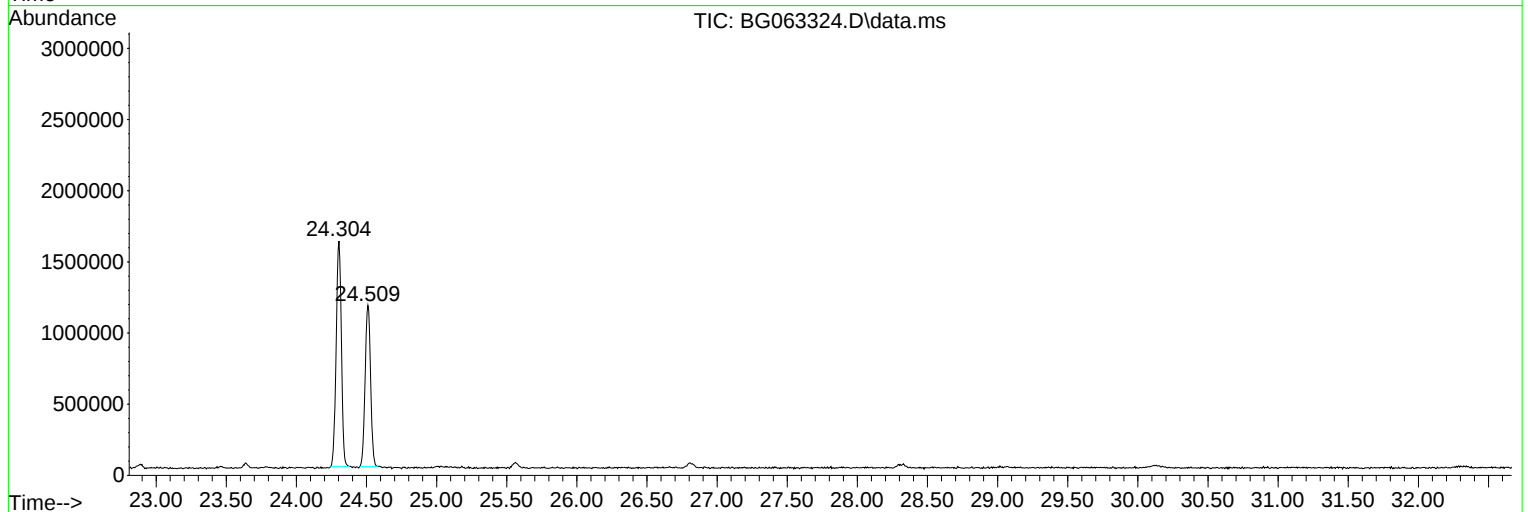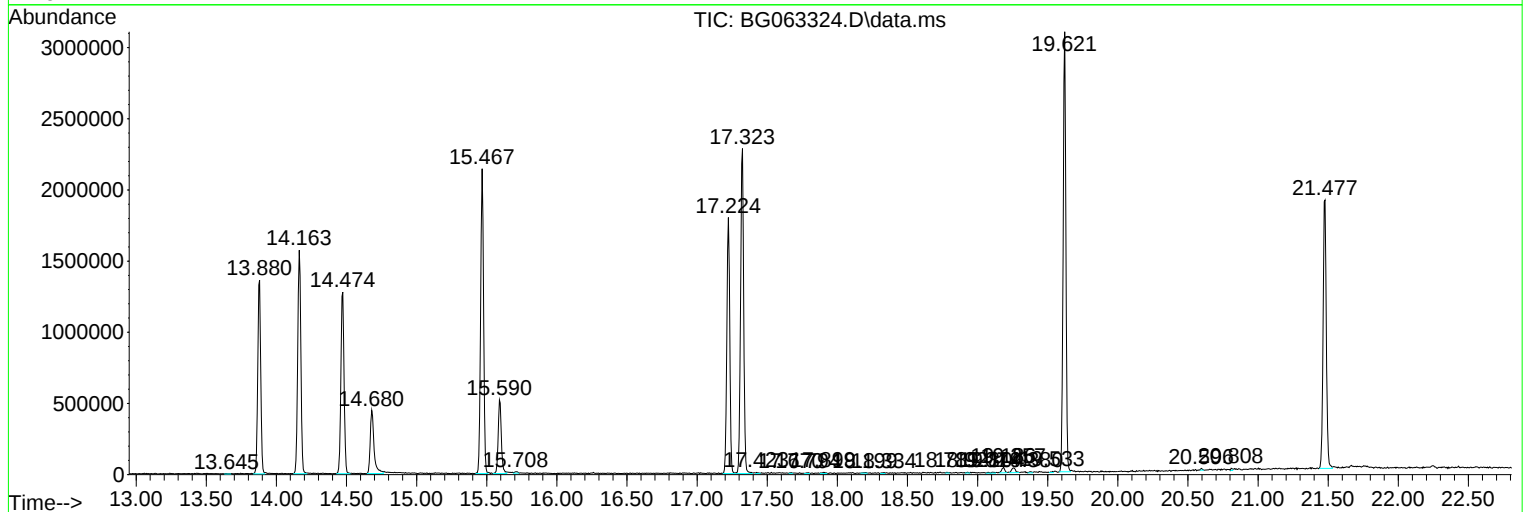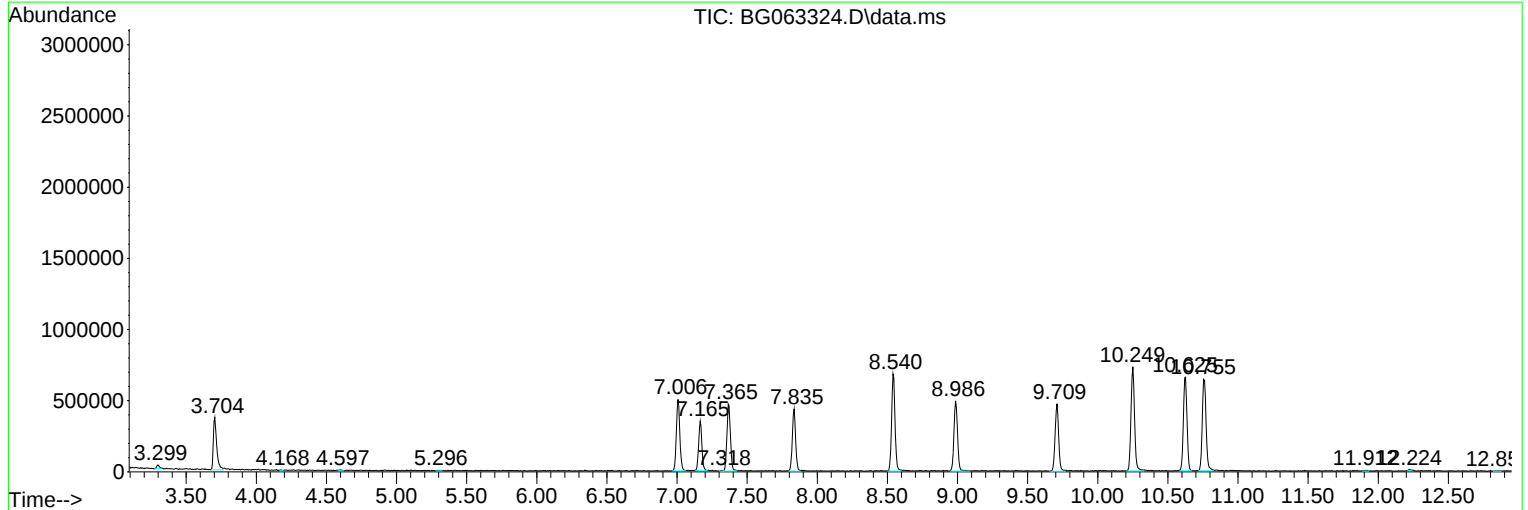

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111124\
Data File : BG063324.D
Acq On : 12 Nov 2024 14:01
Operator : RC/JU
Sample : PB164734BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK734

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111124\
Data File : BG063324.D
Acq On : 12 Nov 2024 14:01
Operator : RC/JU
Sample : PB164734BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK734

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc