

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111124\
 Data File : BG063325.D
 Acq On : 12 Nov 2024 14:39
 Operator : RC/JU
 Sample : PB164895BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK895

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG063325.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.300	33	36	41	rVB2	27613	37572	0.91%	0.093%
2	3.705	101	105	115	rBV	344391	576764	13.93%	1.425%
3	5.045	328	333	335	rBV4	5310	8755	0.21%	0.022%
4	5.303	375	377	380	rBV3	5291	6299	0.15%	0.016%
5	6.014	496	498	502	rVB4	6229	7768	0.19%	0.019%
6	6.355	553	556	559	rBV4	5072	7369	0.18%	0.018%
7	6.408	561	565	567	rBV2	4789	7252	0.18%	0.018%
8	7.007	659	667	675	rBV	506095	838294	20.24%	2.071%
9	7.166	686	694	706	rBV	339005	567162	13.70%	1.401%
10	7.366	723	728	737	rBV	446334	762448	18.41%	1.883%
11	7.836	802	808	816	rBV	374538	629155	15.19%	1.554%
12	8.135	856	859	863	rBV2	4180	6734	0.16%	0.017%
13	8.541	922	928	936	rBV	662776	1122829	27.12%	2.774%
14	8.752	961	964	968	rVB2	5677	6731	0.16%	0.017%
15	8.987	996	1004	1015	rBV	496797	866187	20.92%	2.140%
16	9.134	1026	1029	1032	rBV4	4415	5774	0.14%	0.014%
17	9.193	1034	1039	1041	rBV4	13912	18866	0.46%	0.047%
18	9.416	1075	1077	1082	rVB3	6426	9011	0.22%	0.022%
19	9.545	1094	1099	1101	rBV3	4020	6101	0.15%	0.015%
20	9.710	1117	1127	1141	rBV	453203	823619	19.89%	2.035%
21	10.250	1212	1219	1230	rBV	688752	1253402	30.27%	3.096%
22	10.621	1274	1282	1290	rBV	622213	1080953	26.10%	2.670%
23	10.756	1298	1305	1319	rBV	620009	1134897	27.41%	2.803%
24	12.107	1532	1535	1538	rVB2	6231	7295	0.18%	0.018%
25	12.225	1549	1555	1558	rBV3	8380	15615	0.38%	0.039%
26	12.624	1618	1623	1626	rVB3	3621	6283	0.15%	0.016%
27	13.876	1828	1836	1847	rBV	1347884	1966575	47.49%	4.858%
28	13.993	1853	1856	1859	rVB	5143	6249	0.15%	0.015%
29	14.163	1878	1885	1896	rBV	1527666	2359802	56.99%	5.829%
30	14.334	1910	1914	1917	rBV4	3377	5687	0.14%	0.014%
31	14.469	1926	1937	1946	rBV	1158782	1834324	44.30%	4.531%
32	14.681	1966	1973	1990	rBV	445246	819507	19.79%	2.024%
33	15.468	2098	2107	2117	rBV	2053454	3030993	73.20%	7.487%
34	15.591	2122	2128	2141	rVV	532813	795885	19.22%	1.966%
35	15.826	2166	2168	2174	rVB6	8302	10695	0.26%	0.026%
36	16.038	2200	2204	2207	rVB3	4817	7458	0.18%	0.018%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111124\
 Data File : BG063325.D
 Acq On : 12 Nov 2024 14:39
 Operator : RC/JU
 Sample : PB164895BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK895

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
 Title : SVOA CALIBRATION

37	16.097	2211	2214	2218	rBV3	4256	6832	0.16%	0.017%
38	16.249	2238	2240	2243	rVB3	6091	6001	0.14%	0.015%
39	16.719	2318	2320	2322	rBV	5743	6469	0.16%	0.016%
40	16.901	2347	2351	2353	rBV4	7527	9899	0.24%	0.024%
41	17.219	2399	2405	2412	rVB	1550633	2324208	56.13%	5.741%
42	17.319	2416	2422	2430	rBV	2277912	3401665	82.15%	8.403%
43	17.595	2465	2469	2474	rBV6	4504	10226	0.25%	0.025%
44	17.748	2492	2495	2498	rVB3	4727	6405	0.15%	0.016%
45	17.795	2498	2503	2504	rBV4	5997	8134	0.20%	0.020%
46	17.818	2504	2507	2511	rVV3	4605	6598	0.16%	0.016%
47	17.889	2517	2519	2522	rBV4	7548	8360	0.20%	0.021%
48	18.617	2640	2643	2645	rBV4	6029	7178	0.17%	0.018%
49	18.923	2692	2695	2698	rBV5	5599	6037	0.15%	0.015%
50	18.999	2703	2708	2709	rBV4	5036	7518	0.18%	0.019%
51	19.128	2728	2730	2733	rBV2	5339	6633	0.16%	0.016%
52	19.181	2735	2739	2745	rVV3	37269	60861	1.47%	0.150%
53	19.252	2745	2751	2755	rVV	38360	54261	1.31%	0.134%
54	19.310	2757	2761	2765	rVB6	11457	13494	0.33%	0.033%
55	19.551	2799	2802	2805	rBV5	7563	9727	0.23%	0.024%
56	19.622	2807	2814	2824	rBV	2946397	4140915	100.00%	10.229%
57	19.786	2840	2842	2844	rVB3	9379	6959	0.17%	0.017%
58	20.109	2895	2897	2900	rBV3	8998	7872	0.19%	0.019%
59	20.591	2977	2979	2983	rVB5	15216	18016	0.44%	0.045%
60	21.473	3123	3129	3141	rVB	1774116	2710830	65.46%	6.696%
61	22.583	3316	3318	3326	rVB7	29423	52588	1.27%	0.130%
62	24.299	3600	3610	3622	rBV	1557581	4132284	99.79%	10.208%
63	24.510	3636	3646	3656	rVB	1057079	2802056	67.67%	6.922%



Sum of corrected areas: 40482336

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111124\
Data File : BG063325.D
Acq On : 12 Nov 2024 14:39
Operator : RC/JU
Sample : PB164895BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK895

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

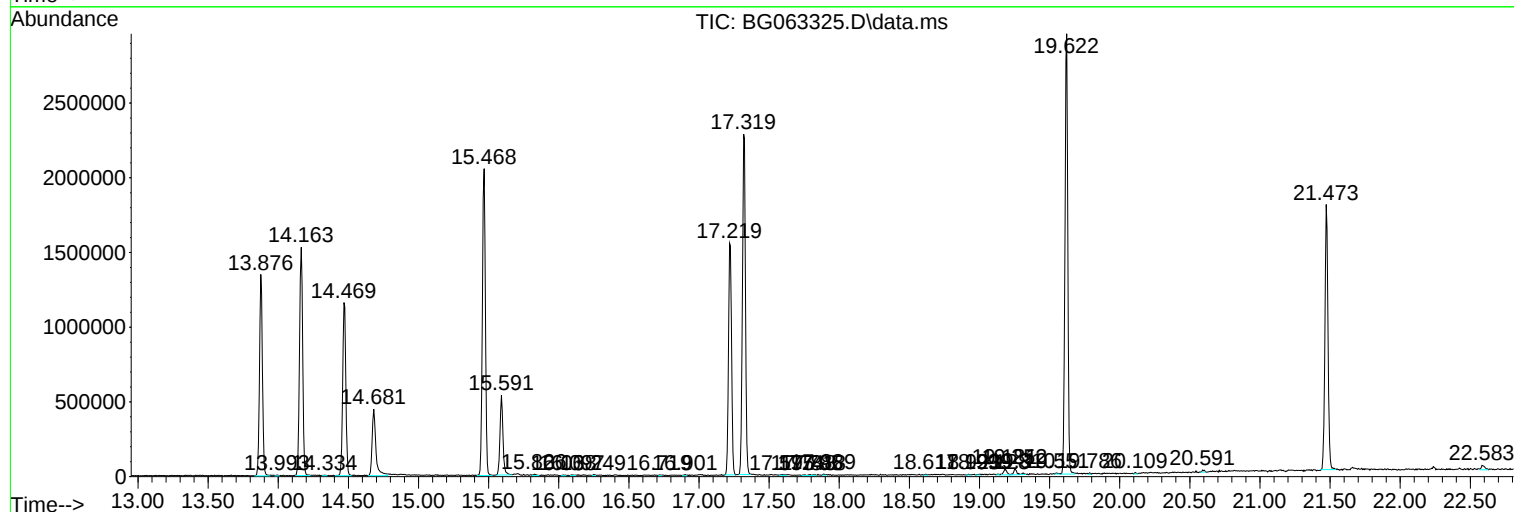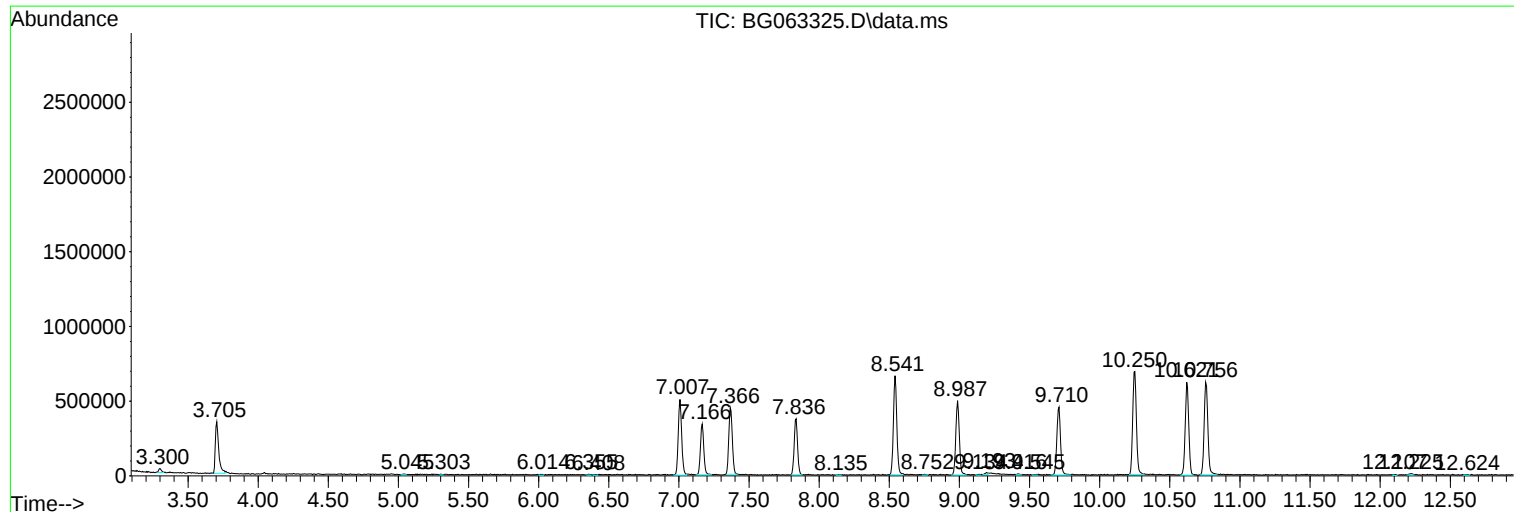

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111124\
Data File : BG063325.D
Acq On : 12 Nov 2024 14:39
Operator : RC/JU
Sample : PB164895BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK895

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111124\
Data File : BG063325.D
Acq On : 12 Nov 2024 14:39
Operator : RC/JU
Sample : PB164895BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK895

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc