

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111124\
 Data File : BG063328.D
 Acq On : 12 Nov 2024 16:33
 Operator : RC/JU
 Sample : P4801-03
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 GCPA4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG063328.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.301	28	36	45	rBV8	22679	62461	1.38%	0.162%
2	3.660	95	97	102	rBV5	5159	8686	0.19%	0.023%
3	3.713	102	106	111	rBV	47915	75502	1.67%	0.196%
4	4.488	234	238	240	rBV4	6978	11925	0.26%	0.031%
5	4.570	243	252	259	rVB3	131976	266697	5.91%	0.693%
6	5.135	344	348	352	rBV6	11214	20145	0.45%	0.052%
7	5.487	404	408	411	rBV3	9934	15351	0.34%	0.040%
8	7.009	660	667	674	rBV	132242	243568	5.40%	0.633%
9	7.062	674	676	679	rVB3	5674	6753	0.15%	0.018%
10	7.162	687	693	702	rBV	305528	514222	11.39%	1.336%
11	7.367	720	728	739	rBV	377599	643428	14.25%	1.672%
12	7.767	791	796	797	rVB5	5451	6952	0.15%	0.018%
13	7.831	801	807	815	rBV	363469	612437	13.57%	1.591%
14	8.484	912	918	919	rBV4	6229	8365	0.19%	0.022%
15	8.542	921	928	936	rVV	406181	704528	15.61%	1.831%
16	8.989	997	1004	1014	rBV	453122	794090	17.59%	2.063%
17	9.095	1021	1022	1029	rVB4	4389	7947	0.18%	0.021%
18	9.412	1072	1076	1083	rVB2	14815	20697	0.46%	0.054%
19	9.706	1120	1126	1136	rBV	412856	728144	16.13%	1.892%
20	10.246	1211	1218	1228	rBV	622169	1163485	25.77%	3.023%
21	10.622	1274	1282	1290	rBV	599048	1055681	23.39%	2.743%
22	10.757	1298	1305	1316	rBV2	287841	542600	12.02%	1.410%
23	11.909	1496	1501	1507	rVB3	26573	44724	0.99%	0.116%
24	12.214	1549	1553	1562	rBV5	11761	29696	0.66%	0.077%
25	12.508	1601	1603	1606	rBV2	7180	6410	0.14%	0.017%
26	12.820	1652	1656	1659	rBV4	4572	7603	0.17%	0.020%
27	13.360	1743	1748	1754	rBV2	30020	51590	1.14%	0.134%
28	13.877	1829	1836	1846	rVB	1423813	1990326	44.09%	5.171%
29	14.165	1875	1885	1893	rBV2	1341829	2189962	48.51%	5.690%
30	14.471	1930	1937	1944	rBV	1131283	1718415	38.07%	4.465%
31	14.612	1957	1961	1965	rVB4	4864	8005	0.18%	0.021%
32	14.682	1968	1973	1982	rBV3	113258	238204	5.28%	0.619%
33	15.276	2069	2074	2081	rVB2	34946	55145	1.22%	0.143%
34	15.358	2084	2088	2093	rVB3	5862	9149	0.20%	0.024%
35	15.399	2093	2095	2100	rBV2	4119	7647	0.17%	0.020%
36	15.469	2100	2107	2116	rBV	2004870	3099329	68.66%	8.053%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111124\
 Data File : BG063328.D
 Acq On : 12 Nov 2024 16:33
 Operator : RC/JU
 Sample : P4801-03
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 GCPA4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
 Title : SVOA CALIBRATION

37	15.593	2121	2128	2136	rBV	658531	1014271	22.47%	2.635%
38	15.704	2143	2147	2151	rBV7	11802	15968	0.35%	0.041%
39	16.081	2207	2211	2212	rBV4	5552	6723	0.15%	0.017%
40	16.363	2255	2259	2265	rBV5	7099	14118	0.31%	0.037%
41	16.703	2313	2317	2320	rBV3	8714	10871	0.24%	0.028%
42	17.009	2367	2369	2373	rBV3	5157	7680	0.17%	0.020%
43	17.091	2381	2383	2387	rBV4	10433	9928	0.22%	0.026%
44	17.144	2387	2392	2396	rBV2	44647	58099	1.29%	0.151%
45	17.220	2399	2405	2415	rVV	1497636	2186978	48.45%	5.682%
46	17.320	2415	2422	2434	rVV	2469423	3631403	80.44%	9.435%
47	17.514	2452	2455	2457	rBV4	9550	12109	0.27%	0.031%
48	17.591	2465	2468	2469	rBV2	6151	7208	0.16%	0.019%
49	17.708	2487	2488	2494	rVB5	7232	8235	0.18%	0.021%
50	17.890	2514	2519	2526	rVB7	57947	89066	1.97%	0.231%
51	18.066	2546	2549	2553	rVB5	7106	7302	0.16%	0.019%
52	18.125	2555	2559	2563	rBV7	24725	40766	0.90%	0.106%
53	18.184	2567	2569	2573	rVB5	7516	8611	0.19%	0.022%
54	18.266	2579	2583	2585	rBV5	6100	8827	0.20%	0.023%
55	18.337	2590	2595	2603	rBV2	82011	152570	3.38%	0.396%
56	18.548	2628	2631	2634	rVB3	16347	19859	0.44%	0.052%
57	19.071	2717	2720	2724	rVB6	20390	27822	0.62%	0.072%
58	19.183	2735	2739	2747	rVB2	43317	67496	1.50%	0.175%
59	19.253	2747	2751	2755	rBV2	36999	54555	1.21%	0.142%
60	19.618	2807	2813	2820	rBV	3129987	4514272	100.00%	11.729%
61	19.835	2848	2850	2852	rBV3	7472	6982	0.15%	0.018%
62	19.853	2852	2853	2855	rVB2	10695	7127	0.16%	0.019%
63	21.474	3122	3129	3141	rBV	1682371	2551517	56.52%	6.629%
64	24.300	3600	3610	3623	rBV	1692053	4369066	96.78%	11.352%
65	24.506	3636	3645	3659	rVB2	963579	2608328	57.78%	6.777%




Sum of corrected areas: 38487626

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111124\
Data File : BG063328.D
Acq On : 12 Nov 2024 16:33
Operator : RC/JU
Sample : P4801-03
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
GCPA4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

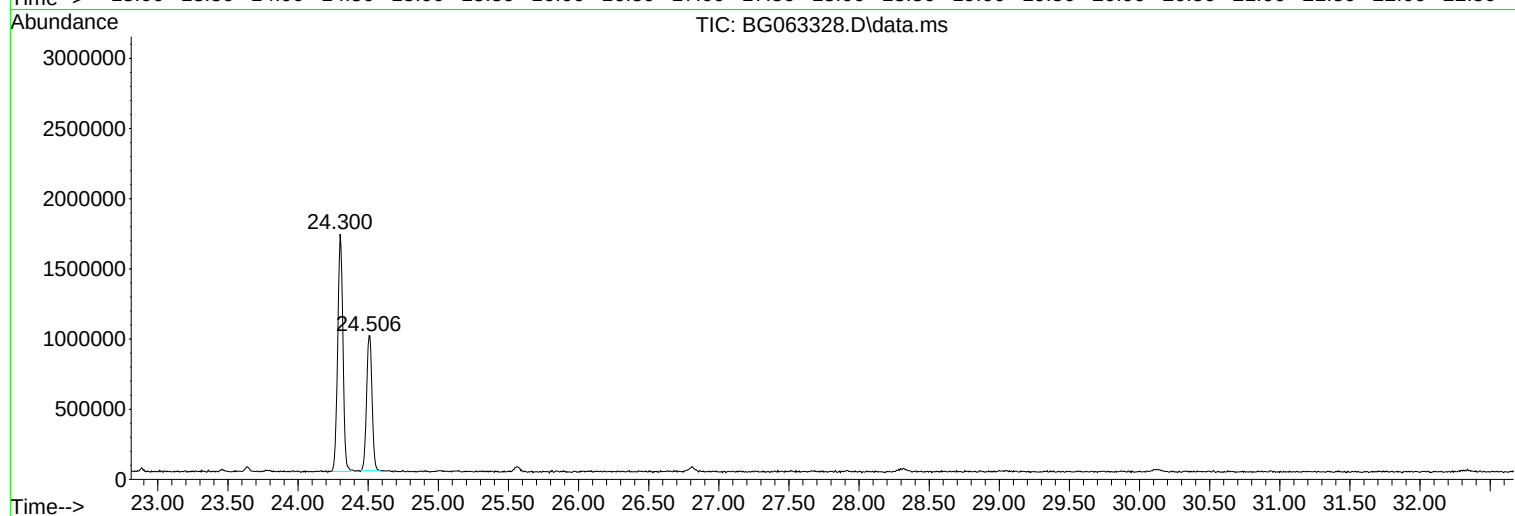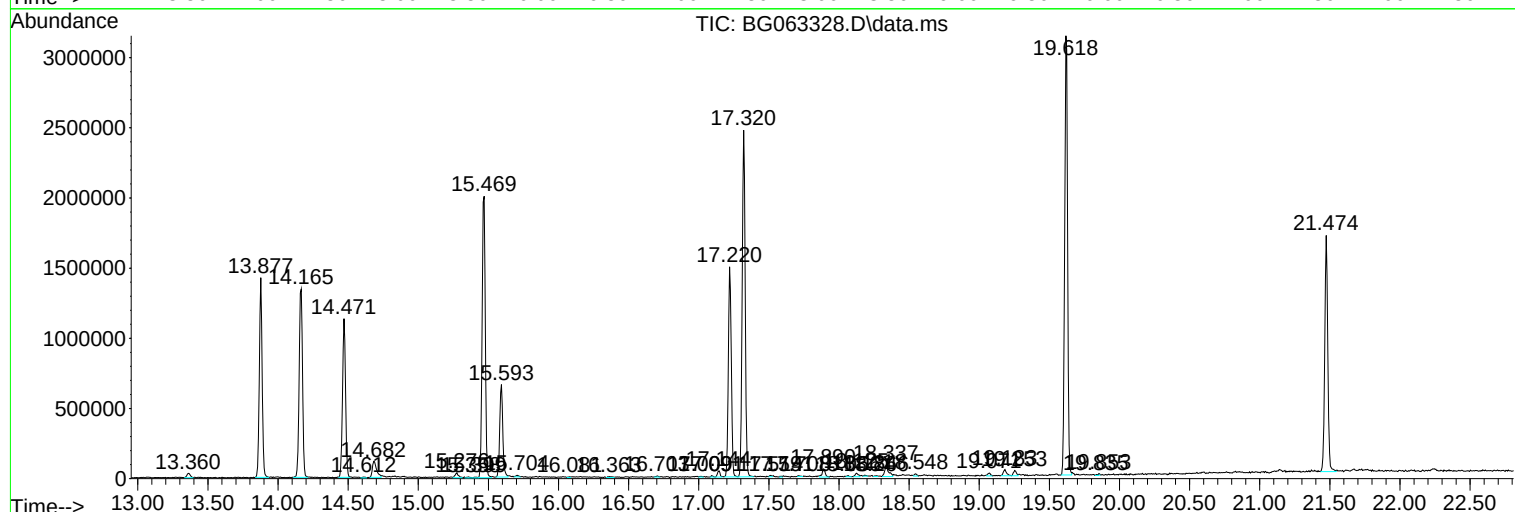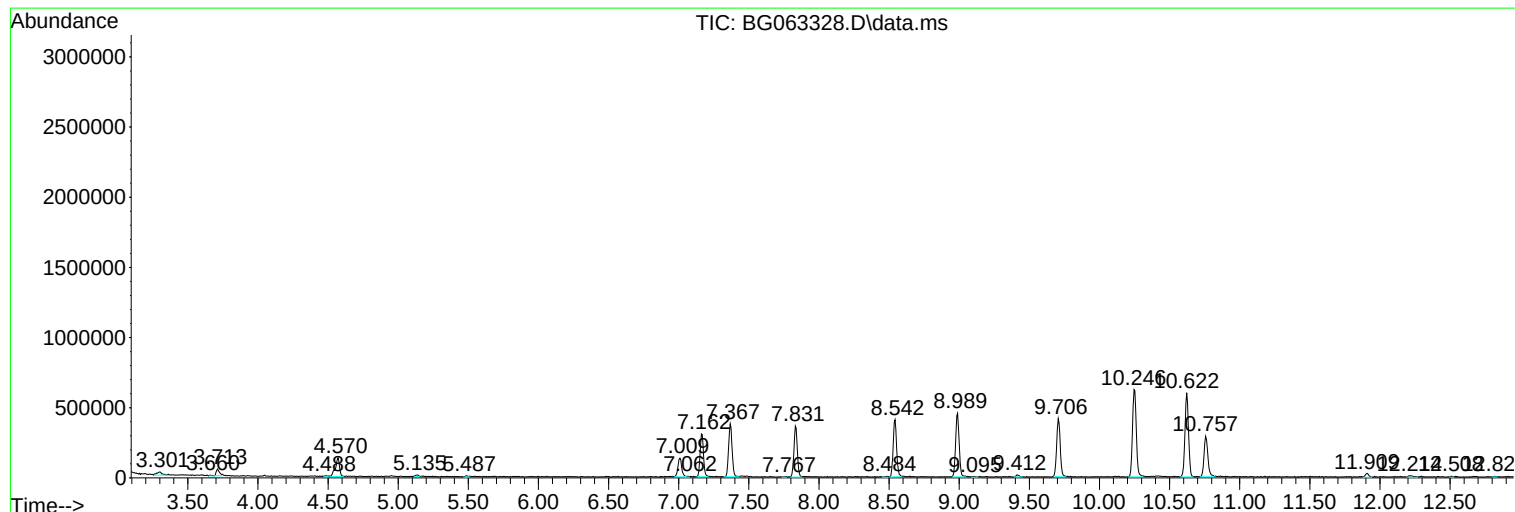

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111124\
Data File : BG063328.D
Acq On : 12 Nov 2024 16:33
Operator : RC/JU
Sample : P4801-03
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
GCPA4










Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Tetrachloroethylene Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.570	8.71 ng/ul	266697	1,4-Dichlorobenzene-d4	7.837

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Tetrachloroethylene	164	C2Cl4	000127-18-4	97
2			Tetrachloroethylene	164	C2Cl4	000127-18-4	96
3			Tetrachloroethylene	164	C2Cl4	000127-18-4	95
4			Tetrachloroethylene	164	C2Cl4	000127-18-4	95
5			Pyrimidine, 5-fluoro-2,4-dichloro-	166	C4HC12FN2	002927-71-1	43

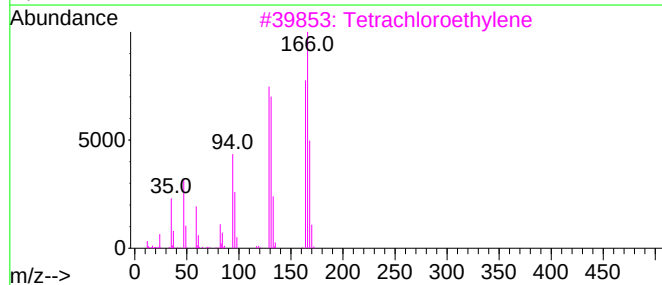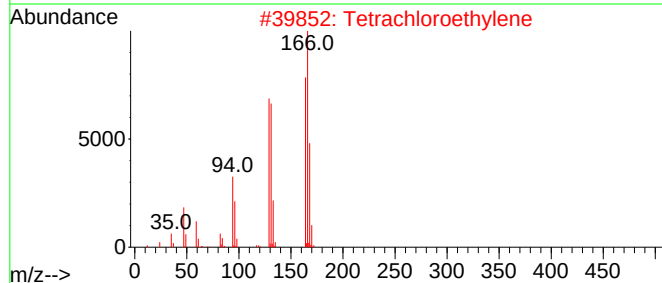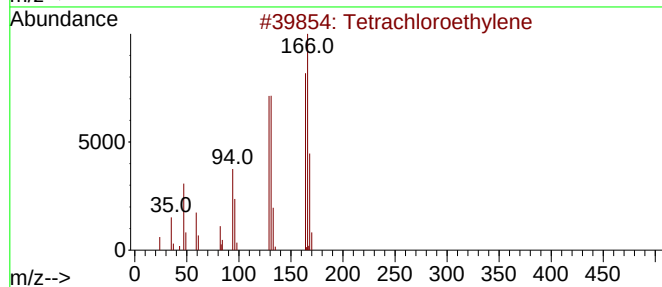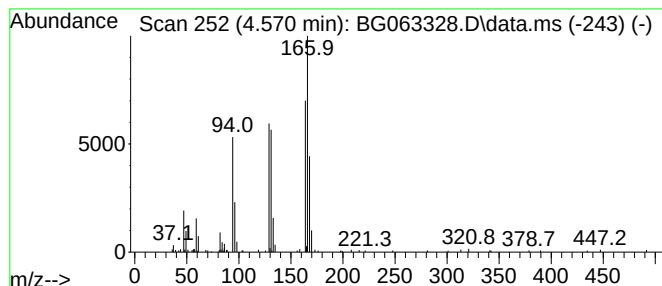

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111124\
Data File : BG063328.D
Acq On : 12 Nov 2024 16:33
Operator : RC/JU
Sample : P4801-03
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
GCPA4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Tetrachloroethy...	4.570	8.7	ng/ul	266697	1	7.837	612437	20.0