

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111124\
 Data File : BG063330.D
 Acq On : 12 Nov 2024 18:03
 Operator : RC/JU
 Sample : P4801-05
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 GCPA6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG063330.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.296	33	35	40	rVB2	22621	25621	0.58%	0.067%
2	3.713	102	106	114	rVB	35837	68175	1.55%	0.178%
3	4.565	242	251	259	rBV3	123690	242694	5.51%	0.633%
4	4.795	288	290	294	rVB6	7152	7129	0.16%	0.019%
5	4.941	311	315	316	rBV2	6511	6936	0.16%	0.018%
6	5.482	404	407	411	rBV5	5557	10325	0.23%	0.027%
7	5.911	477	480	486	rBV4	4405	7536	0.17%	0.020%
8	7.004	658	666	673	rBV	142366	251565	5.72%	0.656%
9	7.162	686	693	702	rBV	302031	490211	11.14%	1.279%
10	7.368	721	728	737	rBV	352515	604352	13.73%	1.577%
11	7.832	800	807	815	rBV	344257	588081	13.36%	1.534%
12	8.537	920	927	938	rBV	423089	742481	16.87%	1.937%
13	8.984	996	1003	1011	rBV	431020	747485	16.98%	1.950%
14	9.148	1027	1031	1032	rBV2	5246	6986	0.16%	0.018%
15	9.413	1072	1076	1080	rVB3	10362	14049	0.32%	0.037%
16	9.706	1116	1126	1136	rBV2	408310	720960	16.38%	1.881%
17	10.059	1183	1186	1189	rBV4	4213	6330	0.14%	0.017%
18	10.247	1211	1218	1227	rBV	636049	1128954	25.65%	2.945%
19	10.623	1273	1282	1290	rBV	569855	1019551	23.16%	2.660%
20	10.758	1297	1305	1321	rBV2	405631	778860	17.69%	2.032%
21	11.169	1372	1375	1379	rBV3	5729	6056	0.14%	0.016%
22	11.916	1499	1502	1507	rVB3	13721	15980	0.36%	0.042%
23	12.221	1548	1554	1557	rBV3	10425	18485	0.42%	0.048%
24	13.249	1724	1729	1732	rVB2	4281	7255	0.16%	0.019%
25	13.367	1743	1749	1755	rVB2	73089	128084	2.91%	0.334%
26	13.878	1829	1836	1843	rBV	1421312	2049865	46.57%	5.348%
27	14.007	1850	1858	1859	rBV3	7521	14232	0.32%	0.037%
28	14.160	1874	1884	1894	rBV	1372130	2233832	50.75%	5.827%
29	14.254	1898	1900	1906	rVB3	5134	7035	0.16%	0.018%
30	14.471	1929	1937	1944	rBV2	1127747	1723367	39.15%	4.496%
31	14.683	1968	1973	1982	rBV3	128216	254025	5.77%	0.663%
32	15.270	2069	2073	2078	rBV2	13563	21178	0.48%	0.055%
33	15.464	2098	2106	2114	rBV	2022650	3086286	70.11%	8.051%
34	15.594	2122	2128	2137	rBV	634575	971338	22.07%	2.534%
35	15.711	2144	2148	2153	rVB8	14220	21107	0.48%	0.055%
36	15.776	2156	2159	2163	rVB5	5937	7906	0.18%	0.021%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111124\
 Data File : BG063330.D
 Acq On : 12 Nov 2024 18:03
 Operator : RC/JU
 Sample : P4801-05
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 GCPA6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
 Title : SVOA CALIBRATION

37	16.040	2199	2204	2207	rBV5	5538	8137	0.18%	0.021%
38	16.363	2253	2259	2261	rBV5	11328	15182	0.34%	0.040%
39	16.704	2313	2317	2322	rBV6	8513	15725	0.36%	0.041%
40	16.810	2333	2335	2337	rBV3	7979	6577	0.15%	0.017%
41	16.992	2362	2366	2368	rBV4	5501	6075	0.14%	0.016%
42	17.010	2368	2369	2374	rVB4	5614	6788	0.15%	0.018%
43	17.145	2388	2392	2396	rVB3	66797	87259	1.98%	0.228%
44	17.221	2398	2405	2414	rVV	1479153	2171133	49.32%	5.664%
45	17.321	2415	2422	2432	rVB	2391872	3577293	81.27%	9.332%
46	17.709	2486	2488	2490	rBV3	14707	15629	0.36%	0.041%
47	17.891	2514	2519	2525	rVB4	77449	100720	2.29%	0.263%
48	18.055	2545	2547	2552	rVB5	19167	24417	0.55%	0.064%
49	18.126	2554	2559	2562	rBV5	32759	52114	1.18%	0.136%
50	18.337	2590	2595	2600	rBV	122769	211702	4.81%	0.552%
51	18.549	2628	2631	2637	rVB3	39659	48777	1.11%	0.127%
52	18.614	2639	2642	2645	rBV5	12810	13664	0.31%	0.036%
53	19.072	2717	2720	2726	rVB7	35804	48309	1.10%	0.126%
54	19.184	2732	2739	2744	rBV2	40322	69986	1.59%	0.183%
55	19.254	2747	2751	2754	rBV	34053	49055	1.11%	0.128%
56	19.618	2806	2813	2824	rBV	3164157	4401835	100.00%	11.483%
57	20.118	2896	2898	2899	rBV2	8786	7219	0.16%	0.019%
58	20.194	2909	2911	2912	rBV2	9784	7938	0.18%	0.021%
59	21.475	3122	3129	3138	rBV	1610879	2522924	57.32%	6.582%
60	24.301	3600	3610	3621	rBV	1671249	4240388	96.33%	11.062%
61	24.507	3636	3645	3656	rVB	966258	2580441	58.62%	6.732%
62	28.890	4389	4391	4392	rBV2	14492	8998	0.20%	0.023%




Sum of corrected areas: 38332597

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111124\
Data File : BG063330.D
Acq On : 12 Nov 2024 18:03
Operator : RC/JU
Sample : P4801-05
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
GCPA6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

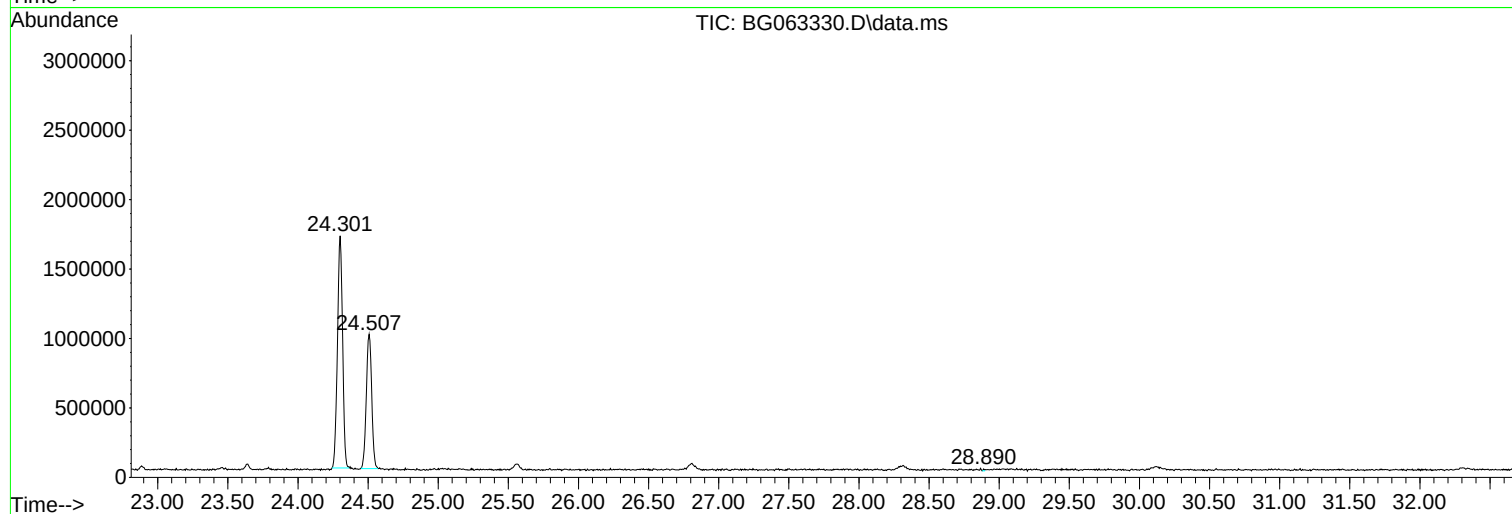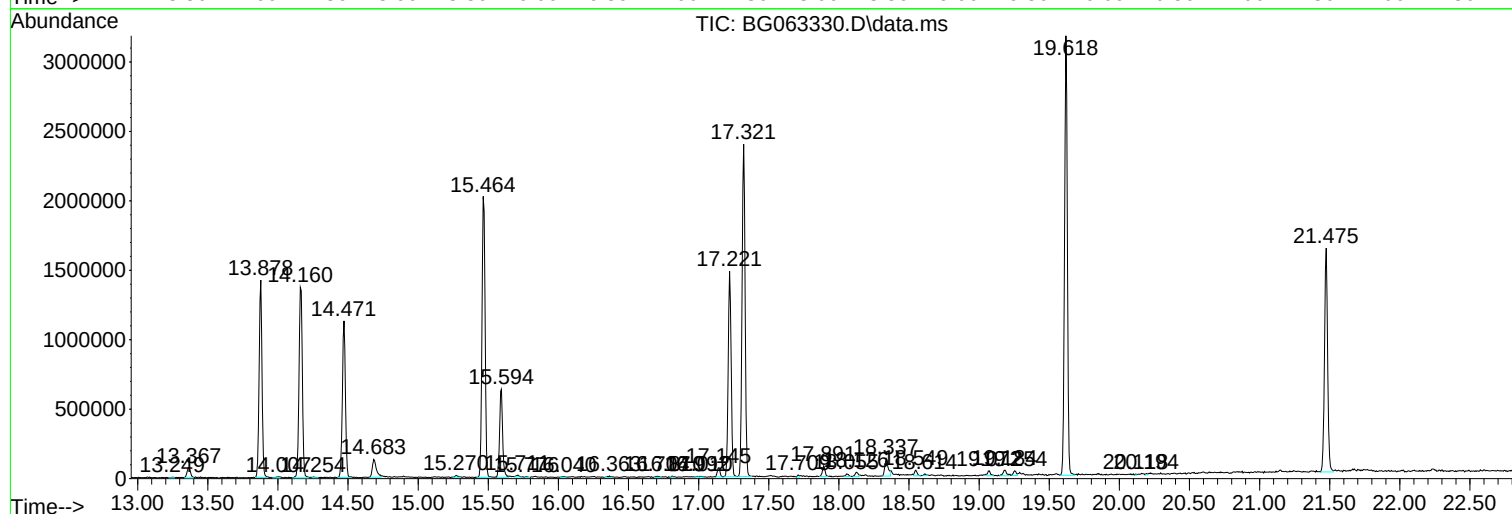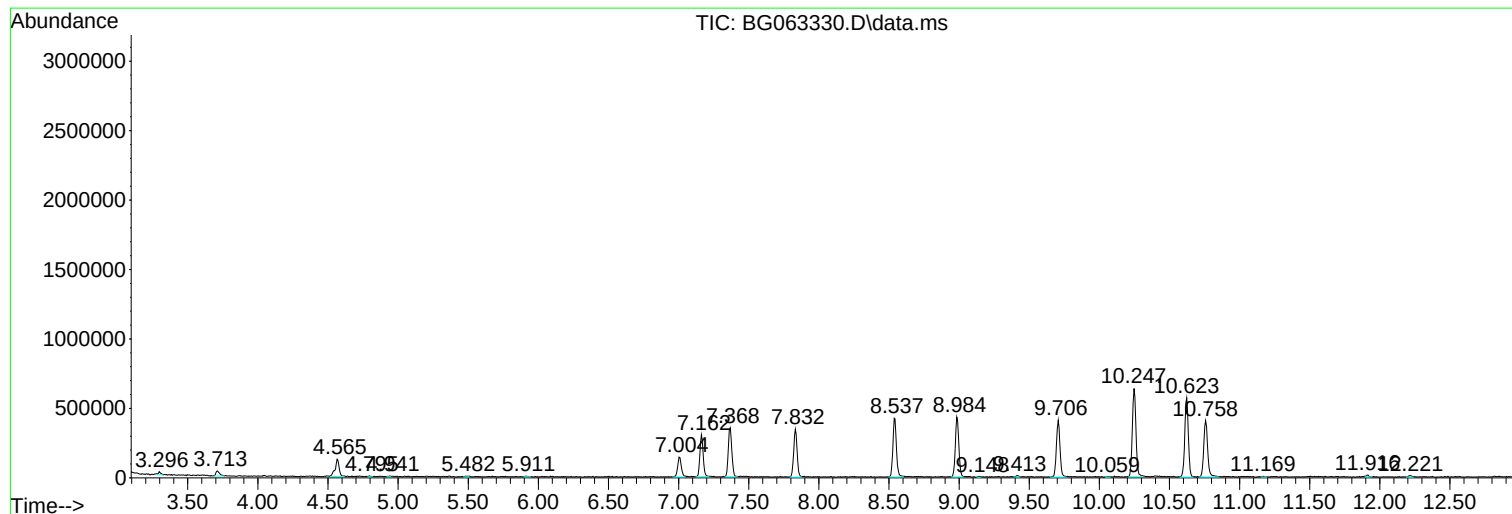

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111124\
Data File : BG063330.D
Acq On : 12 Nov 2024 18:03
Operator : RC/JU
Sample : P4801-05
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
GCPA6










Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Tetrachloroethylene Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.565	8.25 ng/ul	242694	1,4-Dichlorobenzene-d4	7.832

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Tetrachloroethylene	164	C2Cl4	000127-18-4	95
2			Tetrachloroethylene	164	C2Cl4	000127-18-4	95
3			Tetrachloroethylene	164	C2Cl4	000127-18-4	94
4			Tetrachloroethylene	164	C2Cl4	000127-18-4	93
5			Pyrimidine, 5-fluoro-2,4-dichloro-	166	C4HC12FN2	002927-71-1	27

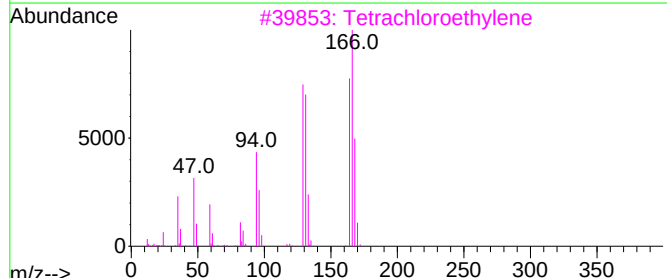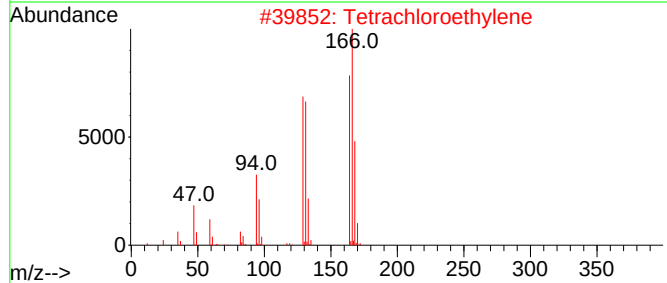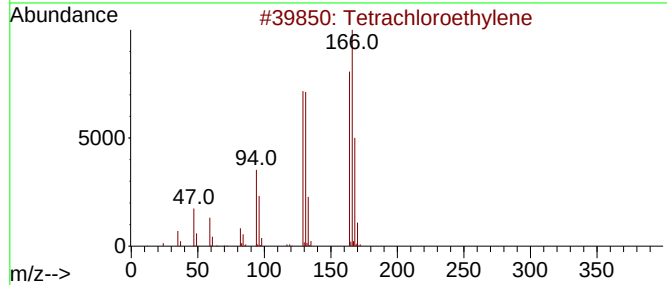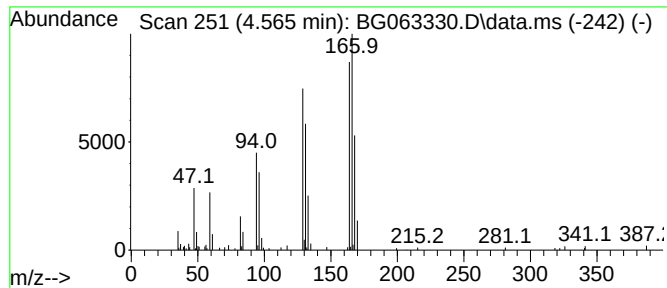

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111124\
Data File : BG063330.D
Acq On : 12 Nov 2024 18:03
Operator : RC/JU
Sample : P4801-05
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
GCPA6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Tetrachloroethy...	4.565	8.3	ng/u1	242694	1	7.832	588081	20.0