

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111124\
 Data File : BG063336.D
 Acq On : 12 Nov 2024 21:51
 Operator : RC/JU
 Sample : PB164901BL
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK901

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG063336.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.296	32	35	41	rVB3	21935	32421	0.78%	0.083%
2	3.701	100	104	113	rBV	318440	506117	12.16%	1.302%
3	4.042	159	162	166	rVB5	6213	9381	0.23%	0.024%
4	5.070	334	337	339	rBV2	5395	6085	0.15%	0.016%
5	5.123	343	346	349	rBV3	3698	5762	0.14%	0.015%
6	5.458	401	403	406	rBV3	5111	6034	0.14%	0.016%
7	5.922	479	482	484	rBV3	5217	6188	0.15%	0.016%
8	6.622	597	601	606	rVB3	3579	6040	0.15%	0.016%
9	7.009	659	667	675	rBV	463523	804931	19.34%	2.071%
10	7.162	686	693	702	rBV	316798	535565	12.87%	1.378%
11	7.368	722	728	736	rBV	436523	721928	17.34%	1.857%
12	7.832	801	807	816	rBV	336458	557439	13.39%	1.434%
13	8.543	921	928	936	rBV	627394	1087833	26.13%	2.799%
14	8.983	996	1003	1012	rBV	450777	793726	19.07%	2.042%
15	9.077	1016	1019	1022	rBV3	4238	6279	0.15%	0.016%
16	9.195	1033	1039	1040	rBV4	13915	18328	0.44%	0.047%
17	9.706	1118	1126	1134	rBV	447532	776556	18.66%	1.998%
18	10.247	1210	1218	1230	rBV	679943	1232859	29.62%	3.172%
19	10.623	1274	1282	1290	rBV	562633	970959	23.33%	2.498%
20	10.758	1298	1305	1318	rBV	614443	1107692	26.61%	2.850%
21	11.539	1435	1438	1441	rBV2	5647	7238	0.17%	0.019%
22	11.592	1445	1447	1451	rBV	4764	5959	0.14%	0.015%
23	11.651	1454	1457	1460	rBV4	5556	8546	0.21%	0.022%
24	11.798	1480	1482	1486	rBV	4482	7220	0.17%	0.019%
25	11.962	1506	1510	1514	rVB3	5559	8176	0.20%	0.021%
26	12.221	1550	1554	1559	rBV4	10434	13797	0.33%	0.035%
27	12.521	1602	1605	1609	rBV	5403	8191	0.20%	0.021%
28	13.878	1826	1836	1843	rBV	1358095	1971733	47.37%	5.073%
29	14.160	1877	1884	1895	rVB	1499462	2335781	56.11%	6.010%
30	14.471	1931	1937	1943	rBV	1061807	1623343	39.00%	4.177%
31	14.677	1966	1972	1983	rBV	418703	784135	18.84%	2.017%
32	14.888	2006	2008	2012	rVB3	7658	8943	0.21%	0.023%
33	15.464	2097	2106	2114	rBV	1957618	3016731	72.47%	7.762%
34	15.588	2121	2127	2137	rBV	550850	859572	20.65%	2.212%
35	15.705	2144	2147	2153	rVB3	13052	21616	0.52%	0.056%
36	15.823	2165	2167	2172	rBV5	7559	10345	0.25%	0.027%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111124\
 Data File : BG063336.D
 Acq On : 12 Nov 2024 21:51
 Operator : RC/JU
 Sample : PB164901BL
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK901

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
 Title : SVOA CALIBRATION

37	16.152	2219	2223	2226	rBV4	7728	10428	0.25%	0.027%
38	16.251	2233	2240	2247	rVB7	8133	16677	0.40%	0.043%
39	16.616	2299	2302	2305	rBV3	3825	5748	0.14%	0.015%
40	16.992	2362	2366	2368	rBV2	7350	11217	0.27%	0.029%
41	17.115	2383	2387	2390	rBV2	5142	7378	0.18%	0.019%
42	17.221	2398	2405	2414	rBV	1439935	2135038	51.29%	5.493%
43	17.321	2415	2422	2429	rVV	2395255	3405928	81.82%	8.763%
44	17.456	2444	2445	2449	rBV	6299	8278	0.20%	0.021%
45	17.885	2516	2518	2522	rVB4	8990	9248	0.22%	0.024%
46	18.731	2660	2662	2665	rVB4	7610	6565	0.16%	0.017%
47	18.919	2692	2694	2699	rBV5	4519	8112	0.19%	0.021%
48	18.978	2702	2704	2706	rVB2	6724	6439	0.15%	0.017%
49	19.183	2735	2739	2744	rBV4	33006	49317	1.18%	0.127%
50	19.254	2747	2751	2757	rVB2	28741	45468	1.09%	0.117%
51	19.553	2798	2802	2804	rVB4	10795	13163	0.32%	0.034%
52	19.618	2807	2813	2827	rVB	3000620	4162659	100.00%	10.710%
53	19.918	2863	2864	2870	rVB5	8397	8379	0.20%	0.022%
54	21.475	3122	3129	3140	rBV	1604633	2473133	59.41%	6.363%
55	24.301	3600	3610	3624	rVB	1625379	4095304	98.38%	10.537%
56	24.506	3636	3645	3656	rVB	952092	2504958	60.18%	6.445%




Sum of corrected areas: 38866886

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111124\
Data File : BG063336.D
Acq On : 12 Nov 2024 21:51
Operator : RC/JU
Sample : PB164901BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK901

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

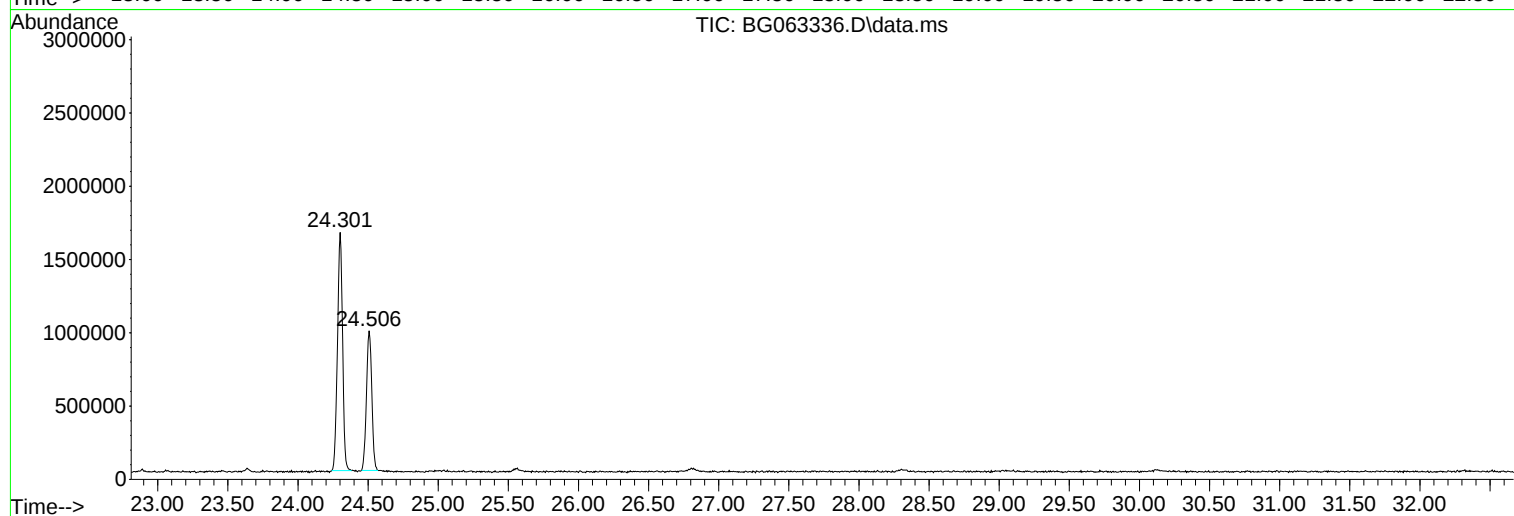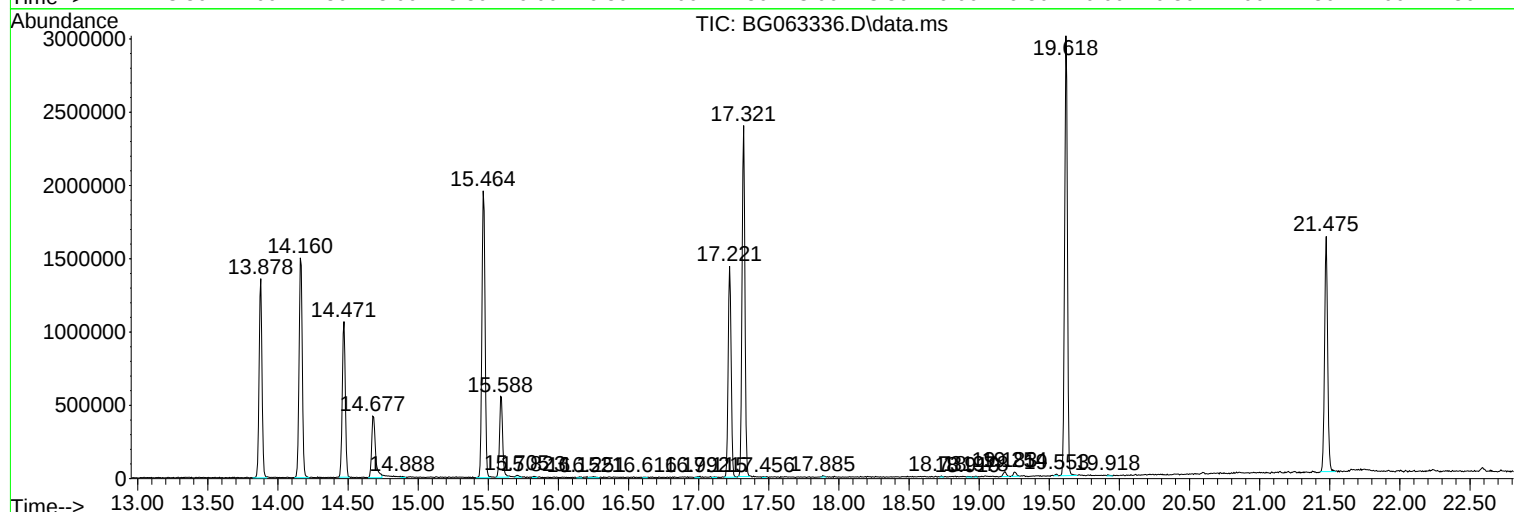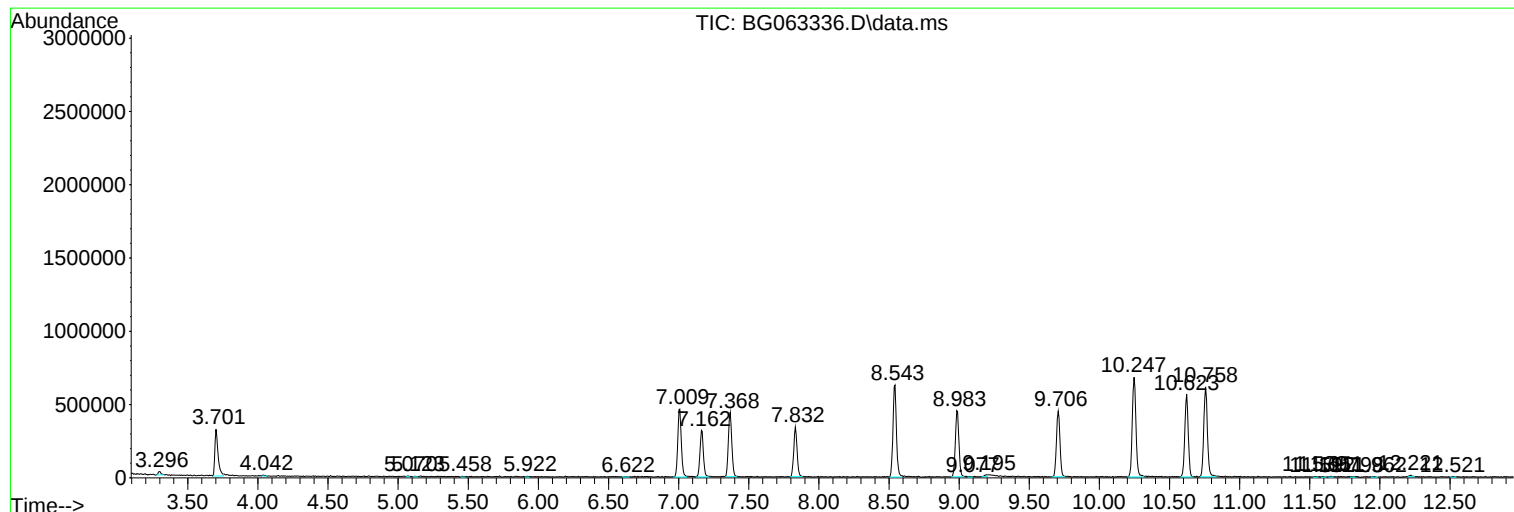

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111124\
Data File : BG063336.D
Acq On : 12 Nov 2024 21:51
Operator : RC/JU
Sample : PB164901BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK901

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111124\
Data File : BG063336.D
Acq On : 12 Nov 2024 21:51
Operator : RC/JU
Sample : PB164901BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK901

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc