

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111124\
 Data File : BG063338.D
 Acq On : 12 Nov 2024 23:44
 Operator : RC/JU
 Sample : PB164897BL
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK897

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG063338.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.299	32	36	40	rBV	28203	34858	0.78%	0.082%
2	3.699	100	104	113	rBV	334475	545043	12.13%	1.282%
3	4.040	158	162	166	rVB5	7793	13664	0.30%	0.032%
4	4.598	253	257	262	rBV6	5054	9479	0.21%	0.022%
5	4.839	296	298	304	rVB6	4052	7826	0.17%	0.018%
6	4.939	311	315	316	rBV2	4901	6067	0.14%	0.014%
7	5.332	379	382	384	rBV3	5256	6045	0.13%	0.014%
8	5.473	403	406	411	rBV3	3767	6550	0.15%	0.015%
9	6.314	547	549	552	rVB3	6173	6898	0.15%	0.016%
10	6.842	637	639	644	rVB3	5124	6160	0.14%	0.014%
11	7.007	658	667	676	rBV	515440	876742	19.51%	2.062%
12	7.165	687	694	702	rBV	359770	574741	12.79%	1.352%
13	7.365	722	728	736	rBV	489766	822547	18.31%	1.935%
14	7.835	798	808	817	rBV	373926	643516	14.32%	1.514%
15	8.540	920	928	939	rBV	698344	1190966	26.51%	2.801%
16	8.734	959	961	964	rVB2	5393	6464	0.14%	0.015%
17	8.811	971	974	979	rVB	4118	6642	0.15%	0.016%
18	8.987	996	1004	1012	rBV	512108	879082	19.56%	2.068%
19	9.192	1034	1039	1040	rBV5	14028	15808	0.35%	0.037%
20	9.710	1119	1127	1136	rBV	484120	852721	18.98%	2.006%
21	10.244	1212	1218	1231	rBV	711553	1307947	29.11%	3.076%
22	10.420	1246	1248	1252	rVB3	5612	6499	0.14%	0.015%
23	10.620	1275	1282	1292	rBV	603777	1062573	23.65%	2.499%
24	10.755	1297	1305	1314	rBV2	632694	1187961	26.44%	2.794%
25	11.913	1499	1502	1509	rBV4	4531	11141	0.25%	0.026%
26	12.224	1547	1555	1559	rBV7	12206	28361	0.63%	0.067%
27	13.711	1807	1808	1814	rBV2	4338	7521	0.17%	0.018%
28	13.875	1828	1836	1851	rVB	1488628	2133233	47.48%	5.018%
29	14.163	1877	1885	1893	rBV	1607892	2517090	56.02%	5.920%
30	14.469	1929	1937	1947	rVB	1156076	1813615	40.36%	4.266%
31	14.680	1967	1973	1985	rBV2	486047	872103	19.41%	2.051%
32	14.886	2004	2008	2009	rBV3	7545	8150	0.18%	0.019%
33	15.467	2100	2107	2116	rBV	2245185	3309288	73.65%	7.784%
34	15.591	2120	2128	2140	rBV	639056	974590	21.69%	2.292%
35	15.703	2144	2147	2149	rBV4	8858	10693	0.24%	0.025%
36	16.249	2236	2240	2247	rVB4	8483	11785	0.26%	0.028%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111124\
Data File : BG063338.D
Acq On : 12 Nov 2024 23:44
Operator : RC/JU
Sample : PB164897BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK897

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
Title : SVOA CALIBRATION

37	17.218	2399	2405	2413	rBV	1555939	2351077	52.33%	5.530%
38	17.318	2416	2422	2432	rVV	2454014	3704413	82.45%	8.713%
39	17.888	2518	2519	2523	rVB3	11667	12285	0.27%	0.029%
40	18.200	2567	2572	2574	rBV5	5031	8078	0.18%	0.019%
41	18.734	2659	2663	2667	rVB3	4357	7507	0.17%	0.018%
42	18.905	2688	2692	2695	rBV5	4325	8212	0.18%	0.019%
43	19.181	2734	2739	2745	rBV2	42353	65171	1.45%	0.153%
44	19.251	2747	2751	2760	rVB	36639	60695	1.35%	0.143%
45	19.422	2778	2780	2785	rVB2	5975	7637	0.17%	0.018%
46	19.557	2797	2803	2805	rBV7	9904	18231	0.41%	0.043%
47	19.621	2808	2814	2823	rBV	3129586	4493162	100.00%	10.568%
48	19.968	2871	2873	2875	rBV3	6014	6720	0.15%	0.016%
49	21.472	3123	3129	3136	rBV	1763557	2701501	60.12%	6.354%
50	24.304	3600	3611	3624	rBV	1762192	4456665	99.19%	10.483%
51	24.510	3636	3646	3657	rVB	1086948	2839450	63.19%	6.679%




Sum of corrected areas: 42515173

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111124\
Data File : BG063338.D
Acq On : 12 Nov 2024 23:44
Operator : RC/JU
Sample : PB164897BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK897

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

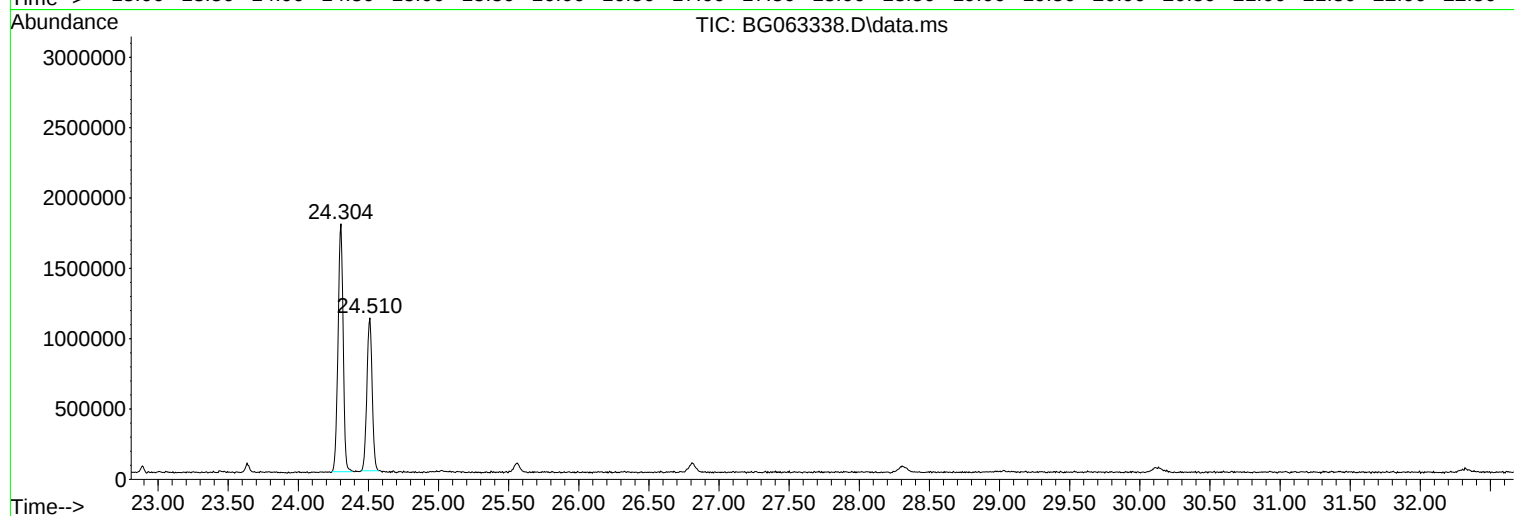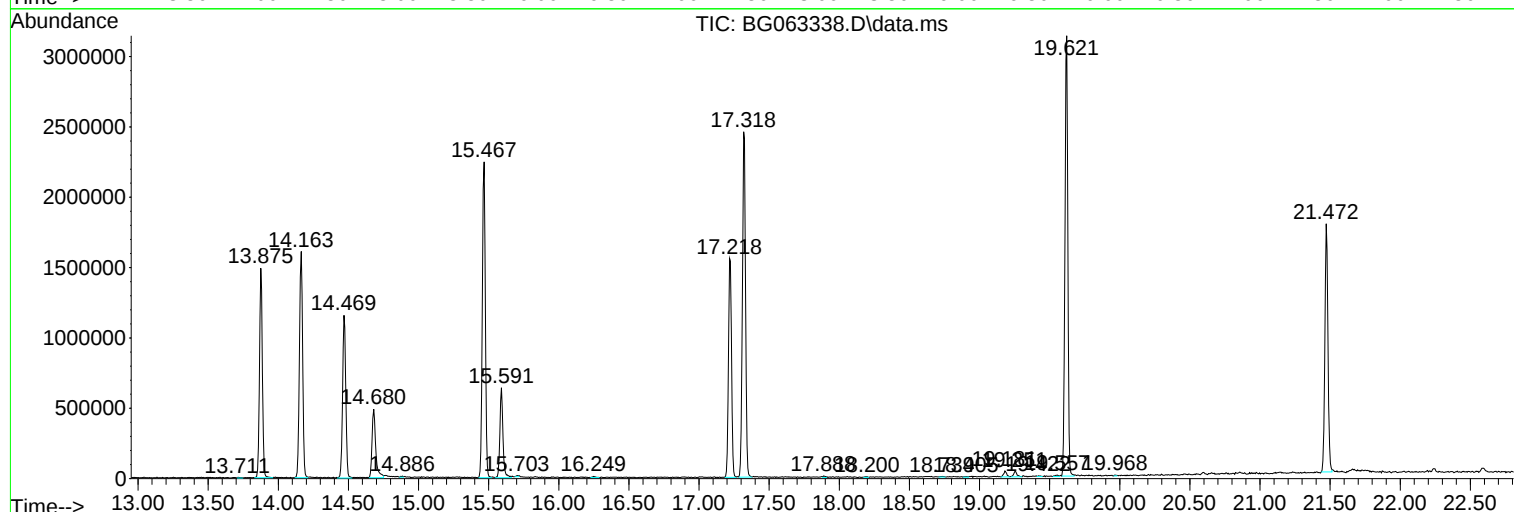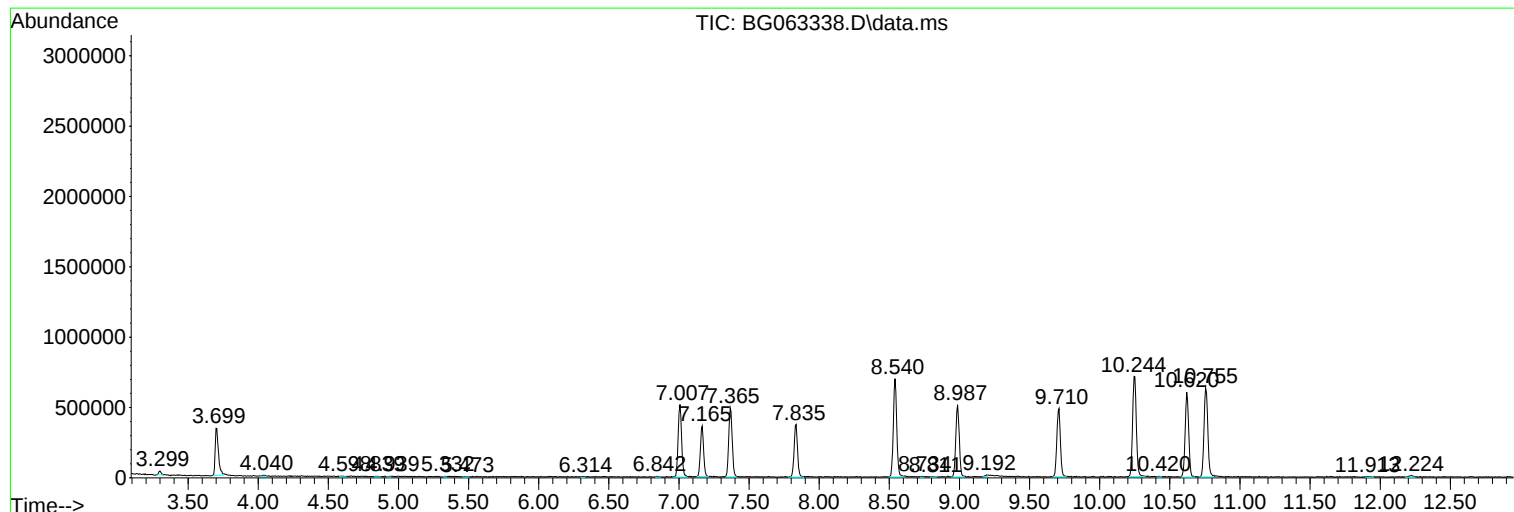

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111124\
Data File : BG063338.D
Acq On : 12 Nov 2024 23:44
Operator : RC/JU
Sample : PB164897BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK897

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111124\
Data File : BG063338.D
Acq On : 12 Nov 2024 23:44
Operator : RC/JU
Sample : PB164897BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK897

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc