

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111124\
 Data File : BG063339.D
 Acq On : 12 Nov 2024 00:22
 Operator : RC/JU
 Sample : PB164899BL
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK899

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG063339.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.200	17	19	22	rVB3	8214	7148	0.16%	0.017%
2	3.300	33	36	40	rVB2	25282	31310	0.72%	0.074%
3	3.699	100	104	117	rBV	319159	537443	12.32%	1.262%
4	4.052	158	164	165	rVB6	7960	10323	0.24%	0.024%
5	5.221	361	363	366	rBV4	5062	6013	0.14%	0.014%
6	7.007	661	667	678	rBV	475833	823512	18.88%	1.934%
7	7.166	686	694	703	rBV	351181	576696	13.22%	1.355%
8	7.366	721	728	737	rBV2	458083	792343	18.17%	1.861%
9	7.830	800	807	816	rBV	384935	660524	15.14%	1.552%
10	8.288	882	885	891	rVB4	4375	6706	0.15%	0.016%
11	8.541	921	928	936	rBV	677803	1154597	26.47%	2.712%
12	8.987	997	1004	1011	rBV	491312	861098	19.74%	2.023%
13	9.210	1031	1042	1046	rBV7	14534	44583	1.02%	0.105%
14	9.257	1048	1050	1055	rVB4	7838	10582	0.24%	0.025%
15	9.704	1117	1126	1135	rBV	459349	841566	19.30%	1.977%
16	9.945	1162	1167	1170	rBV2	5766	7708	0.18%	0.018%
17	10.244	1210	1218	1229	rBV	713465	1300170	29.81%	3.054%
18	10.621	1275	1282	1291	rBB	642467	1108796	25.42%	2.605%
19	10.756	1298	1305	1318	rBV	658809	1202487	27.57%	2.825%
20	12.213	1549	1553	1554	rBV	7357	9540	0.22%	0.022%
21	13.876	1829	1836	1845	rBV	1473136	2067613	47.41%	4.857%
22	14.163	1875	1885	1893	rBV	1590793	2453554	56.26%	5.763%
23	14.469	1929	1937	1945	rBV	1257112	1912690	43.86%	4.493%
24	14.680	1965	1973	1983	rBV	461556	827838	18.98%	1.945%
25	15.350	2085	2087	2093	rVB5	4001	6527	0.15%	0.015%
26	15.468	2100	2107	2119	rBV	2166158	3184760	73.02%	7.481%
27	15.591	2122	2128	2138	rBV	610623	926290	21.24%	2.176%
28	15.691	2143	2145	2146	rVV2	8060	7645	0.18%	0.018%
29	15.703	2146	2147	2154	rVB3	14542	19499	0.45%	0.046%
30	15.826	2165	2168	2171	rBV5	7134	8915	0.20%	0.021%
31	16.249	2237	2240	2244	rBV3	9718	14219	0.33%	0.033%
32	16.602	2297	2300	2302	rBV3	5658	5901	0.14%	0.014%
33	16.901	2348	2351	2353	rBV2	7341	7472	0.17%	0.018%
34	17.225	2399	2406	2413	rBV	1605607	2434327	55.82%	5.718%
35	17.319	2415	2422	2431	rBV	2353899	3582379	82.14%	8.415%
36	17.489	2449	2451	2456	rVB5	5227	6813	0.16%	0.016%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111124\
 Data File : BG063339.D
 Acq On : 12 Nov 2024 00:22
 Operator : RC/JU
 Sample : PB164899BL
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK899

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
 Title : SVOA CALIBRATION

37	17.636	2475	2476	2482	rVB4	5193	7829	0.18%	0.018%
38	17.888	2516	2519	2524	rVB4	8894	13820	0.32%	0.032%
39	18.194	2568	2571	2572	rBV2	5819	6660	0.15%	0.016%
40	18.505	2621	2624	2627	rBV4	5075	6591	0.15%	0.015%
41	18.635	2642	2646	2647	rVB4	6904	8024	0.18%	0.019%
42	19.128	2726	2730	2731	rBV3	5358	6251	0.14%	0.015%
43	19.181	2735	2739	2745	rVB3	37054	57120	1.31%	0.134%
44	19.252	2748	2751	2758	rVV	32852	46101	1.06%	0.108%
45	19.545	2796	2801	2806	rBV8	8093	14294	0.33%	0.034%
46	19.622	2807	2814	2823	rBV	3063094	4352328	99.79%	10.223%
47	20.591	2978	2979	2984	rBV5	16626	13193	0.30%	0.031%
48	20.809	3014	3016	3018	rBV3	10432	9888	0.23%	0.023%
49	21.473	3123	3129	3138	rBV	1842234	2796684	64.12%	6.569%
50	22.242	3256	3260	3263	rBV5	21409	31692	0.73%	0.074%
51	22.589	3317	3319	3325	rVB6	32896	38890	0.89%	0.091%
52	23.641	3492	3498	3504	rBV6	63425	143992	3.30%	0.338%
53	24.304	3601	3611	3626	rVB	1649321	4361350	100.00%	10.245%
54	24.510	3636	3646	3657	rVB	1125737	2973539	68.18%	6.985%
55	25.562	3818	3825	3836	rVB7	77398	224362	5.14%	0.527%




Sum of corrected areas: 42572195

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111124\
Data File : BG063339.D
Acq On : 12 Nov 2024 00:22
Operator : RC/JU
Sample : PB164899BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK899

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

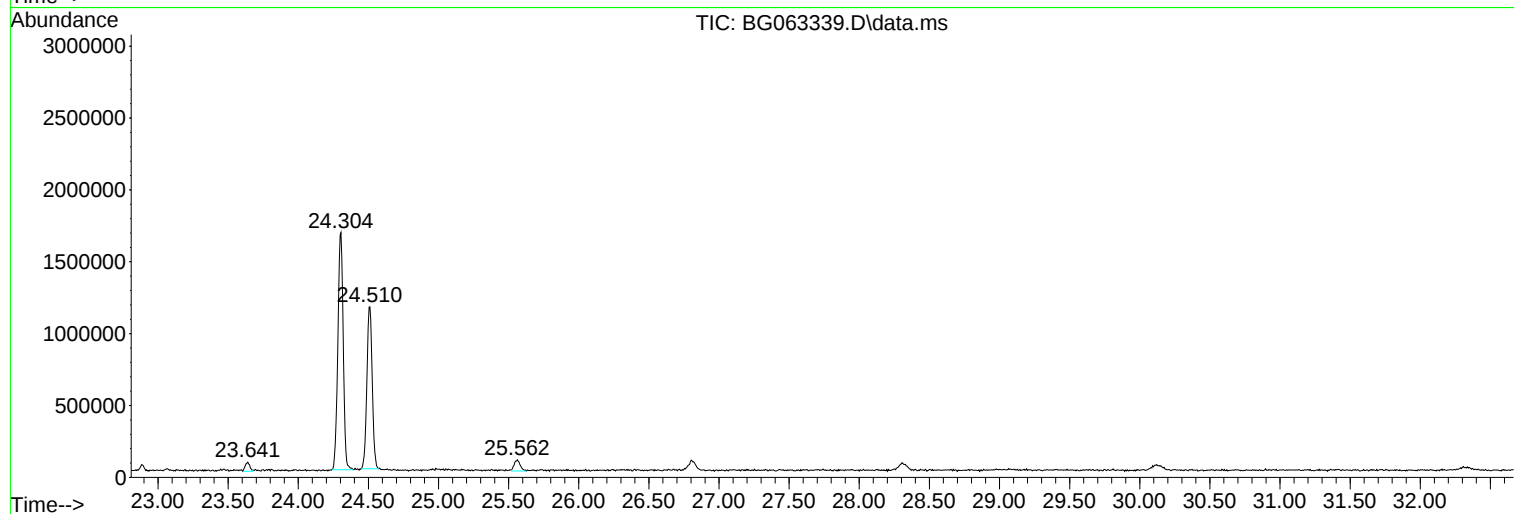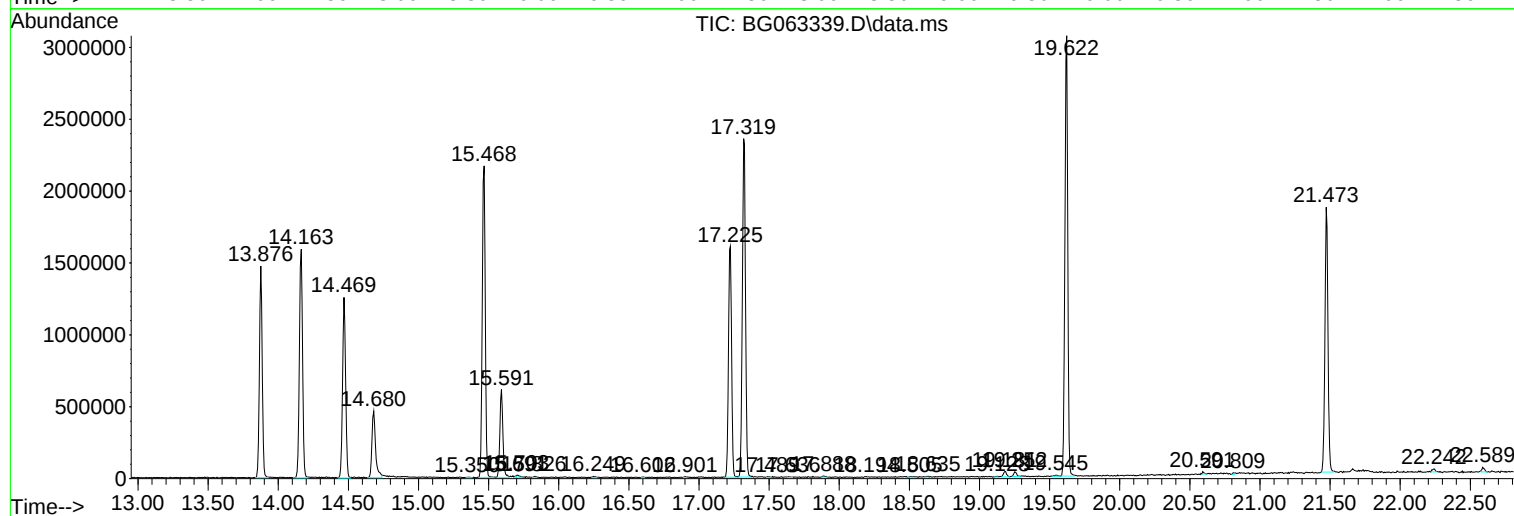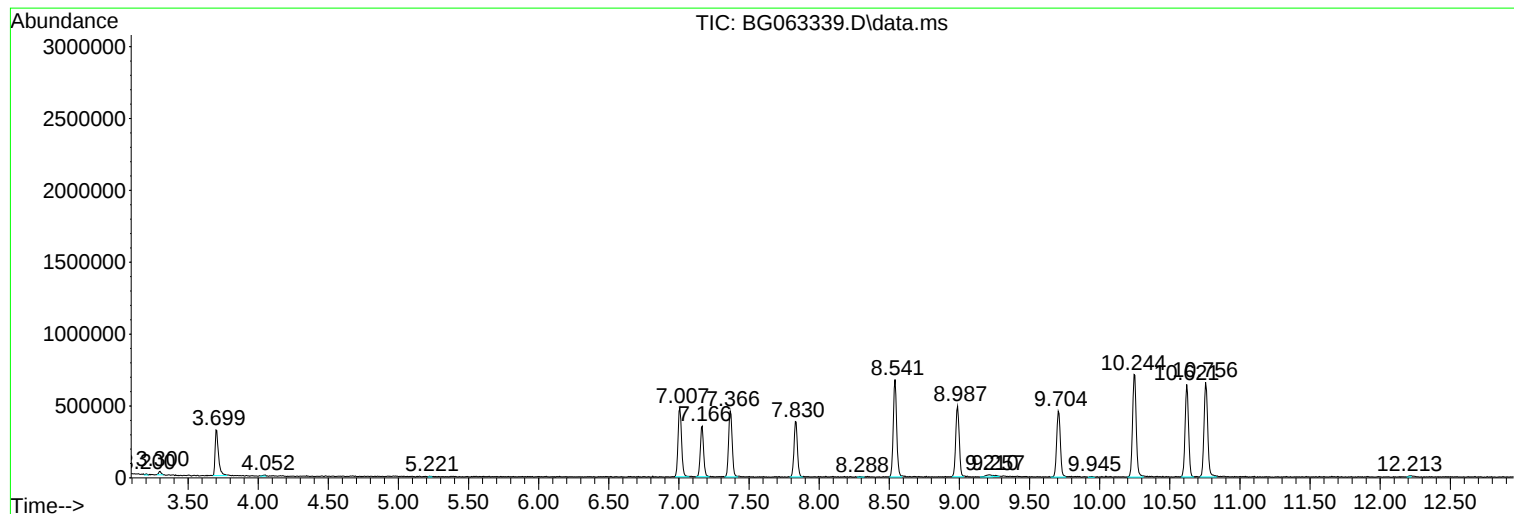

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111124\
Data File : BG063339.D
Acq On : 12 Nov 2024 00:22
Operator : RC/JU
Sample : PB164899BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK899

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111124\
Data File : BG063339.D
Acq On : 12 Nov 2024 00:22
Operator : RC/JU
Sample : PB164899BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK899

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc