

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111124\
 Data File : BG063344.D
 Acq On : 13 Nov 2024 3:31
 Operator : RC/JU
 Sample : P4801-14
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 GCPB5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG063344.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.294	32	35	41	rVB3	23348	34744	0.71%	0.082%
2	3.706	102	105	114	rBV	63186	114724	2.35%	0.270%
3	4.481	233	237	242	rBV4	8571	16122	0.33%	0.038%
4	4.540	242	247	254	rVB	142007	202884	4.15%	0.477%
5	5.492	406	409	410	rBV3	9764	10022	0.21%	0.024%
6	6.925	649	653	656	rBV2	6865	9048	0.19%	0.021%
7	7.008	659	667	675	rBV2	157824	292739	5.99%	0.689%
8	7.166	685	694	702	rBV	371255	630673	12.91%	1.484%
9	7.366	721	728	740	rVB	474109	785376	16.08%	1.847%
10	7.484	740	748	754	rBV8	11449	30614	0.63%	0.072%
11	7.636	770	774	777	rBV5	4964	6900	0.14%	0.016%
12	7.830	801	807	817	rVB	409334	678901	13.90%	1.597%
13	8.541	921	928	940	rBV	484133	811868	16.63%	1.910%
14	8.988	996	1004	1012	rBV	519334	929470	19.03%	2.186%
15	9.223	1041	1044	1049	rBV4	5591	6849	0.14%	0.016%
16	9.417	1071	1077	1083	rVB2	30954	48702	1.00%	0.115%
17	9.704	1119	1126	1136	rBV2	499909	898076	18.39%	2.113%
18	10.245	1210	1218	1231	rBV	770837	1392531	28.52%	3.276%
19	10.621	1275	1282	1290	rBV	633534	1114462	22.82%	2.622%
20	10.756	1298	1305	1316	rBV	537721	1007435	20.63%	2.370%
21	10.997	1343	1346	1351	rBV4	8050	11725	0.24%	0.028%
22	11.632	1451	1454	1456	rBV4	6391	6908	0.14%	0.016%
23	11.908	1497	1501	1506	rVB3	19575	33657	0.69%	0.079%
24	12.213	1549	1553	1559	rBV4	10758	21476	0.44%	0.051%
25	12.654	1624	1628	1630	rBV3	4350	7032	0.14%	0.017%
26	13.876	1829	1836	1845	rBV	1641282	2300166	47.10%	5.411%
27	14.164	1877	1885	1892	rBV2	1679013	2643347	54.13%	6.218%
28	14.469	1930	1937	1946	rBV	1205919	1823473	37.34%	4.289%
29	14.681	1967	1973	1986	rBV2	122919	261629	5.36%	0.615%
30	14.898	2005	2010	2017	rVV7	8930	18382	0.38%	0.043%
31	15.004	2021	2028	2030	rVB3	4169	6520	0.13%	0.015%
32	15.292	2075	2077	2079	rVB2	8563	7636	0.16%	0.018%
33	15.468	2099	2107	2116	rBV	2373337	3497761	71.63%	8.228%
34	15.592	2122	2128	2138	rBV	789860	1149226	23.53%	2.703%
35	15.703	2146	2147	2154	rVB6	13270	16495	0.34%	0.039%
36	16.038	2200	2204	2207	rVB4	8217	10470	0.21%	0.025%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111124\
 Data File : BG063344.D
 Acq On : 13 Nov 2024 3:31
 Operator : RC/JU
 Sample : P4801-14
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 GCPB5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
 Title : SVOA CALIBRATION

37	16.250	2236	2240	2245	rBV5	8962	10673	0.22%	0.025%
38	16.908	2351	2352	2359	rVB5	7664	11025	0.23%	0.026%
39	17.143	2389	2392	2394	rBV3	6040	9386	0.19%	0.022%
40	17.219	2397	2405	2415	rVV	1594753	2332444	47.76%	5.487%
41	17.319	2415	2422	2431	rBV	2699367	4062537	83.19%	9.556%
42	17.783	2497	2501	2503	rVB4	7446	10681	0.22%	0.025%
43	17.801	2503	2504	2507	rBV2	6151	6495	0.13%	0.015%
44	17.889	2515	2519	2525	rVB6	8710	16234	0.33%	0.038%
45	18.118	2553	2558	2565	rBV7	22384	50241	1.03%	0.118%
46	18.435	2610	2612	2615	rBV3	5875	7367	0.15%	0.017%
47	18.829	2677	2679	2680	rBV2	7776	6781	0.14%	0.016%
48	19.041	2713	2715	2723	rVB7	8345	15262	0.31%	0.036%
49	19.182	2735	2739	2746	rBV3	47519	66530	1.36%	0.156%
50	19.252	2748	2751	2754	rBV	35883	44316	0.91%	0.104%
51	19.281	2754	2756	2759	rVB3	12529	14101	0.29%	0.033%
52	19.405	2772	2777	2779	rBV6	12616	16064	0.33%	0.038%
53	19.616	2807	2813	2820	rBV	3366791	4883279	100.00%	11.487%
54	20.586	2976	2978	2979	rBV2	18040	13608	0.28%	0.032%
55	21.473	3123	3129	3143	rVB2	1664119	2637997	54.02%	6.205%
56	24.299	3600	3610	3622	rBV	1844460	4704210	96.33%	11.066%
57	24.505	3635	3645	3660	rVB	1046435	2754035	56.40%	6.478%




Sum of corrected areas: 42511309

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111124\
Data File : BG063344.D
Acq On : 13 Nov 2024 3:31
Operator : RC/JU
Sample : P4801-14
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
GCPB5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

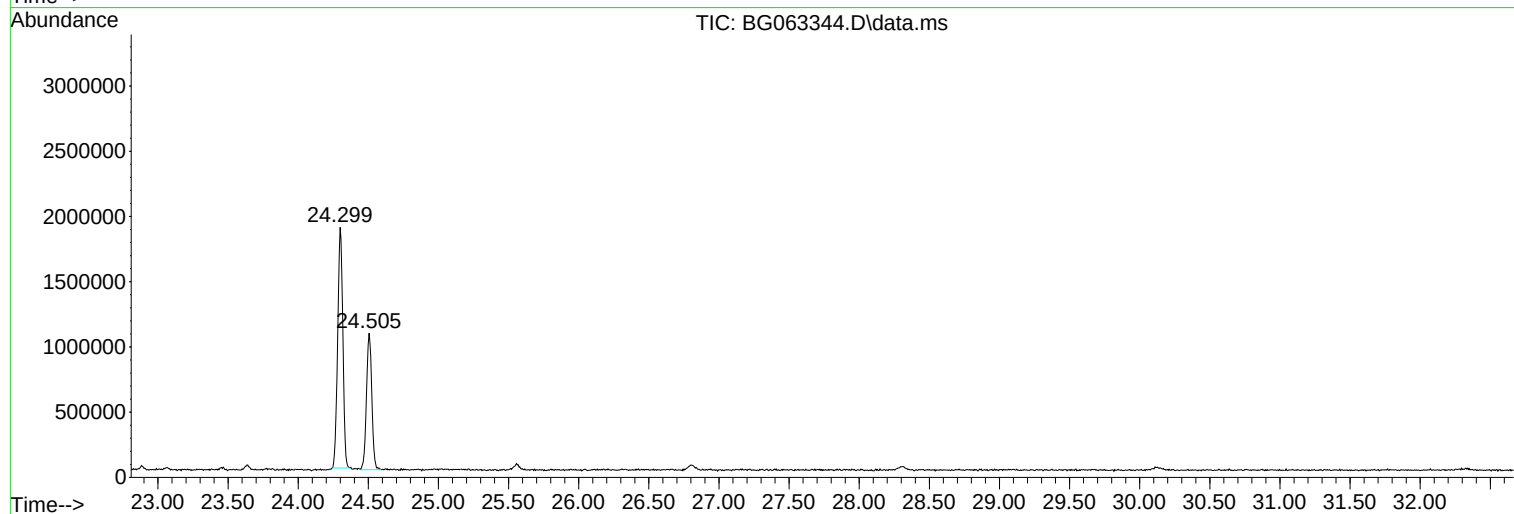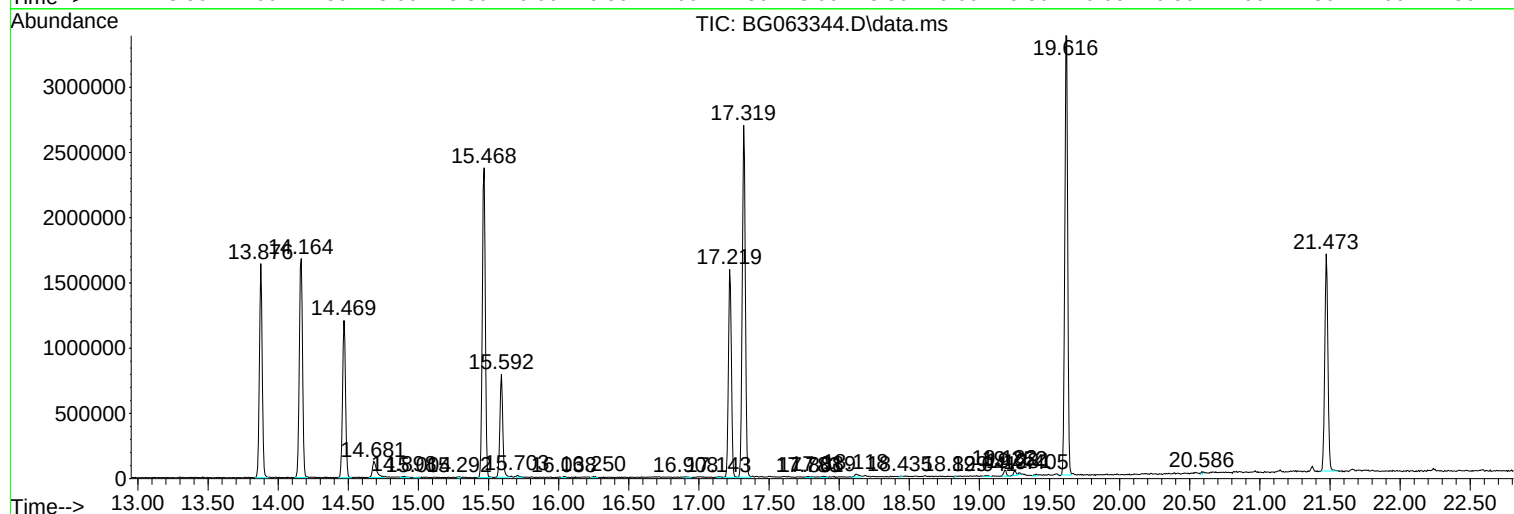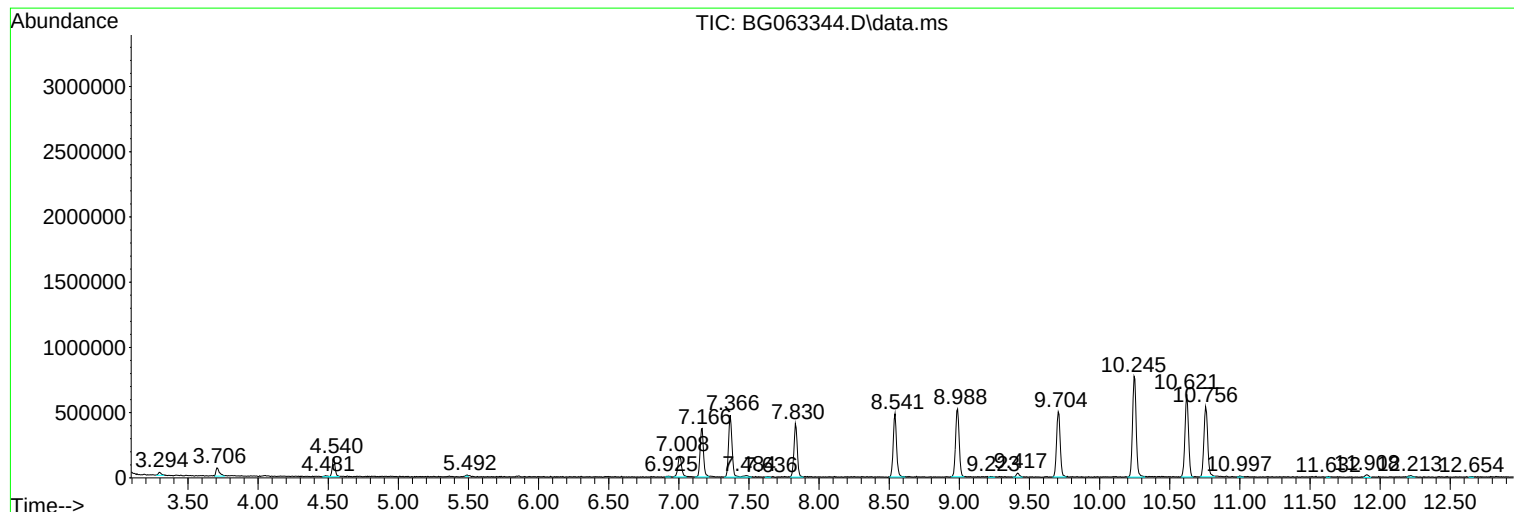

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111124\
Data File : BG063344.D
Acq On : 13 Nov 2024 3:31
Operator : RC/JU
Sample : P4801-14
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
GCPB5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111124\
Data File : BG063344.D
Acq On : 13 Nov 2024 3:31
Operator : RC/JU
Sample : P4801-14
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
GCPB5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc