

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG111215\
 Data File : BG019583.D
 Acq On : 12 Nov 2015 14:32
 Operator : UM/NP
 Sample : PB86584BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK84

Quant Time: Nov 13 10:15:00 2015
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG102815.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Nov 13 10:06:43 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.17	152	23829	20.00	ng/ul	0.00
18) Naphthalene-d8	11.00	136	102943	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.81	164	83845	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.54	188	245619	20.00	ng/ul	0.00
78) Chrysene-d12	21.83	240	300959	20.00	ng/ul	0.00
86) Perylene-d12	25.18	264	279401	20.00	ng/ul	-0.01

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.48	96	3755	7.55	ng/uL	0.00
5) Phenol-d5	7.31	99	73036	33.39	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.48	67	53052	38.26	ng/ul	0.00
9) 2-Chlorophenol-d4	7.70	132	46302	33.91	ng/ul	0.00
13) 4-Methylphenol-d8	8.88	113	60934	34.97	ng/ul	0.00
19) Nitrobenzene-d5	9.35	128	25200	33.31	ng/ul	0.00
22) 2-Nitrophenol-d4	10.07	143	30830	34.33	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.62	165	61624	31.63	ng/ul	0.00
29) 4-Chloroaniline-d4	11.13	131	80021	40.60	ng/ul	0.00
44) Dimethylphthalate-d6	14.20	166	256957	37.17	ng/ul	0.00
47) Acenaphthylene-d8	14.50	160	261092	34.10	ng/ul	0.00
52) 4-Nitrophenol-d4	14.99	143	35282	32.13	ng/ul	0.00
58) Fluorene-d10	15.79	176	219312	34.29	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.90	200	39366	24.76	ng/ul	0.00
71) Anthracene-d10	17.64	188	380661	34.00	ng/ul	0.00
79) Pyrene-d10	19.92	212	445215	33.80	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.95	264	499191	35.60	ng/ul	0.00


Target Compounds					Qvalue
15) N-Nitroso-di-n-propylamine	8.87	70	2063	1.08 ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG111215\
Data File : BG019583.D
Acq On : 12 Nov 2015 14:32
Operator : UM/NP
Sample : PB86584BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK84

Quant Time: Nov 13 10:15:00 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG102815.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Nov 13 10:06:43 2015
Response via : Initial Calibration

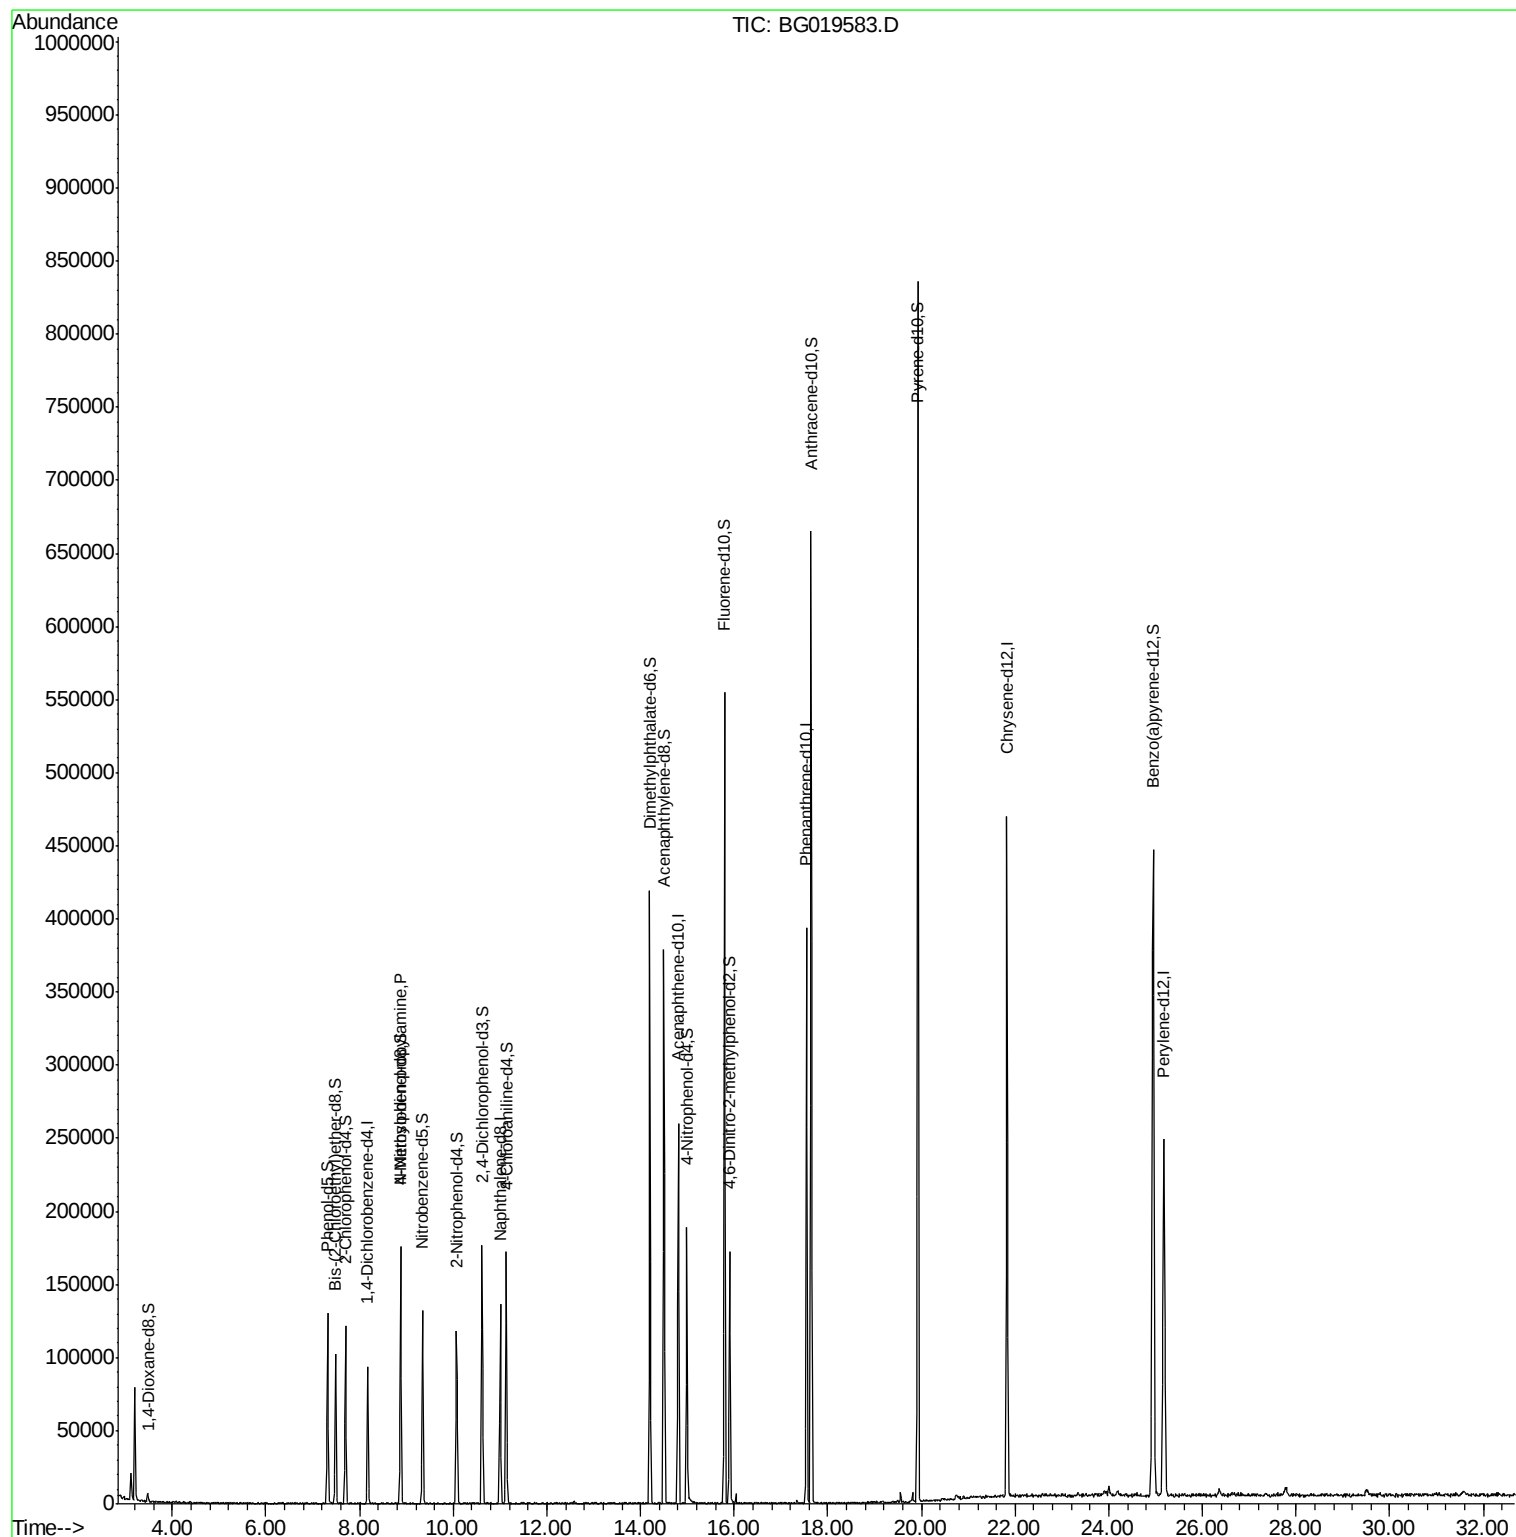

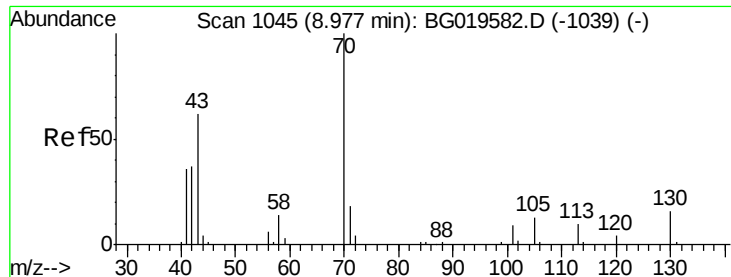

#15
 N-Nitroso-di-n-propylamine
 Concen: 1.08 ng/ul
 RT: 8.87 min Scan# 1027
 Delta R.T. -0.11 min
 Lab File: BG019583.D
 Acq: 12 Nov 2015 14:32

Instrument :
 BNA_G
 ClientSampleId :
 SBLK84

Tgt Ion:	70	Resp:	2063
Ion	Ratio	Lower	Upper
70	100		
42	238.8	36.6	55.0#
101	0.0	5.8	8.8#
130	0.0	14.6	22.0#

