

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG111315\
 Data File : BG019583.D
 Acq On : 13 Nov 2015 14:08
 Operator : UM/NP
 Sample : PB86633BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK01

Quant Time: Nov 14 00:07:50 2015
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG102815.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Nov 14 00:06:36 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.16	152	27981	20.00	ng/ul	0.00
18) Naphthalene-d8	10.99	136	115571	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.79	164	89175	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.54	188	258512	20.00	ng/ul	0.00
78) Chrysene-d12	21.81	240	342931	20.00	ng/ul	0.00
86) Perylene-d12	25.15	264	327732	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.46	96	3606	6.17	ng/uL	0.00
5) Phenol-d5	7.31	99	83722	32.59	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.47	67	61399	37.71	ng/ul	0.00
9) 2-Chlorophenol-d4	7.68	132	53376	33.29	ng/ul	0.00
13) 4-Methylphenol-d8	8.87	113	66459	32.48	ng/ul	0.00
19) Nitrobenzene-d5	9.34	128	28860	33.98	ng/ul	0.00
22) 2-Nitrophenol-d4	10.06	143	33545	33.27	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.60	165	63440	29.00	ng/ul	0.00
29) 4-Chloroaniline-d4	11.12	131	84275	38.08	ng/ul	0.00
44) Dimethylphthalate-d6	14.19	166	277821	37.79	ng/ul	0.00
47) Acenaphthylene-d8	14.49	160	276883	34.00	ng/ul	0.00
52) 4-Nitrophenol-d4	14.98	143	41398	35.44	ng/ul	0.00
58) Fluorene-d10	15.79	176	226042	33.23	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.89	200	49647	29.67	ng/ul	0.00
71) Anthracene-d10	17.64	188	409269	34.73	ng/ul	0.00
79) Pyrene-d10	19.91	212	530015	35.32	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.92	264	574872	34.95	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
15) N-Nitroso-di-n-propylamine	8.87	70	2292	1.02	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG111315\
Data File : BG019583.D
Acq On : 13 Nov 2015 14:08
Operator : UM/NP
Sample : PB86633BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK01

Quant Time: Nov 14 00:07:50 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG102815.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Nov 14 00:06:36 2015
Response via : Initial Calibration

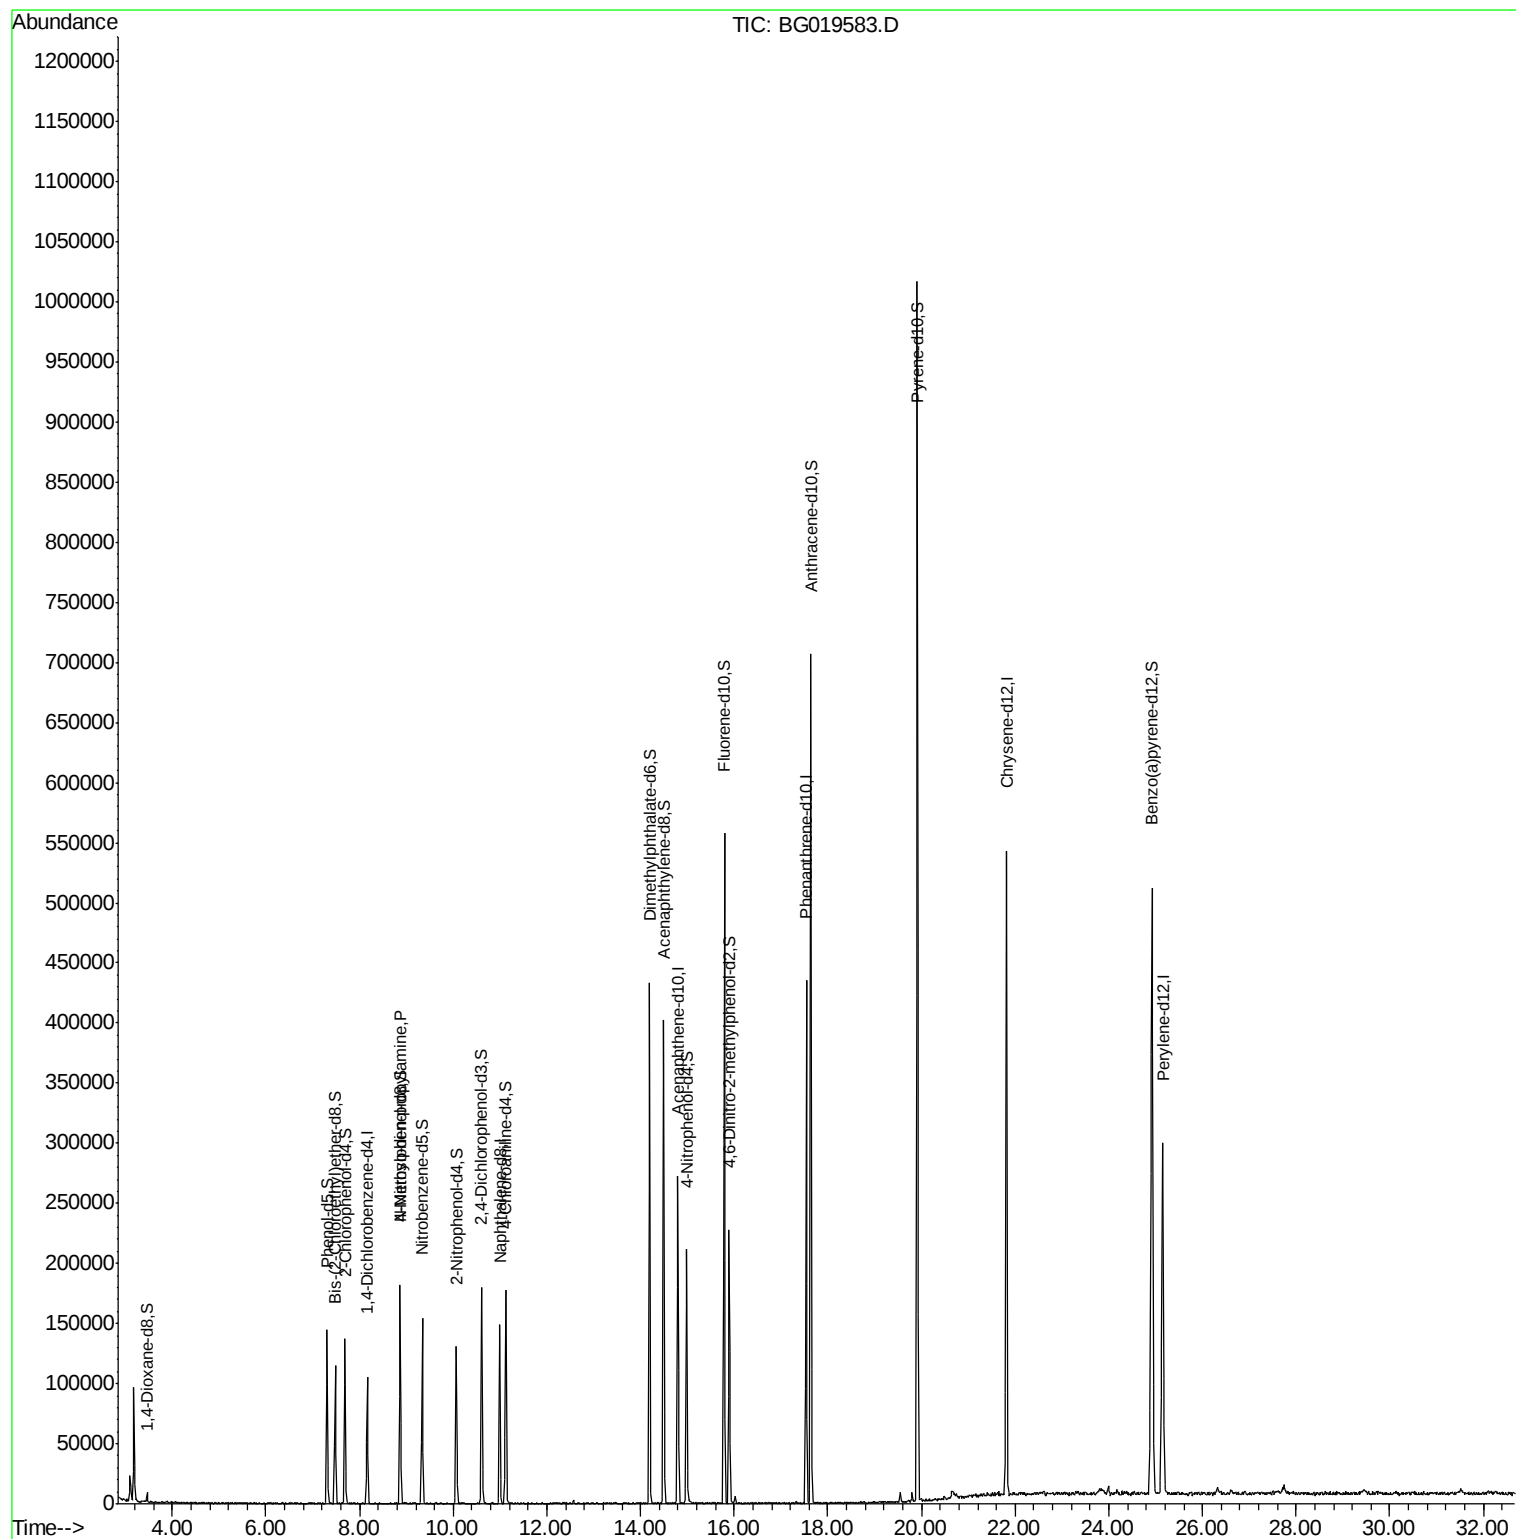

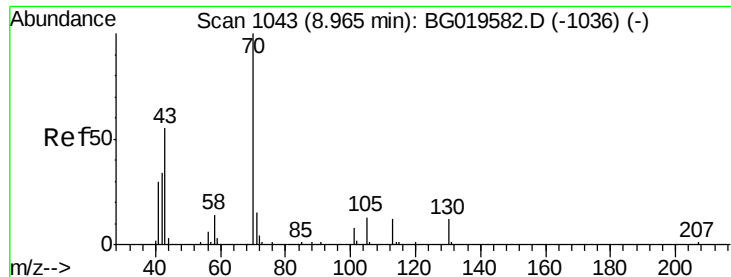

#15
 N-Nitroso-di-n-propylamine
 Concen: 1.02 ng/ul
 RT: 8.87 min Scan# 1026
 Delta R.T. -0.10 min
 Lab File: BG019583.D
 Acq: 13 Nov 2015 14:08

Instrument :
 BNA_G
 ClientSampleId :
 SBLK01

Tgt Ion: 70 Resp: 2292
 Ion Ratio Lower Upper
 70 100
 42 164.0 36.6 55.0#
 101 0.0 5.8 8.8#
 130 0.0 14.6 22.0#

