

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG111315\
 Data File : BG019589.D
 Acq On : 13 Nov 2015 18:23
 Operator : UM/NP
 Sample : G4342-10
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP22

Quant Time: Nov 14 00:36:37 2015
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG102815.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Nov 14 00:34:28 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.16	152	25030	20.00	ng/ul	0.00
18) Naphthalene-d8	10.99	136	98557	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.79	164	77913	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.53	188	223468	20.00	ng/ul	0.00
78) Chrysene-d12	21.81	240	295597	20.00	ng/ul	0.00
86) Perylene-d12	25.14	264	277246	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.46	96	1789	3.42	ng/uL	0.00
5) Phenol-d5	7.31	99	39002	16.97	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.47	67	28110	19.30	ng/ul	0.00
9) 2-Chlorophenol-d4	7.69	132	24032	16.75	ng/ul	0.00
13) 4-Methylphenol-d8	8.86	113	32974	18.02	ng/ul	0.00
19) Nitrobenzene-d5	9.33	128	13397	18.50	ng/ul	0.00
22) 2-Nitrophenol-d4	10.06	143	16301	18.96	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.60	165	30903	16.57	ng/ul	0.00
29) 4-Chloroaniline-d4	11.12	131	38424	20.36	ng/ul	0.00
44) Dimethylphthalate-d6	14.19	166	130822	20.36	ng/ul	0.00
47) Acenaphthylene-d8	14.49	160	129743	18.24	ng/ul	0.00
52) 4-Nitrophenol-d4	14.98	143	20800	20.38	ng/ul	0.00
58) Fluorene-d10	15.78	176	108780	18.30	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.89	200	23908	16.53	ng/ul	0.00
71) Anthracene-d10	17.63	188	205410	20.16	ng/ul	0.00
79) Pyrene-d10	19.90	212	259338	20.05	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.91	264	287590	20.67	ng/ul	0.00


Target Compounds						Qvalue
45) Dimethylphthalate	14.23	163	70150	10.68	ng/ul#	97
84) Bis(2-ethylhexyl)phthalate	21.67	149	15789	2.06	ng/ul#	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG111315\
Data File : BG019589.D
Acq On : 13 Nov 2015 18:23
Operator : UM/NP
Sample : G4342-10
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP22

Quant Time: Nov 14 00:36:37 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG102815.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Nov 14 00:34:28 2015
Response via : Initial Calibration




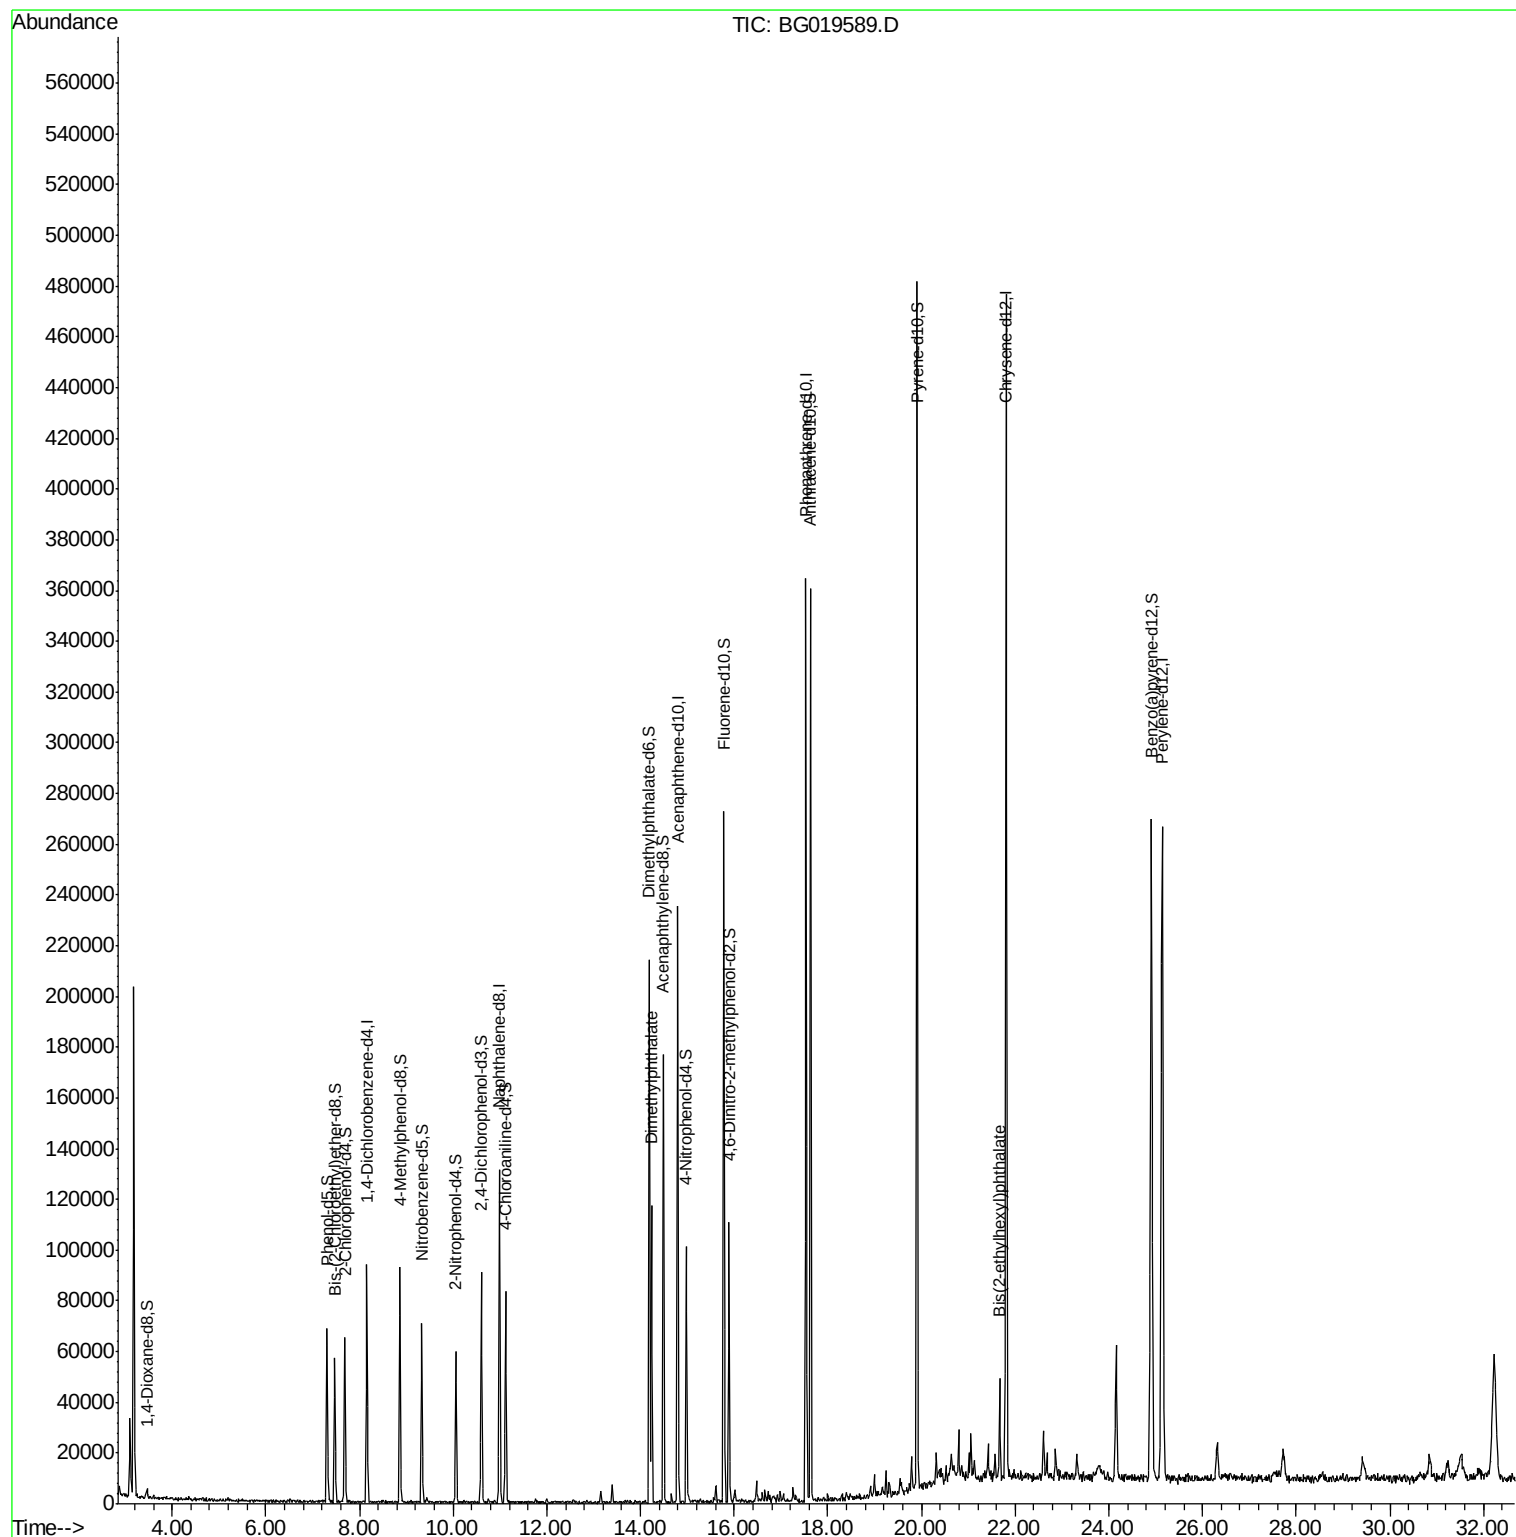


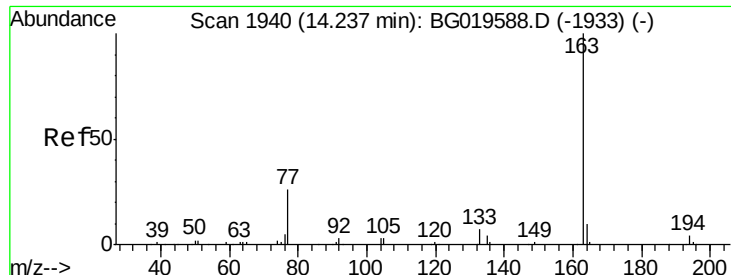

#45
 Dimethylphthalate
 Concen: 10.68 ng/ul
 RT: 14.23 min Scan# 1939
 Delta R.T. -0.00 min
 Lab File: BG019589.D
 Acq: 13 Nov 2015 18:23

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP22

Tgt Ion:163 Resp: 70150
 Ion Ratio Lower Upper
 163 100
 194 3.9 4.3 6.5#
 164 10.2 7.5 11.3

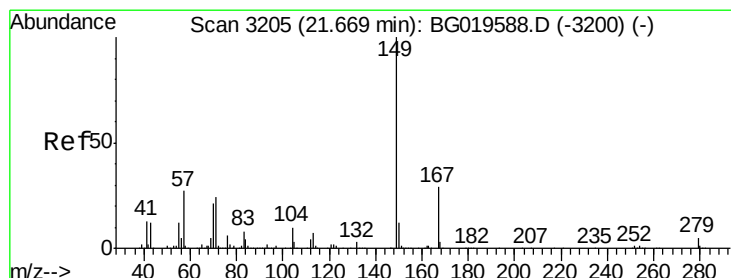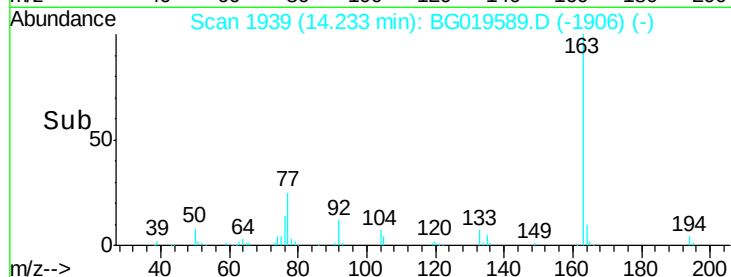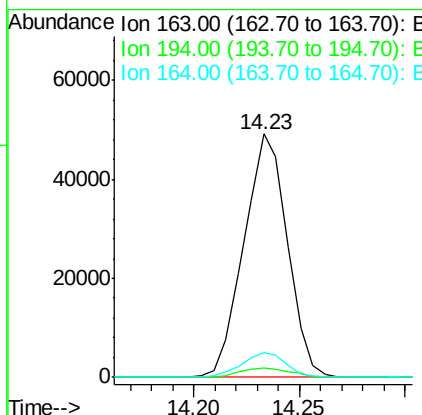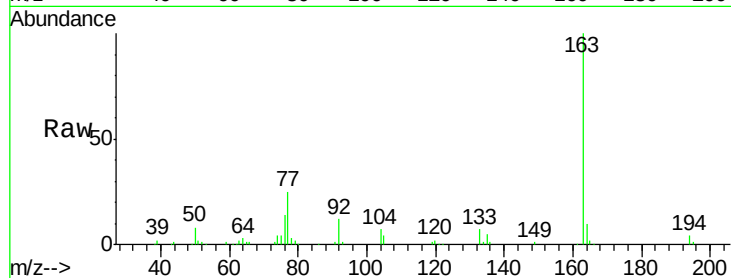

#84
 Bis(2-ethylhexyl)phthalate
 Concen: 2.06 ng/ul
 RT: 21.67 min Scan# 3205
 Delta R.T. 0.00 min
 Lab File: BG019589.D
 Acq: 13 Nov 2015 18:23

Tgt Ion:149 Resp: 15789
 Ion Ratio Lower Upper
 149 100
 167 25.2 23.2 34.8
 279 3.9 5.0 7.4#

