

Data Path : Z:\HPCHEM1\BNA G\DATA\BG111315\
 Data File : BG019595.D
 Acq On : 13 Nov 2015 17:06
 Operator : UM/NP
 Sample : G4342-08MSD
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 D9KP7MSD

Manual Integrations
 APPROVED

mmdadoda
 11/16/2015 3:26:08 PM

Quant Time: Nov 14 00:29:36 2015
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG102815.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Nov 14 00:06:36 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.16	152	23785	20.00	ng/ul	0.00
18) Naphthalene-d8	10.99	136	96999	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.79	164	75058	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.53	188	221846	20.00	ng/ul	0.00
78) Chrysene-d12	21.80	240	290382	20.00	ng/ul	-0.01
86) Perylene-d12	25.14	264	275231	20.00	ng/ul	-0.02

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.46	96	2626	5.29	ng/uL	0.00
5) Phenol-d5	7.30	99	55190	25.28	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.47	67	37597	27.16	ng/ul	0.00
9) 2-Chlorophenol-d4	7.69	132	33982	24.93	ng/ul	0.00
13) 4-Methylphenol-d8	8.87	113	44709	25.71	ng/ul	0.00
19) Nitrobenzene-d5	9.34	128	18600	26.09	ng/ul	0.00
22) 2-Nitrophenol-d4	10.06	143	21941	25.93	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.61	165	41311	22.50	ng/ul	0.00
29) 4-Chloroaniline-d4	11.12	131	50608	27.25	ng/ul	0.00
44) Dimethylphthalate-d6	14.19	166	186991	30.22	ng/ul	0.00
47) Acenaphthylene-d8	14.49	160	176474	25.75	ng/ul	0.00
52) 4-Nitrophenol-d4	14.98	143	28898	29.39	ng/ul	0.00
58) Fluorene-d10	15.78	176	146933	25.66	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.89	200	35529	24.74	ng/ul	0.00
71) Anthracene-d10	17.63	188	277422	27.43	ng/ul	0.00
79) Pyrene-d10	19.91	212	348415	27.42	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.91	264	380261	27.53	ng/ul	-0.02

Target Compounds

						Ovalue
6) Phenol	7.33	94	66968	28.79	ng/ul	90
10) 2-Chlorophenol	7.72	128	37722	26.89	ng/ul	98
15) N-Nitroso-di-n-propylamine	8.97	70	56866	29.72	ng/ul#	86
33) 4-Chloro-3-methylphenol	12.25	107	69101	29.34	ng/ul	94
45) Dimethylphthalate	14.24	163	86560	13.68	ng/ul	97
50) Acenaphthene	14.86	153	132795	28.01	ng/ul	94
53) 4-Nitrophenol	14.99	109	40094m	26.15	ng/ul	
55) 2,4-Dinitrotoluene	15.15	165	57790	28.56	ng/ul#	78
69) Pentachlorophenol	17.18	266	44181	26.75	ng/ul	97
80) Pyrene	19.94	202	478194	29.35	ng/ul#	90
84) Bis(2-ethylhexyl)phthalate	21.67	149	11940	1.59	ng/ul#	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA G\DATA\BG111315\
Data File : BG019595.D
Acq On : 13 Nov 2015 17:06
Operator : UM/NP
Sample : G4342-08MSD
Misc :
ALS Vial : 7 Sample Multiplier: 1


Instrument :
BNA_G
ClientSampleId :
D9KP7MSD

Manual Integrations
APPROVED

mmdadoda
11/16/2015 3:26:08 PM

Quant Time: Nov 14 00:29:36 2015
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG102815.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Nov 14 00:06:36 2015
Response via : Initial Calibration

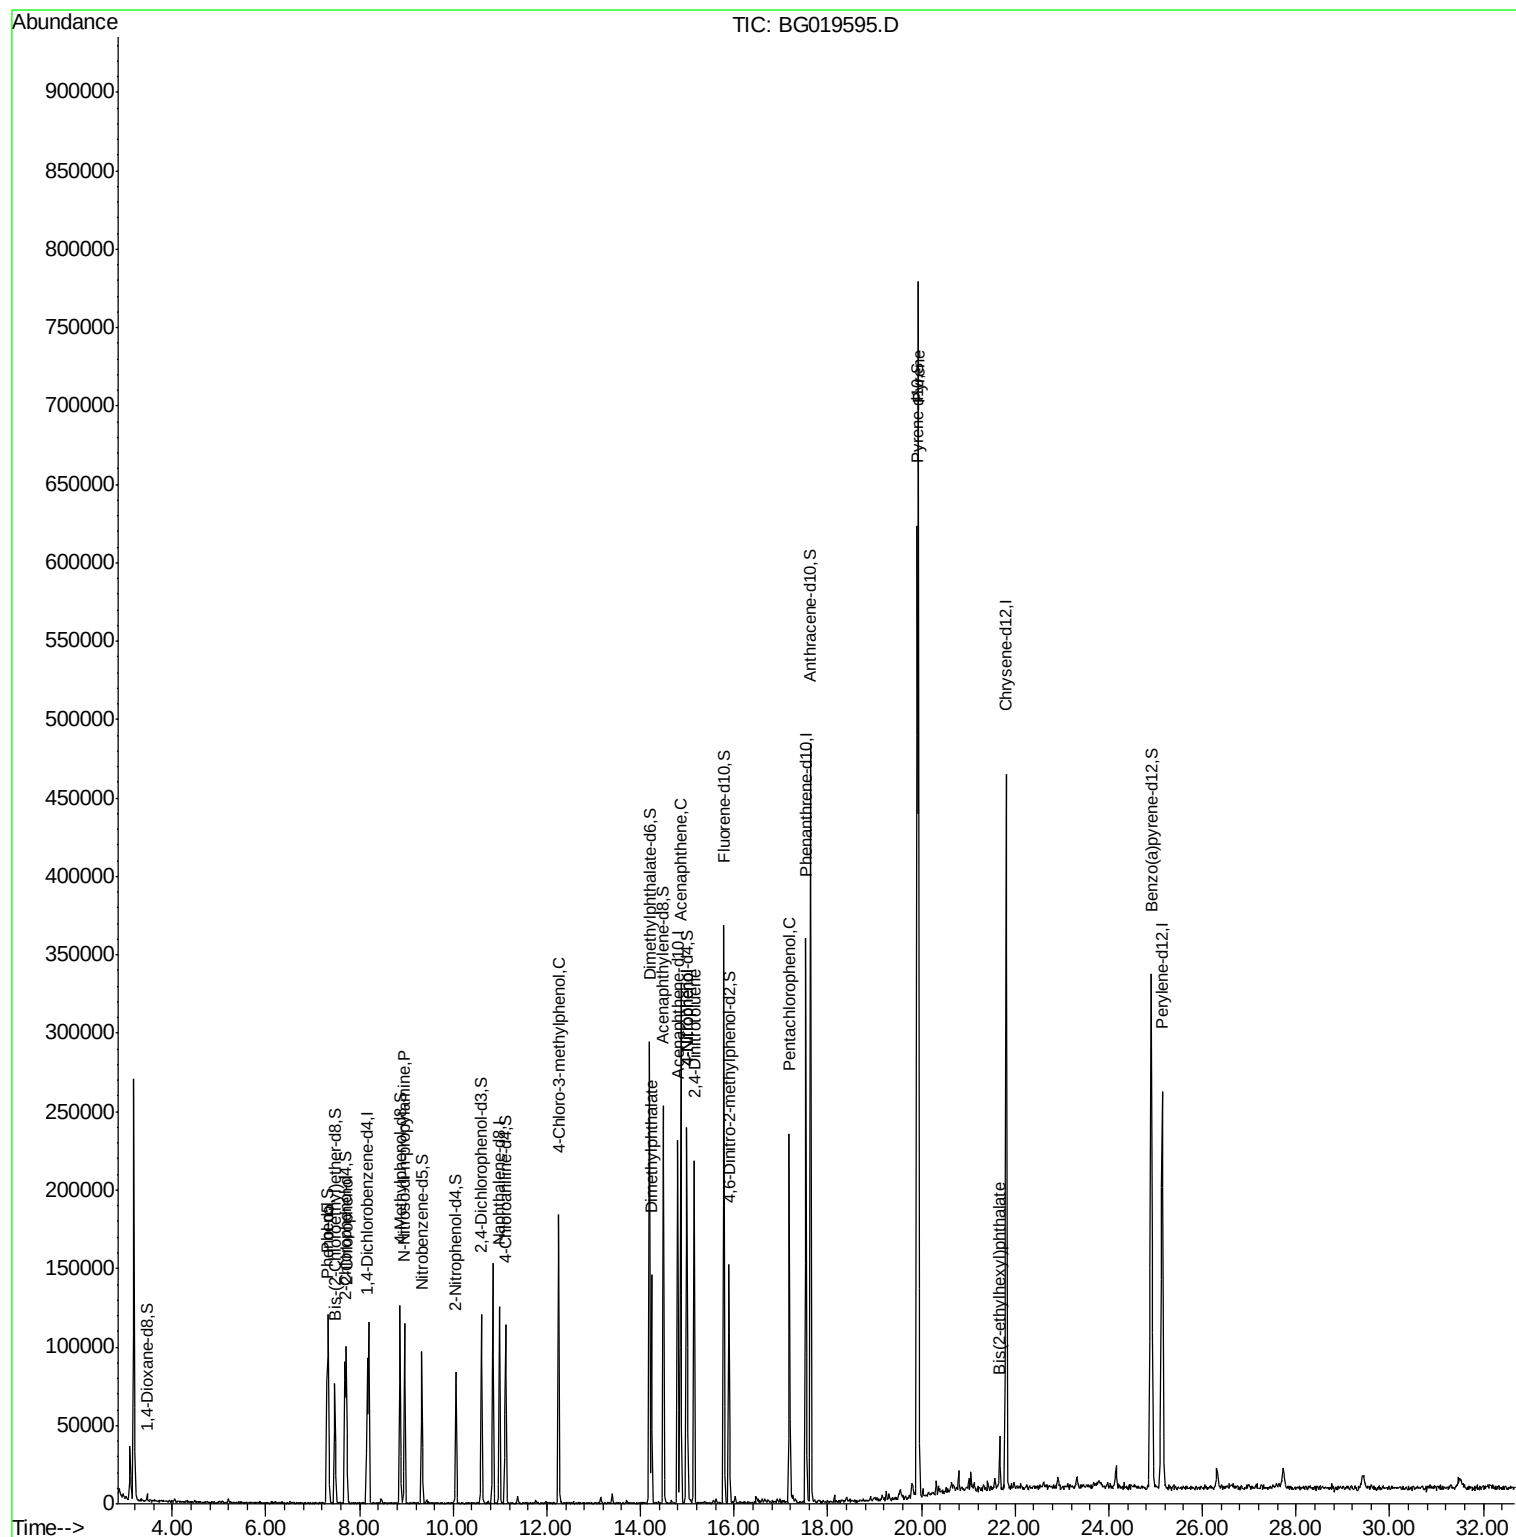

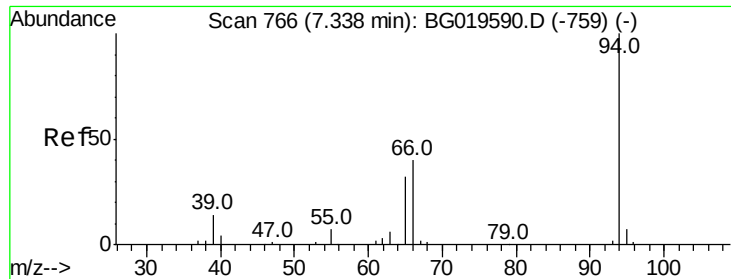

#6

Phenol

Concen: 28.79 ng/ul

RT: 7.33 min Scan# 765

Delta R.T. -0.00 min

Lab File: BG019595.D

Acq: 13 Nov 2015 17:06

Instrument :

BNA_G





ClientSampleId :

D9KP7MSD

Tot Ion:	94	Resp:	66968
Ion	Ratio	Lower	Upper
94	100		
65	33.5	29.3	43.9
66	47.2	45.0	67.6

Manual Integrations
APPROVED

mmdadoda
11/16/2015 3:26:08 PM

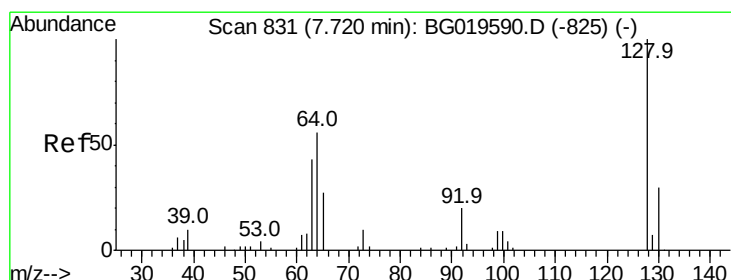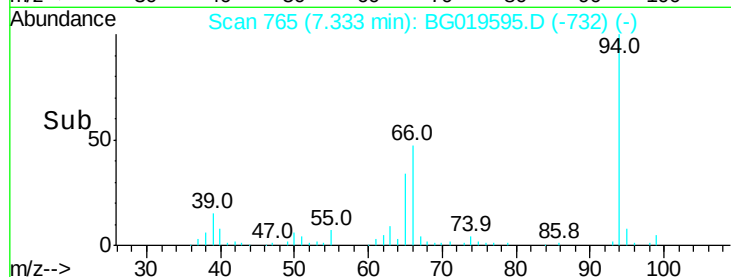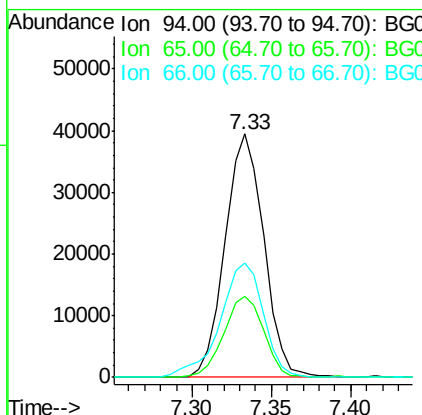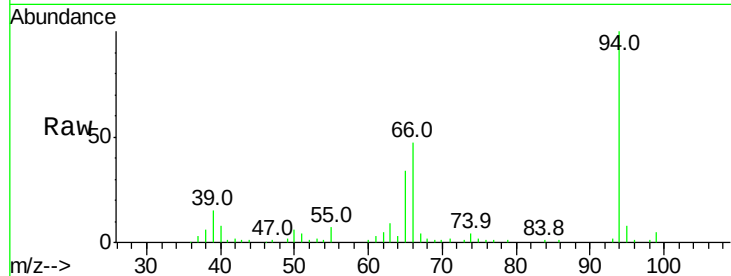

#10

2-Chlorophenol

Concen: 26.89 ng/ul




RT: 7.72 min Scan# 830


Delta R.T. -0.00 min

Lab File: BG019595.D

Acq: 13 Nov 2015 17:06

Tgt Ion:	128	Resp:	37722
Ion	Ratio	Lower	Upper
128	100		
64	64.6	53.2	79.8
130	32.3	25.9	38.9

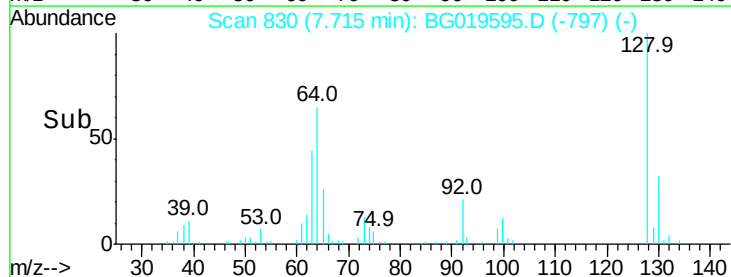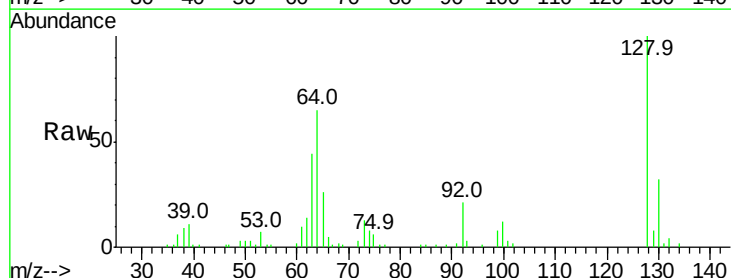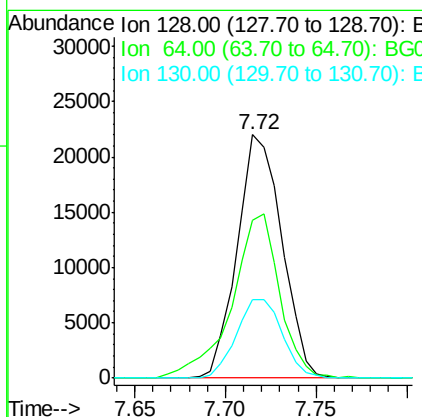

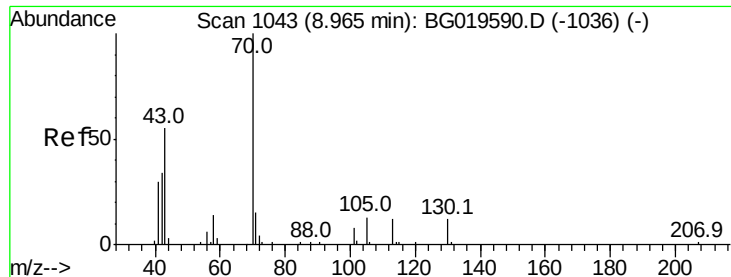

#15

N-Nitroso-di-n-propylamine

Concen: 29.72 ng/ul

RT: 8.97 min Scan# 1043

Delta R.T. 0.00 min

Lab File: BG019595.D

Acq: 13 Nov 2015 17:06

Instrument :

BNA_G

ClientSampleId :

D9KP7MSD

Tot Ion: 70 Resp: 56866

Ion Ratio Lower Upper

70 100


42 34.8 36.6 55.0#

101 8.3 5.8 8.8

130 13.5 14.6 22.0#

Manual Integrations
APPROVED

mmdadoda
11/16/2015 3:26:08 PM

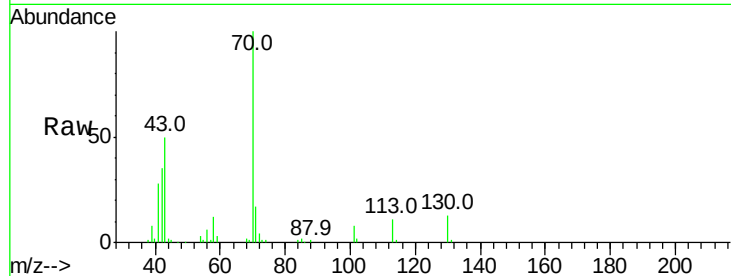




Abundance Ion 70.00 (69.70 to 70.70): BG019595.D (-1036) (-)

Ion 42.00 (41.70 to 42.70): BG019595.D (-1036) (-)

Ion 101.00 (100.70 to 101.70): BG019595.D (-1036) (-)

Ion 130.00 (129.70 to 130.70): BG019595.D (-1036) (-)

Time-->

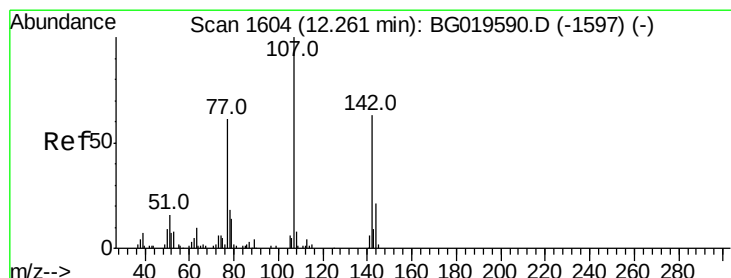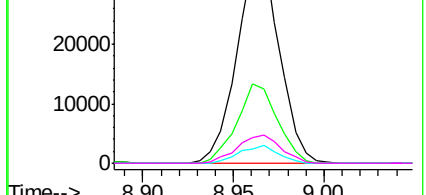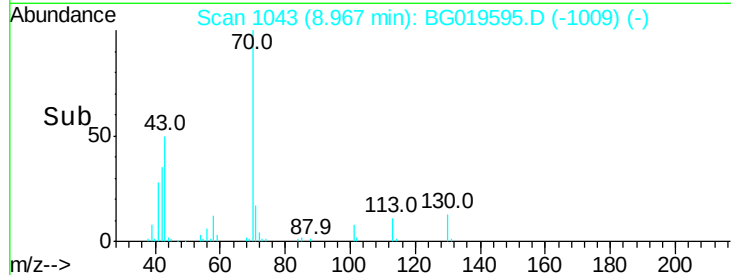

#33

4-Chloro-3-methylphenol

Concen: 29.34 ng/ul

RT: 12.25 min Scan# 1602

Delta R.T. -0.01 min

Lab File: BG019595.D

Acq: 13 Nov 2015 17:06


Tgt Ion: 107 Resp: 69101

Ion Ratio Lower Upper

107 100

144 19.1 13.0 19.6

142 54.8 47.0 70.6


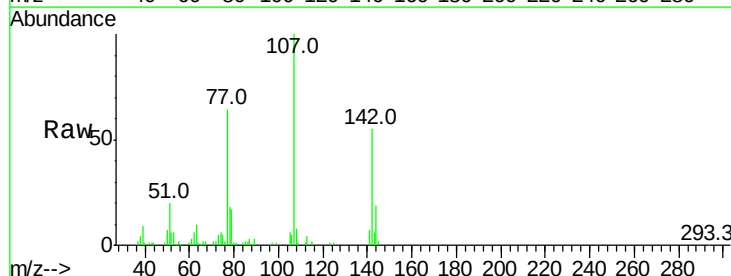



Abundance Ion 107.00 (106.70 to 107.70): BG019595.D (-1570) (-)

Ion 144.00 (143.70 to 144.70): BG019595.D (-1570) (-)

Ion 142.00 (141.70 to 142.70): BG019595.D (-1570) (-)

Time-->

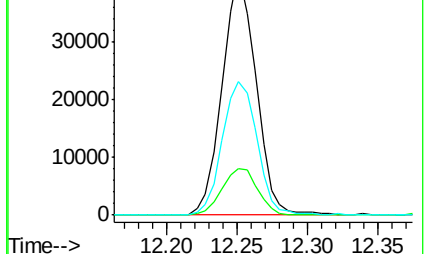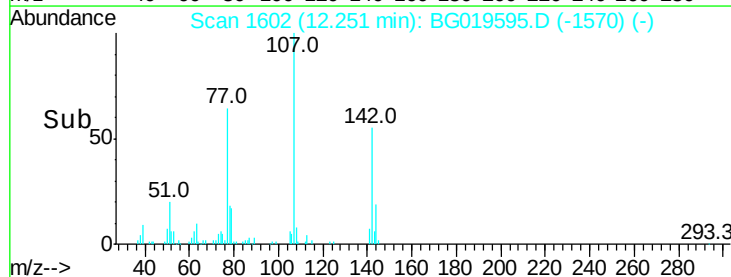

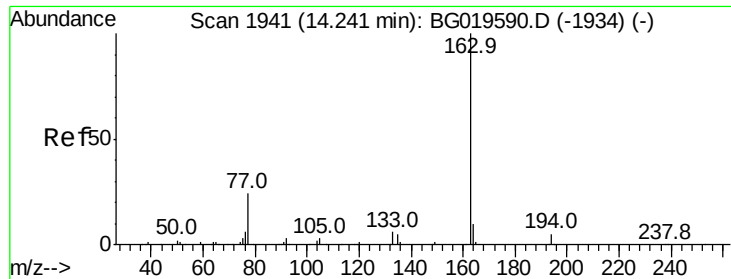


#45
Dimethylphthalate
Concen: 13.68 ng/ul
RT: 14.24 min Scan# 1940
Delta R.T. -0.00 min
Lab File: BG019595.D
Acq: 13 Nov 2015 17:06

Instrument :
BNA_G
ClientSampleId :
D9KP7MSD

Tot Ion	Ratio	Lower	Upper
163	100		
194	4.9	4.3	6.5
164	10.9	7.5	11.3

Manual Integrations
APPROVED

mmdadoda
11/16/2015 3:26:08 PM



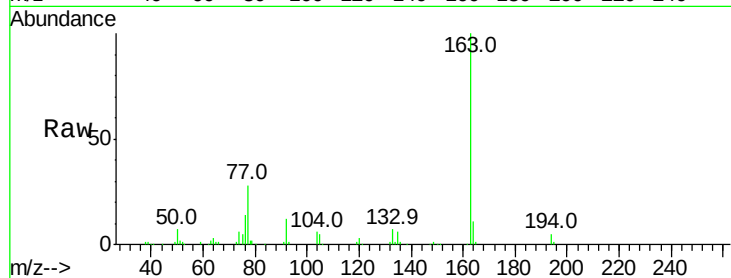


Abundance

Ion 163.00 (162.70 to 163.70): E


Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

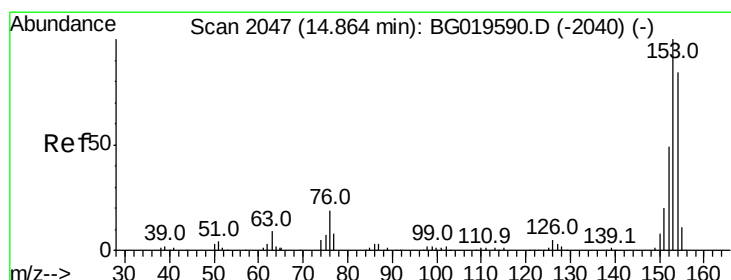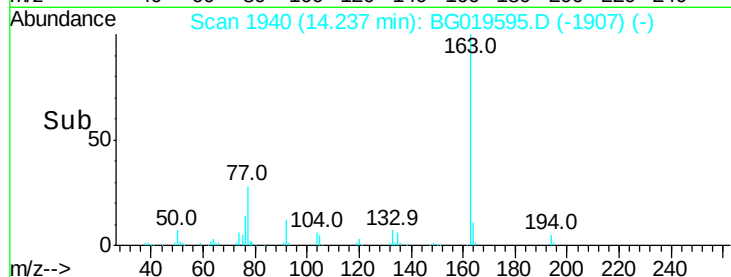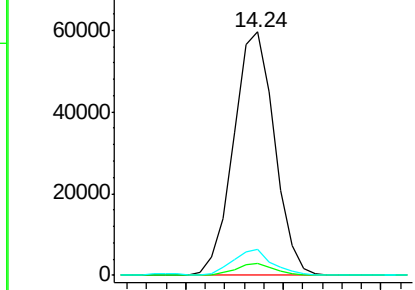

#50
Acenaphthene
Concen: 28.01 ng/ul
RT: 14.86 min Scan# 2046
Delta R.T. -0.00 min
Lab File: BG019595.D
Acq: 13 Nov 2015 17:06

Tgt Ion	Ratio	Lower	Upper
153	100		
152	45.2	38.8	58.2
154	82.7	71.5	107.3


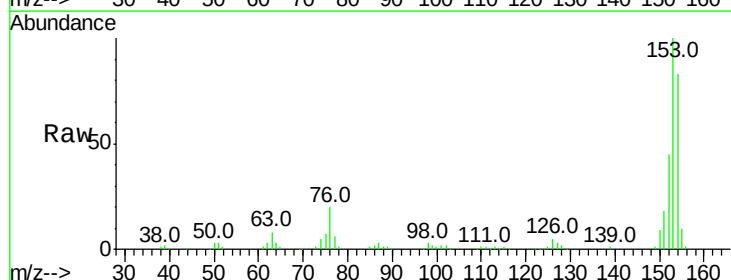



Abundance

Ion 153.00 (152.70 to 153.70): E

Ion 152.00 (151.70 to 152.70): E

Ion 154.00 (153.70 to 154.70): E

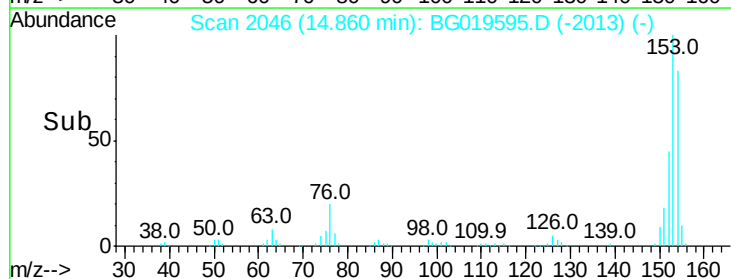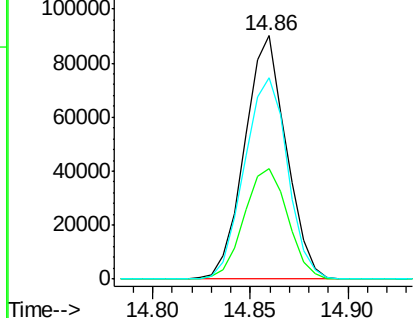

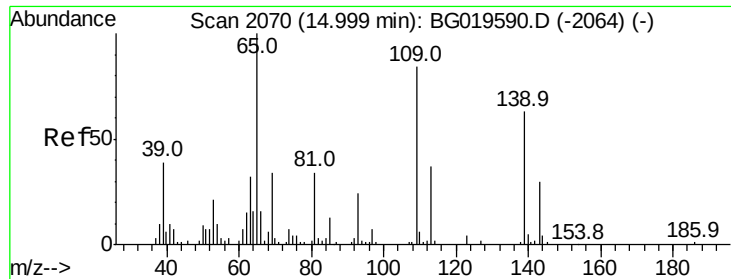





#53
4-Nitrophenol
Concen: 26.15 ng/ul m
RT: 14.99 min Scan# 2069
Delta R.T. -0.00 min
Lab File: BG019595.D
Acq: 13 Nov 2015 17:06

Instrument :
BNA_G
ClientSampleId :
D9KP7MSD

Tot Ion	Ratio	Resp	Lower	Upper
109	100			
139	78.3	41.5	62.3#	
65	113.4	73.7	110.5#	




Manual Integrations
APPROVED


mmdadoda
11/16/2015 3:26:08 PM

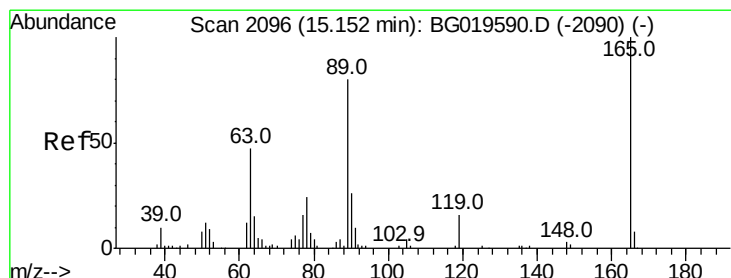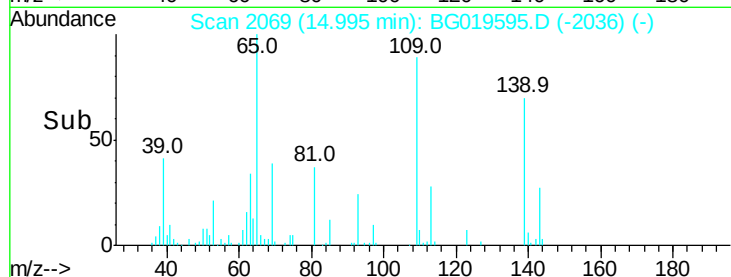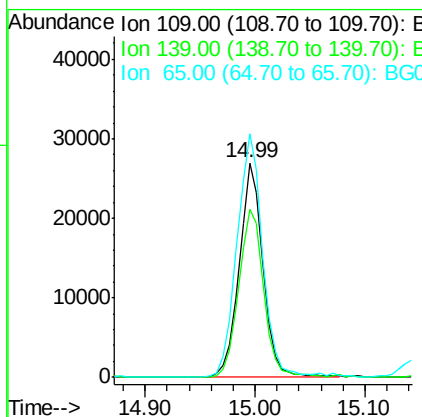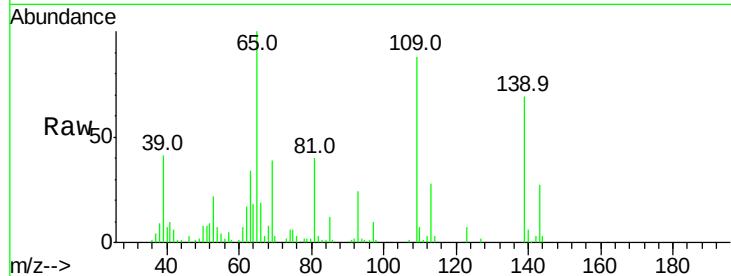

#55
2,4-Dinitrotoluene
Concen: 28.56 ng/ul
RT: 15.15 min Scan# 2095
Delta R.T. -0.00 min
Lab File: BG019595.D
Acq: 13 Nov 2015 17:06

Tgt Ion	Ratio	Resp	Lower	Upper
165	100			
63	45.7	51.1	76.7#	
182	2.7	3.3	4.9#	

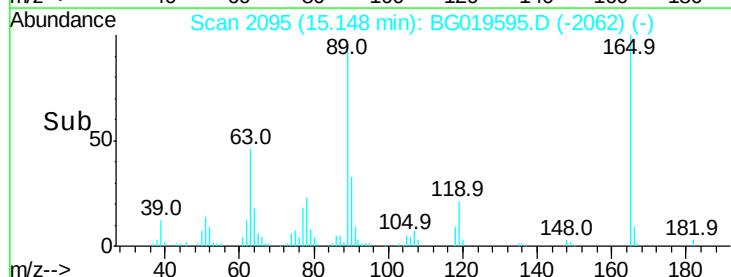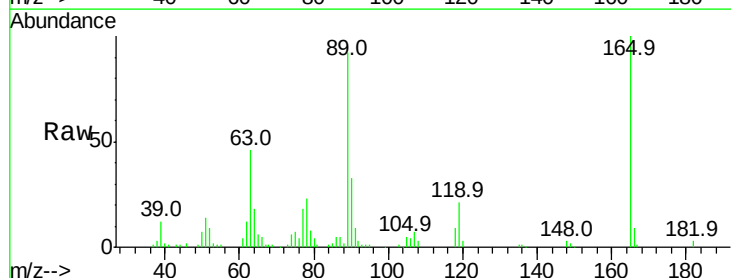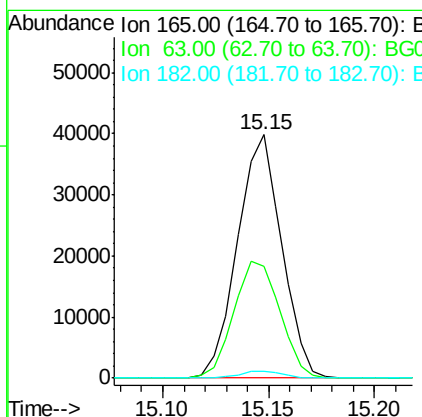

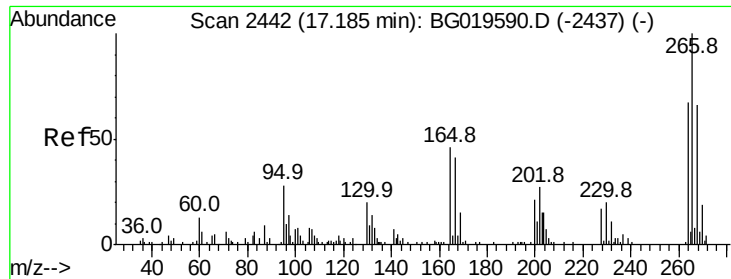





#69
 Pentachlorophenol
 Concen: 26.75 ng/ul
 RT: 17.18 min Scan# 2441
 Delta R.T. -0.00 min
 Lab File: BG019595.D
 Acq: 13 Nov 2015 17:06

Instrument :
 BNA_G
 ClientSampleId :
 D9KP7MSD

Tot Ion	Ratio	Resp	Lower	Upper
266	100	44181		
264	62.2	49.5	74.3	
268	64.7	48.7	73.1	




Manual Integrations
 APPROVED


mmdadoda
 11/16/2015 3:26:08 PM

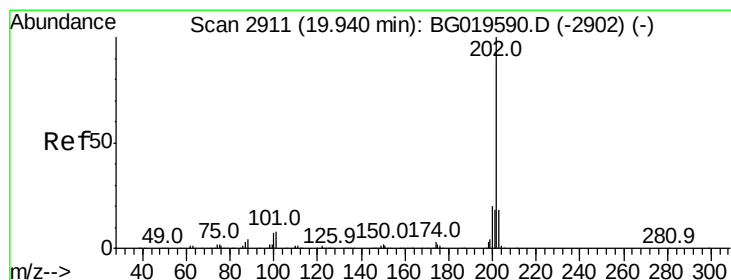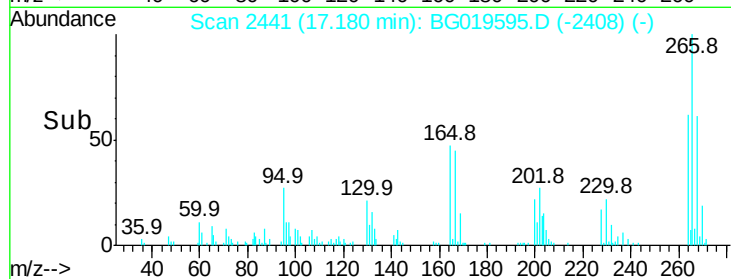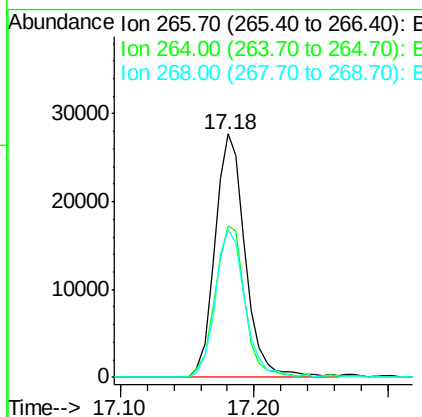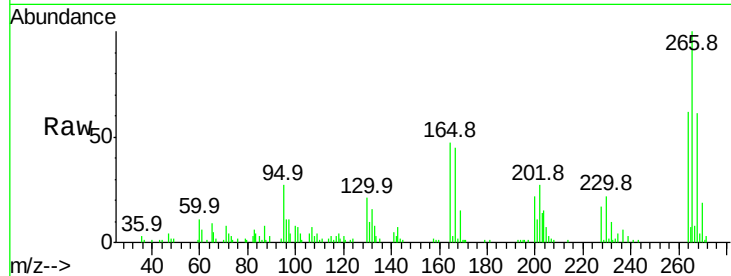

#80
 Pyrene
 Concen: 29.35 ng/ul
 RT: 19.94 min Scan# 2910
 Delta R.T. -0.00 min
 Lab File: BG019595.D
 Acq: 13 Nov 2015 17:06

Tgt Ion	Ratio	Resp	Lower	Upper
202	100	478194		
101	8.4	4.3	6.5#	
100	7.9	3.6	5.4#	

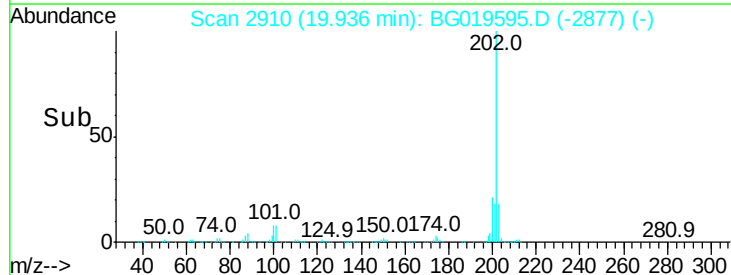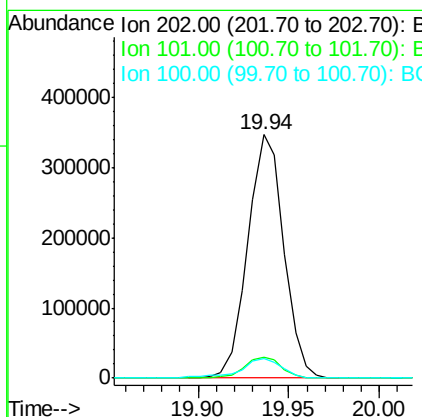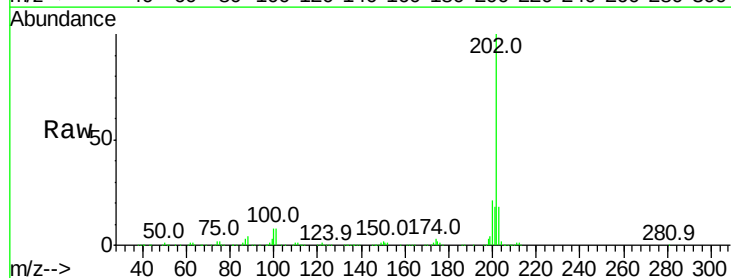

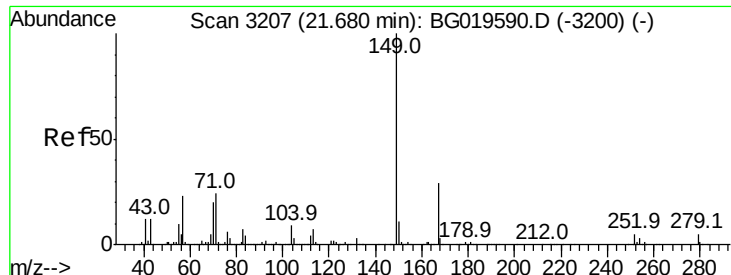

#84

Bis(2-ethylhexyl)phthalate

Concen: 1.59 ng/ul

RT: 21.67 min Scan# 3205

Delta R.T. -0.01 min

Lab File: BG019595.D


Acq: 13 Nov 2015 17:06

Instrument :

BNA_G

ClientSampleId :

D9KP7MSD

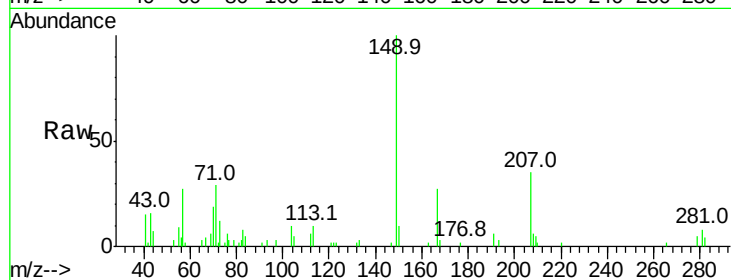

Tot Ion:	149	Resp:	11940
Ion Ratio	Lower	Upper	
149	100		
167	27.2	23.2	34.8
279	4.9	5.0	7.4#

Manual Integrations
APPROVED

mmdadoda
11/16/2015 3:26:08 PM

