


Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA G\DATA\BG111317\
 Data File : BG030987.D
 Acq On : 13 Nov 2017 23:54
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG111017.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Nov 10 15:38:25 2017

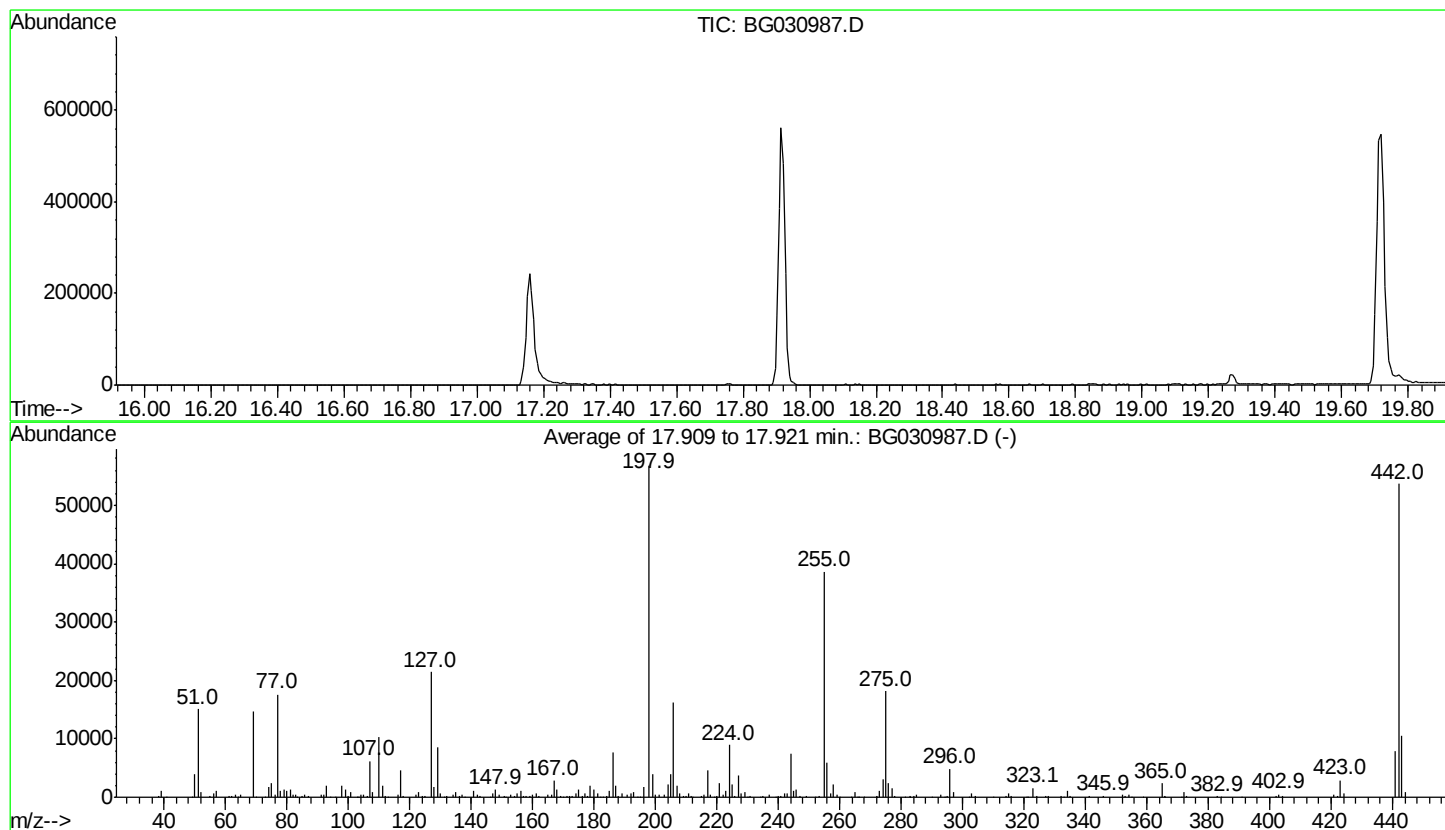

AutoFind: Scans 2488, 2489, 2490; Background Corrected with Scan 2482

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	26.5	15067	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	25.8	14630	PASS
70	69	0.00	2	0.4	55	PASS
127	198	10	80	37.7	21416	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	56776	PASS
199	198	5	9	6.9	3936	PASS
275	198	10	60	31.9	18127	PASS
365	198	1	100	4.1	2336	PASS
441	442	0.01	24	14.8	7933	PASS
442	198	50	100	94.5	53677	PASS
443	442	15	24	19.5	10487	PASS