
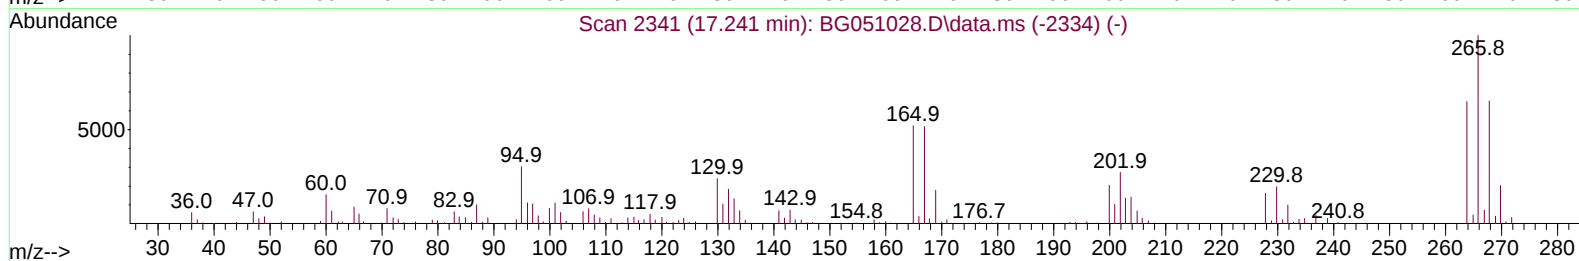
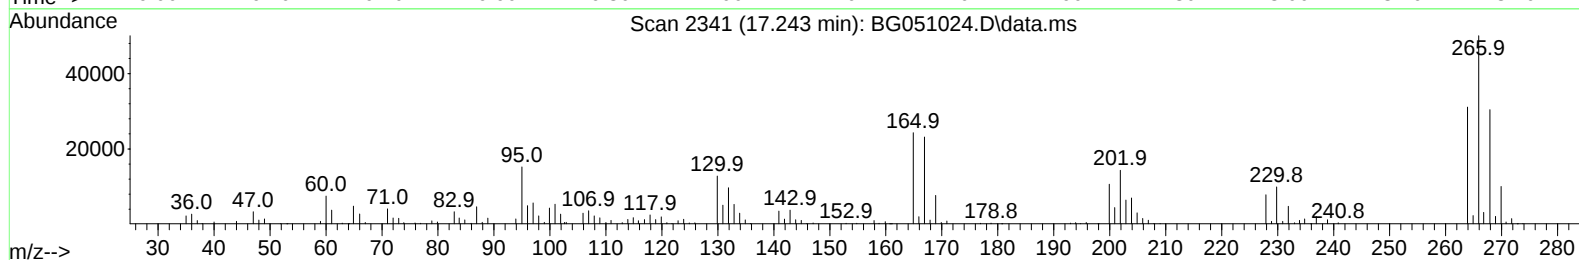


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111321\
Data File : BG051024.D
Acq On : 13 Nov 2021 15:21
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 15 08:12:04 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 15 03:55:35 2021
Response via : Initial Calibration

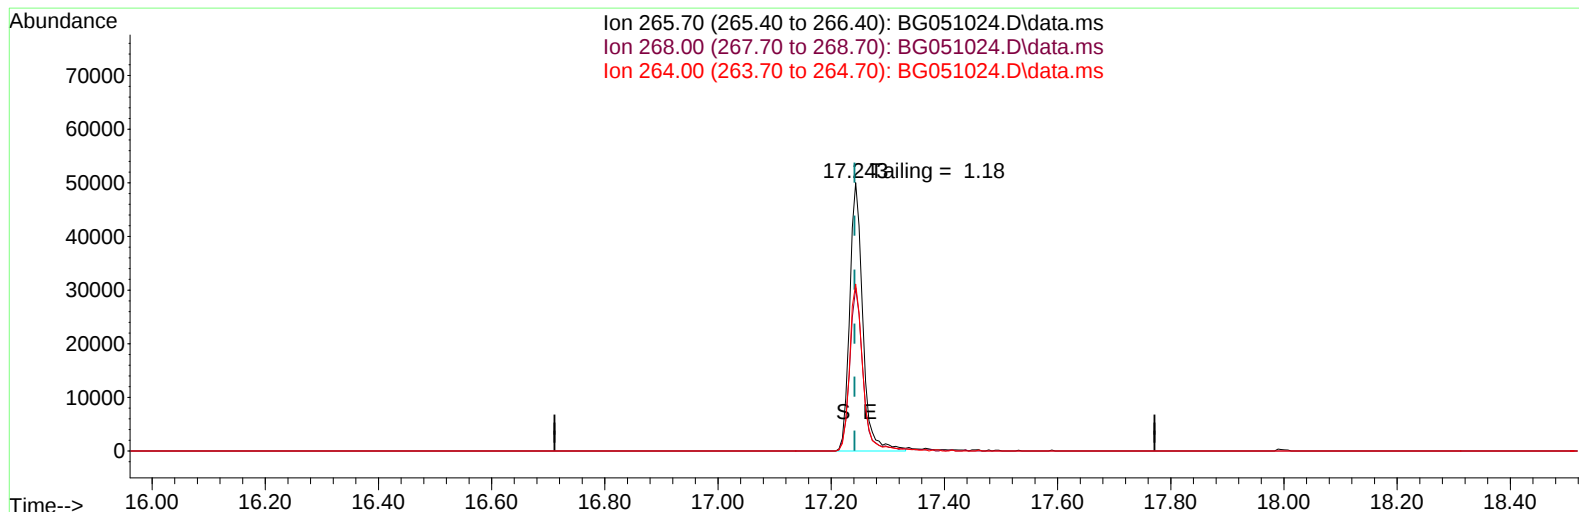

TIC: BG051024.D\data.ms

(70) Pentachlorophenol (C)




17.243min (+ 0.002) 29156.99 ng

response 81547

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.20	60.78
264.00	61.30	62.16
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111321\
Data File : BG051024.D
Acq On : 13 Nov 2021 15:21
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 15 08:12:04 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 15 03:55:35 2021
Response via : Initial Calibration

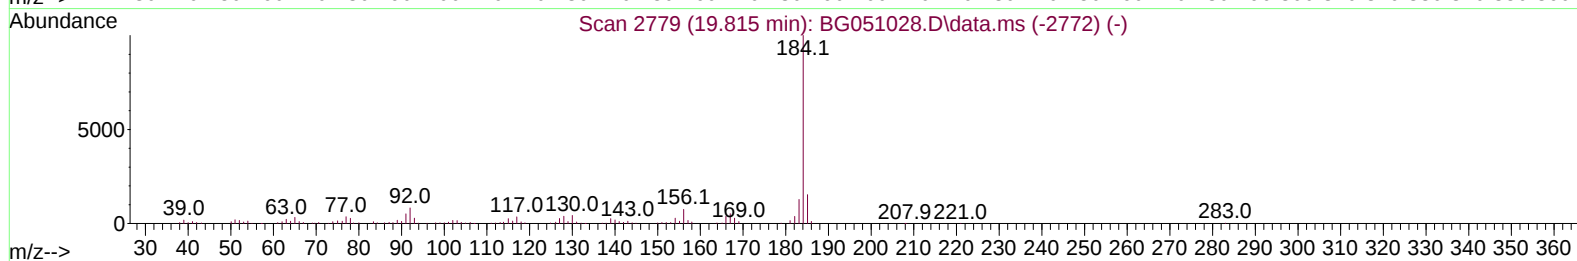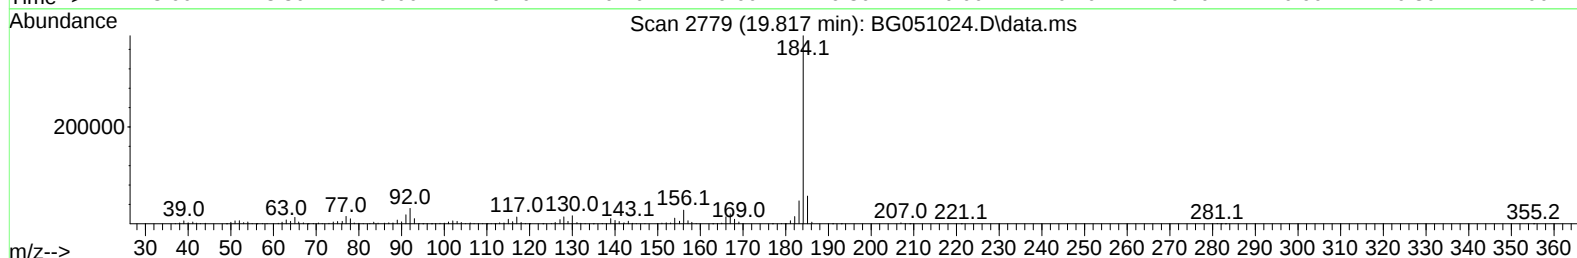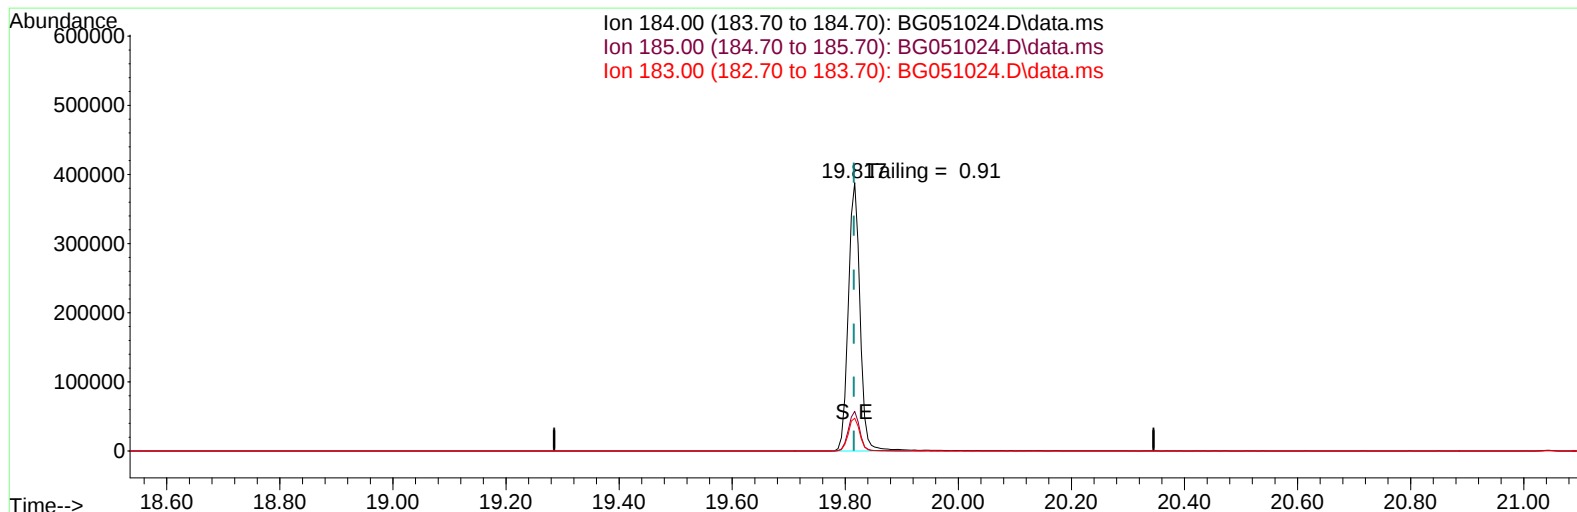

TIC: BG051024.D\data.ms

(77) Benzidine**19.817min (+ 0.002) 44884.62 ng****response 559109**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.40	14.77
183.00	11.70	12.25
0.00	0.00	0.00