
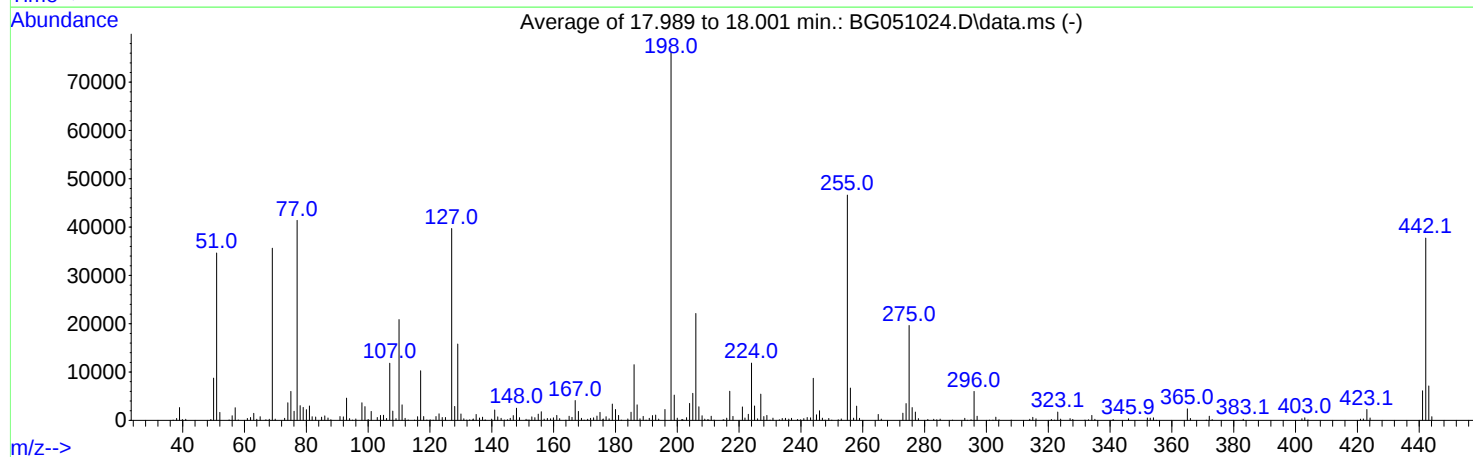


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111321\
 Data File : BG051024.D
 Acq On : 13 Nov 2021 15:21
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111321.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Nov 15 03:55:35 2021

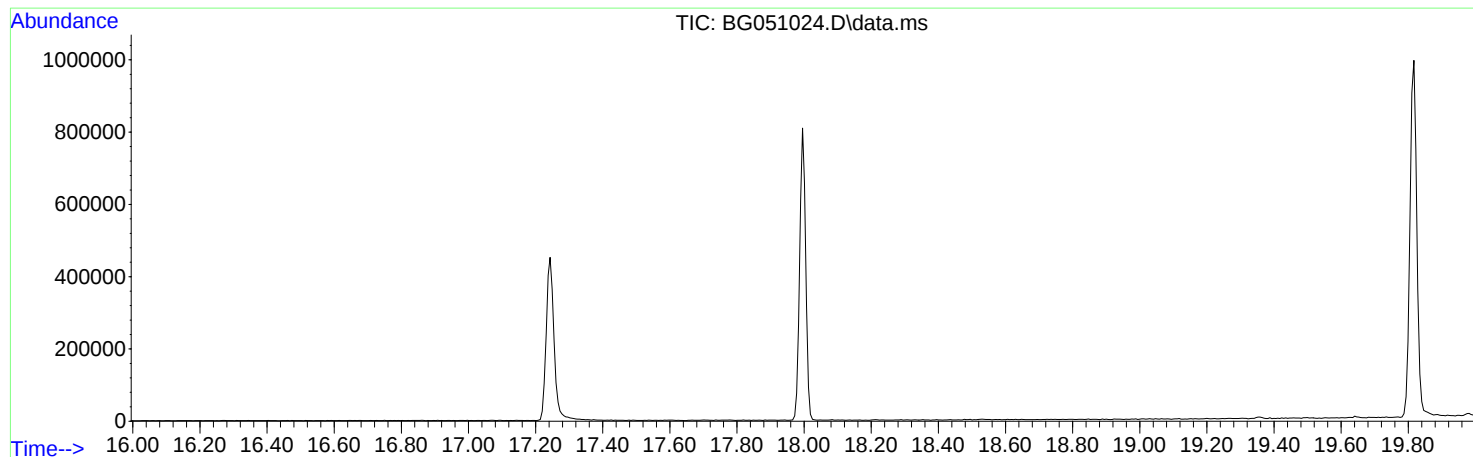




AutoFind: Scans 2468, 2469, 2470; Background Corrected with Scan 2461

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	45.5	34643	PASS
68	69	0.00	2	0.6	229	PASS
69	198	0.00	100	46.8	35627	PASS
70	69	0.00	2	0.7	254	PASS
127	198	10	80	52.2	39712	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	76139	PASS
199	198	5	9	6.9	5231	PASS
275	198	10	60	25.8	19655	PASS
365	198	1	100	3.1	2391	PASS
441	198	0.01	100	8.0	6123	PASS
442	442	50	100	100.0	37733	PASS
443	442	15	24	18.9	7138	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111321\
Data File : BG051024.D
Acq On : 13 Nov 2021 15:21
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Nov 15 08:12:04 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 15 03:55:35 2021
Response via : Initial Calibration

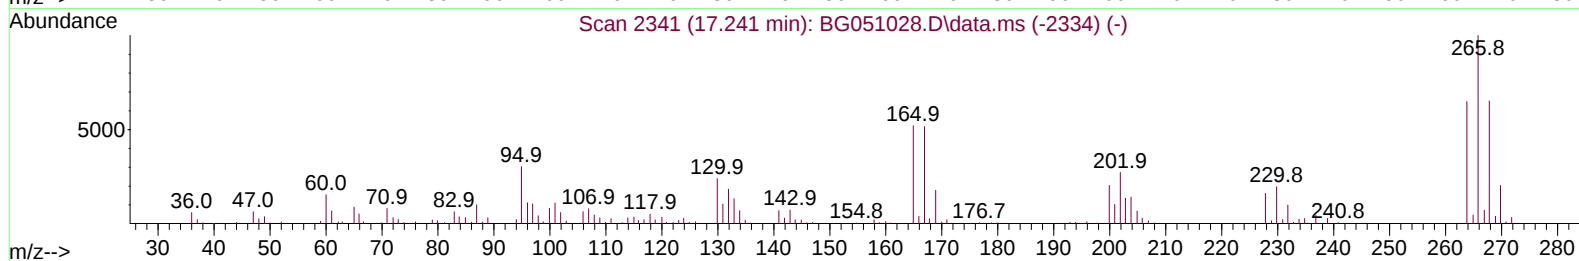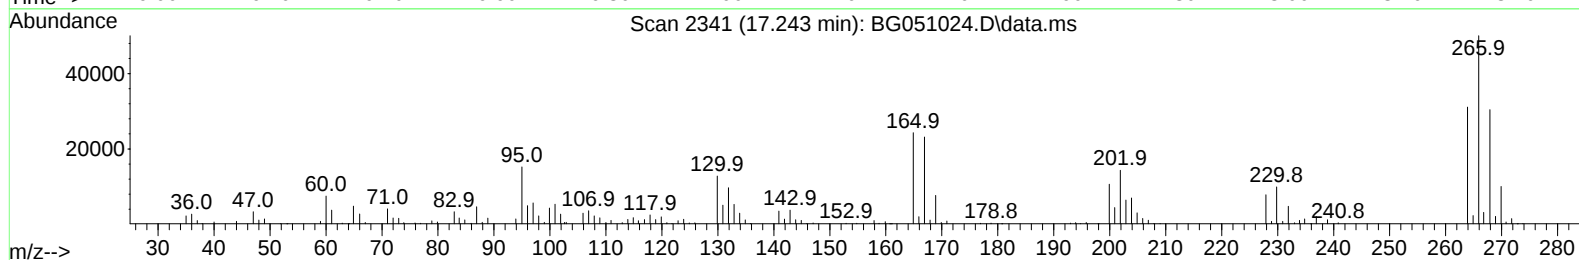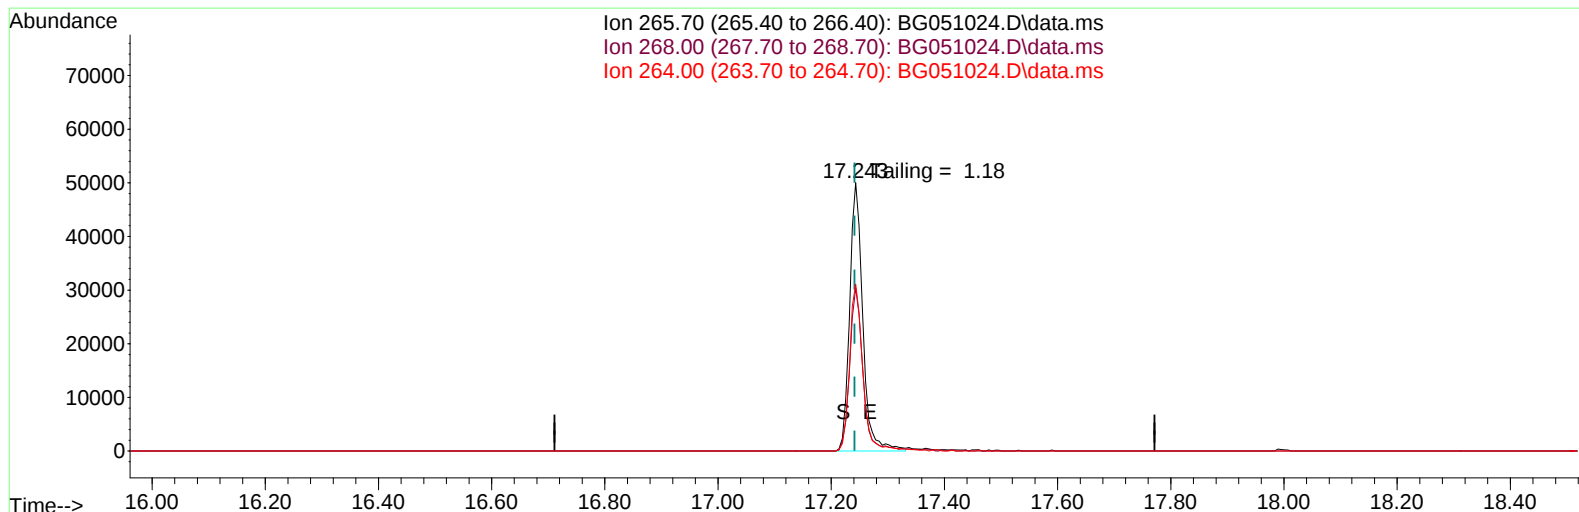

TIC: BG051024.D\data.ms

(70) Pentachlorophenol (C)

17.243min (+ 0.002) 29156.99 ng




response 81547

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.20	60.78
264.00	61.30	62.16
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111321\
Data File : BG051024.D
Acq On : 13 Nov 2021 15:21
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Nov 15 08:12:04 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 15 03:55:35 2021
Response via : Initial Calibration

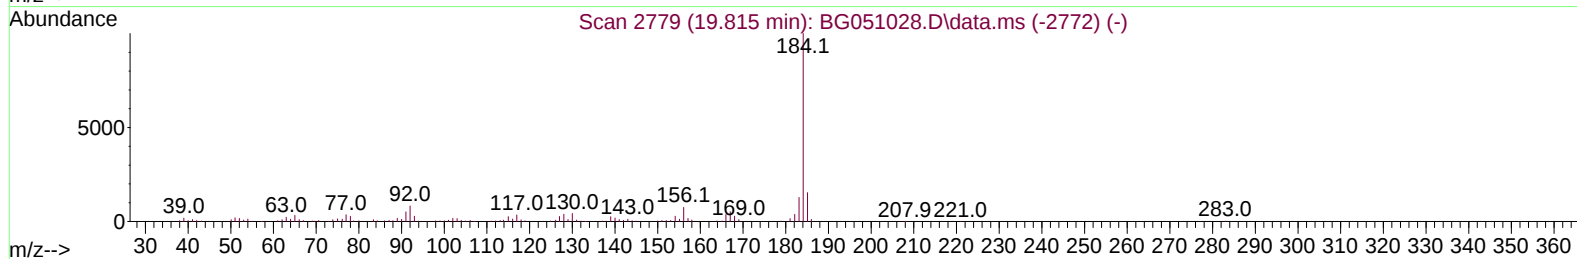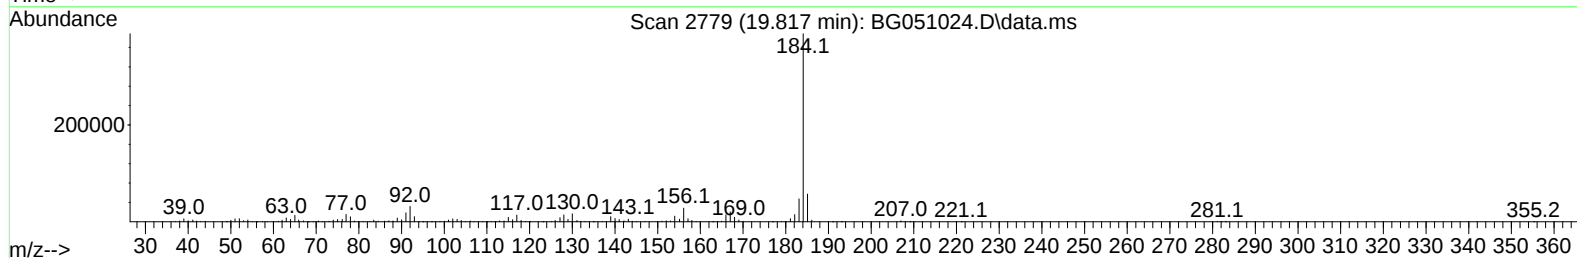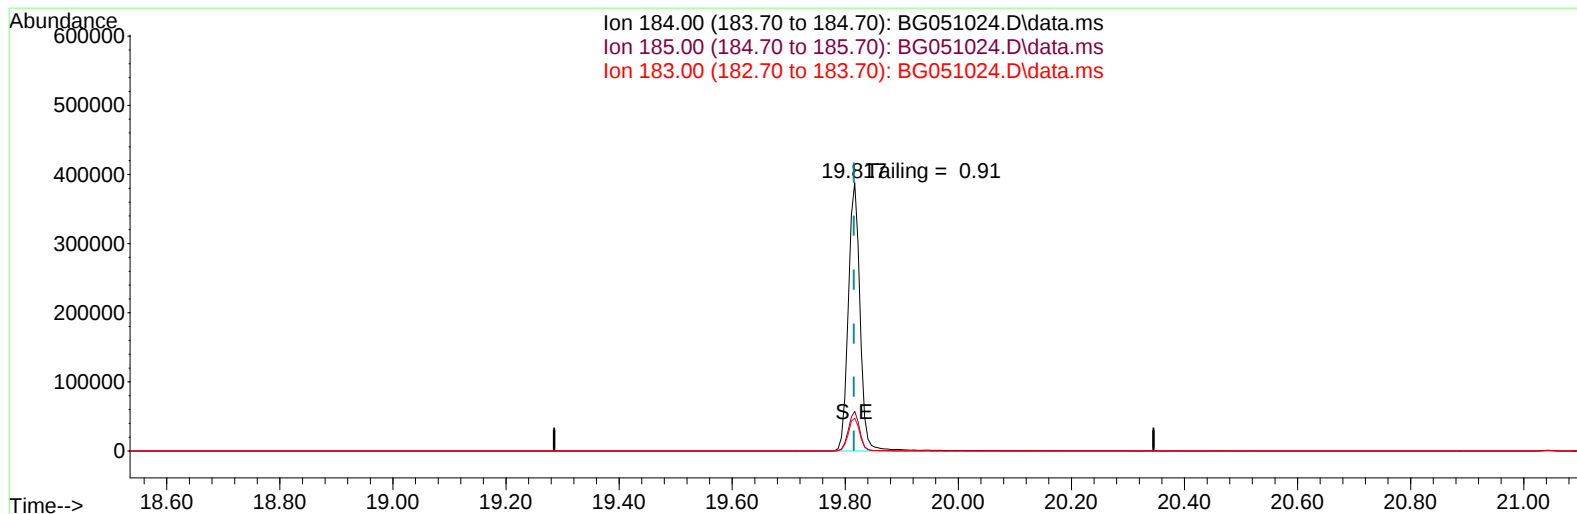

TIC: BG051024.D\data.ms

(77) Benzidine

19.817min (+ 0.002) 44884.62 ng

response 559109

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.40	14.77
183.00	11.70	12.25
0.00	0.00	0.00

Instrument :
BNA_G
ClientSampleId :
DFTPP

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/13/2021	BNA_G	BG051024.D
Compound Name	Response	Retention Time
DDT	254847	21.045
DDD	3077	20.645
DDE	0	20.075
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
3077	257924	1.19