
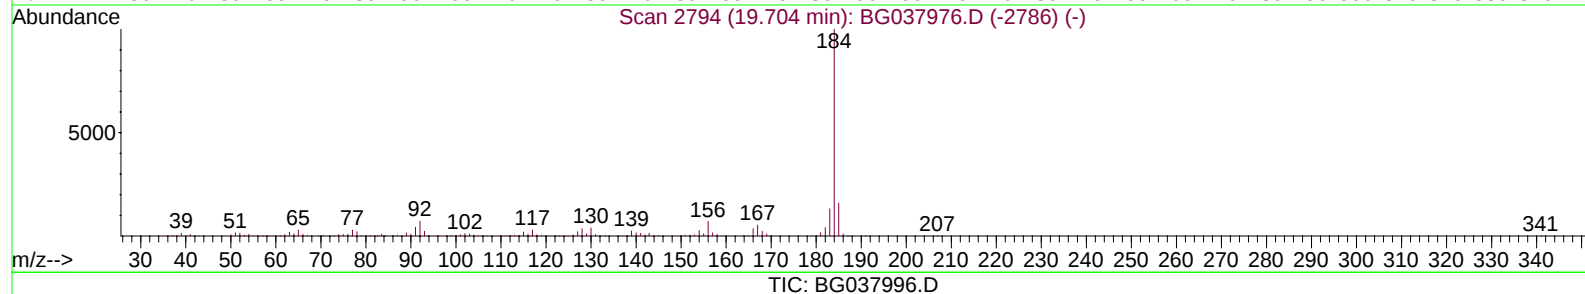
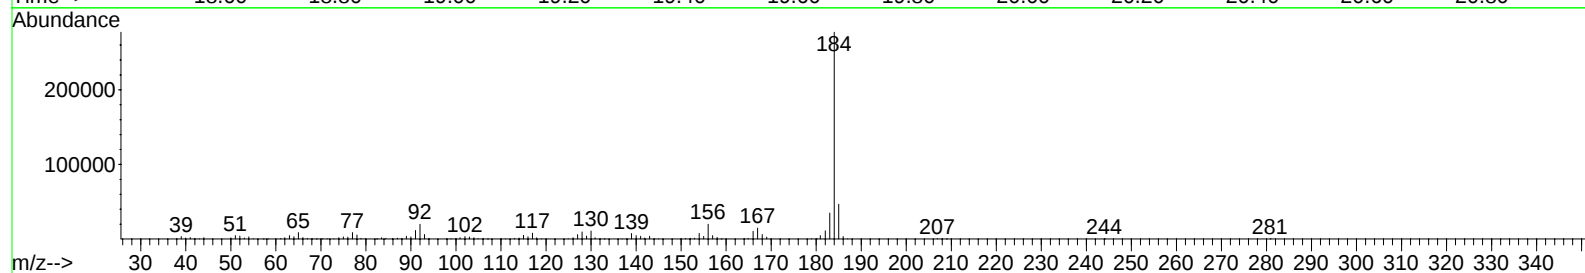


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG111418\
Data File : BG037996.D
Acq On : 14 Nov 2018 14:25
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 14 15:02:05 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG111318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 13 16:39:28 2018
Response via : Initial Calibration

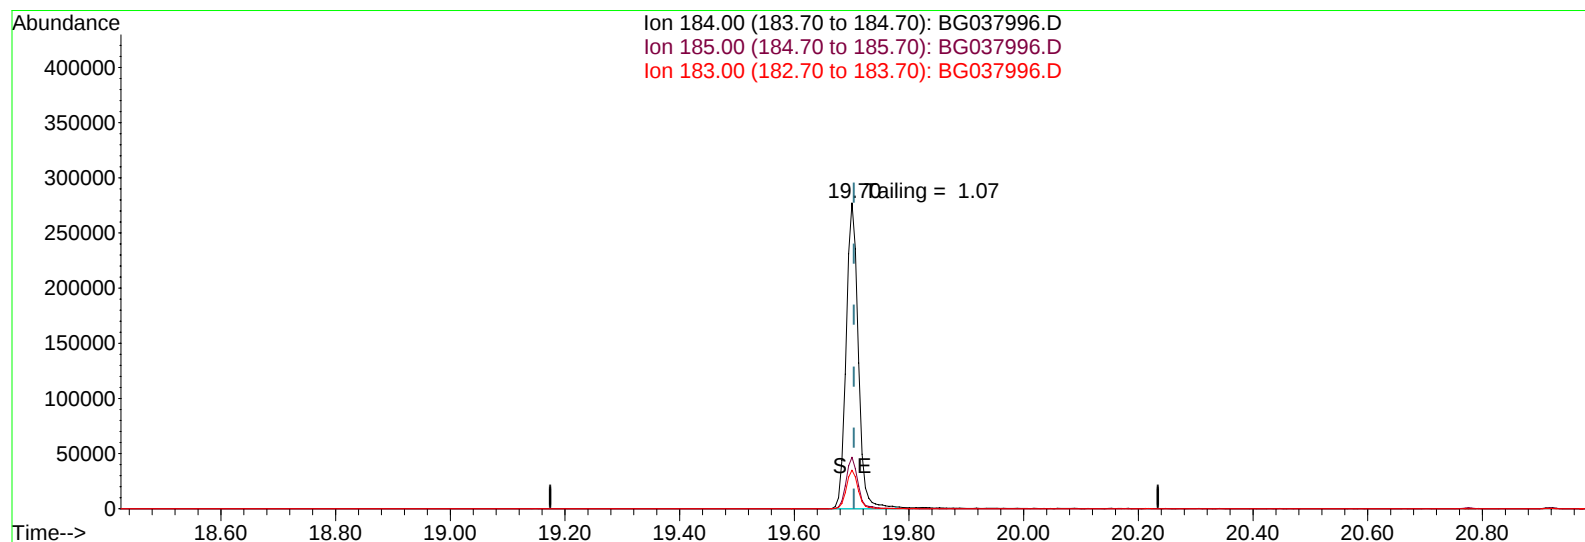

(77) Benzidine




19.701min (-0.004) 182798.80ng

response 410513

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	16.86
183.00	12.70	12.62
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG111418\
Data File : BG037996.D
Acq On : 14 Nov 2018 14:25
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 14 15:02:05 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG111318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 13 16:39:28 2018
Response via : Initial Calibration

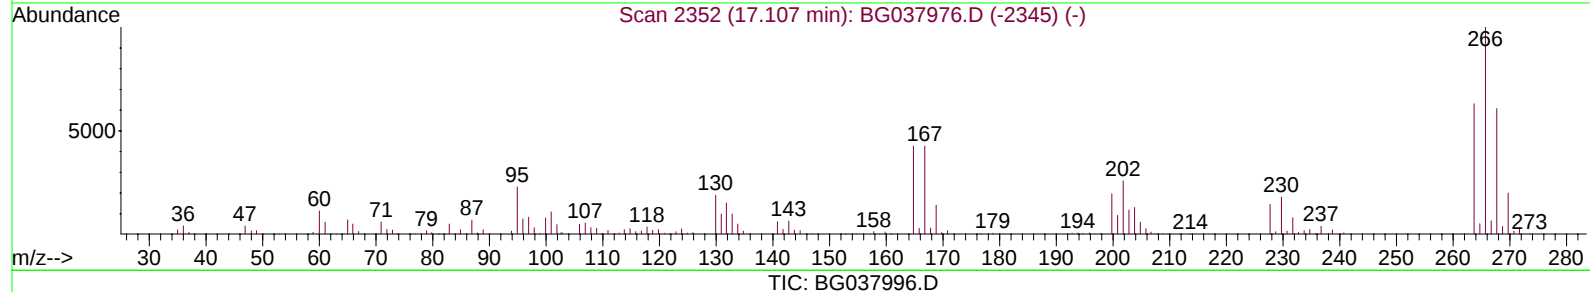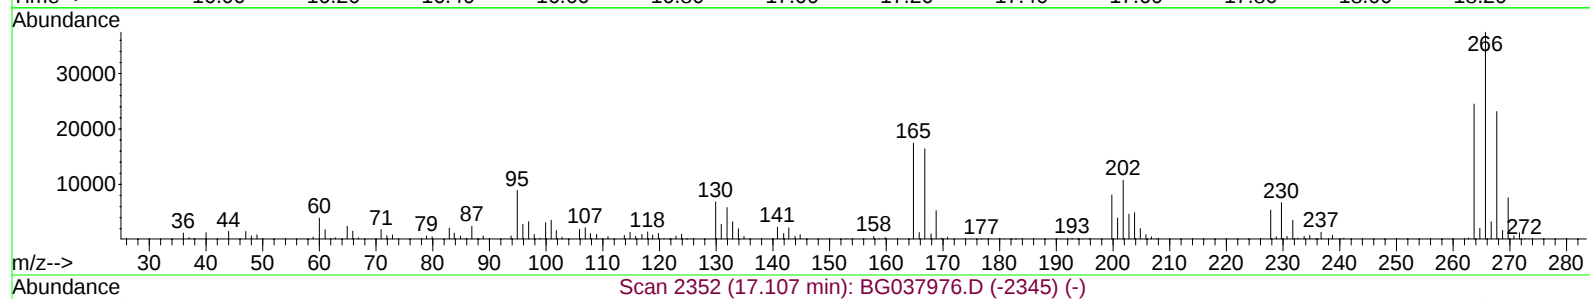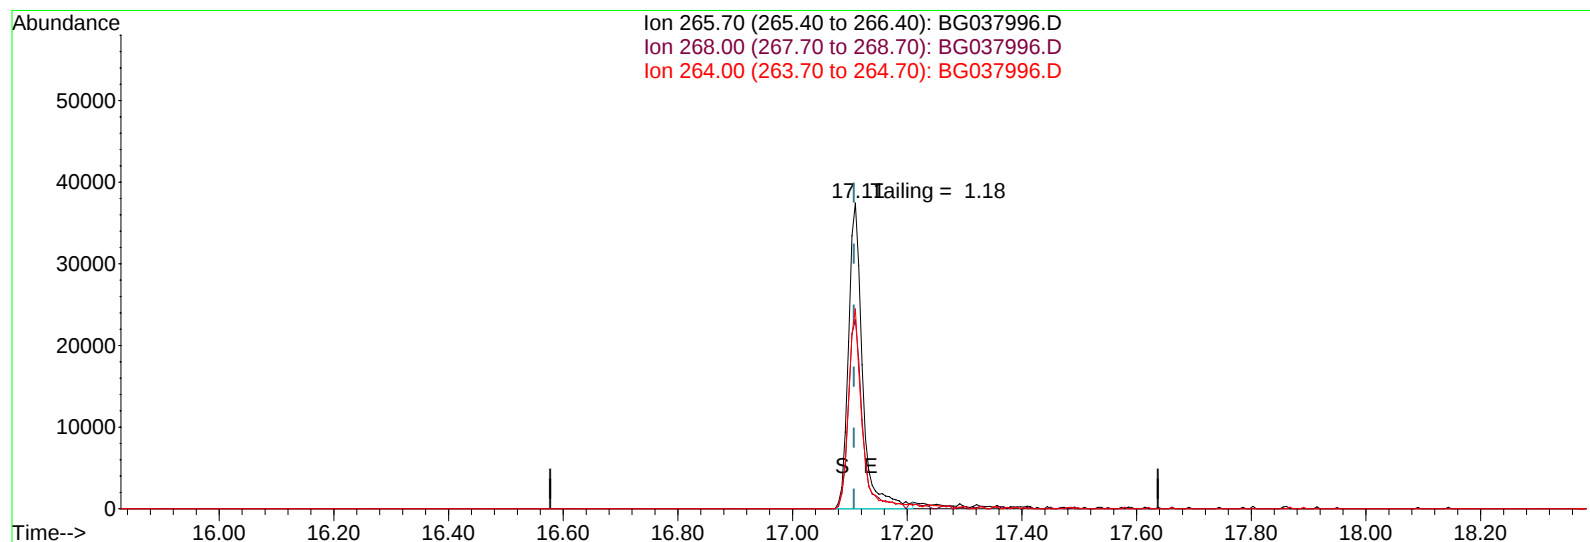

(70) Pentachlorophenol (C)

17.109min (+0.002) 28852.87ng

response 64160

Ion	Exp%	Act%
265.70	100	100
268.00	68.80	66.39
264.00	73.60	70.86
0.00	0.00	0.00